


Data Path : Z:\HPCHEM1\BNA G\Data\BG102017\
 Data File : BG029368.D
 Acq On : 20 Oct 2017 11:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 17:32:15 2017

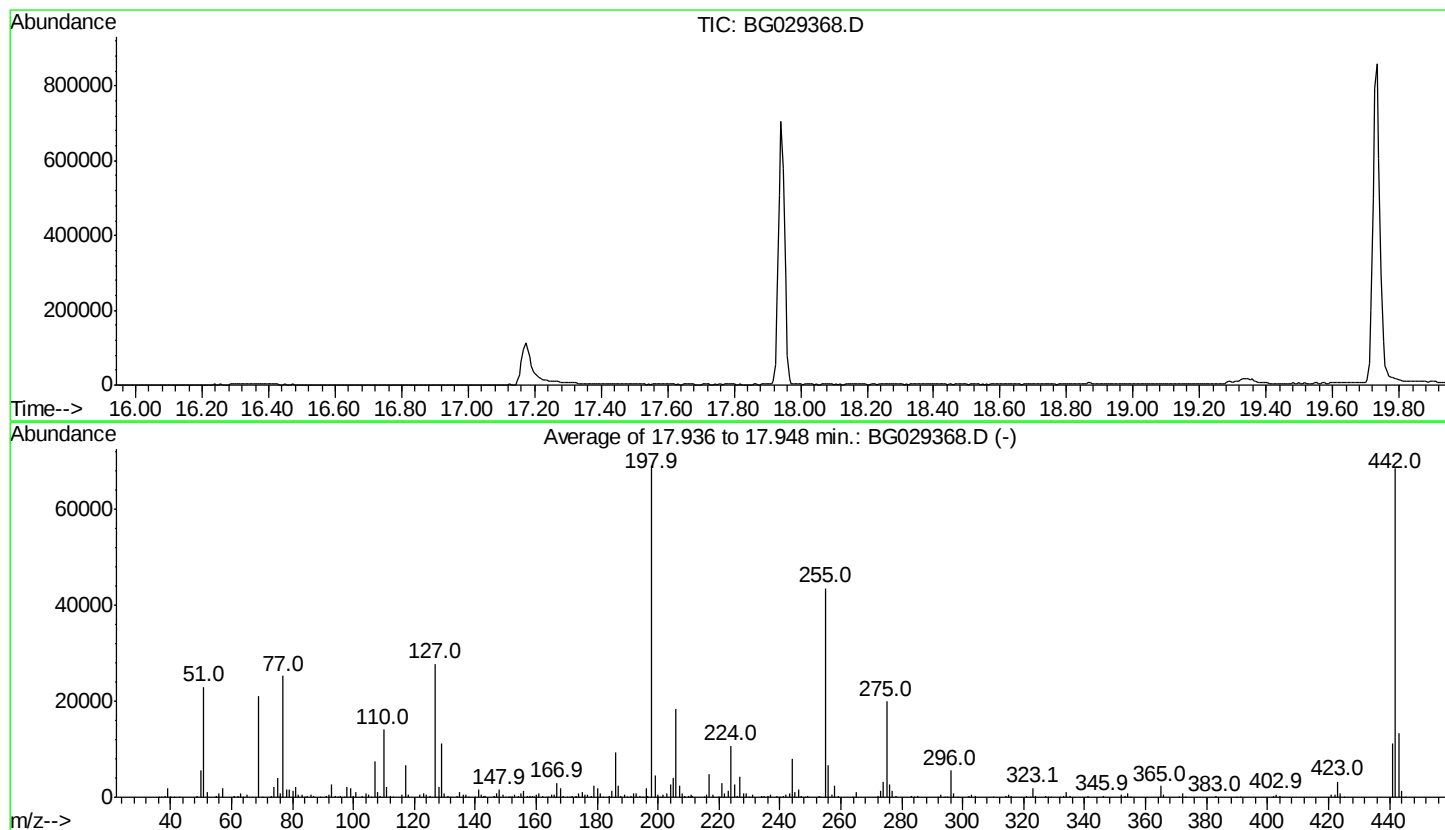

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	22992	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	30.6	21104	PASS
70	69	0.00	2	0.3	58	PASS
127	198	10	80	40.2	27738	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69034	PASS
199	198	5	9	6.8	4665	PASS
275	198	10	60	28.9	19920	PASS
365	198	1	100	3.4	2357	PASS
441	442	0.01	24	16.1	11071	PASS
442	198	50	100	99.4	68589	PASS
443	442	15	24	19.5	13403	PASS