


Data Path : Z:\HPCHEM1\BNA G\Data\BG102017\
 Data File : BG029385.D
 Acq On : 21 Oct 2017 9:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101617.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 16 17:32:15 2017

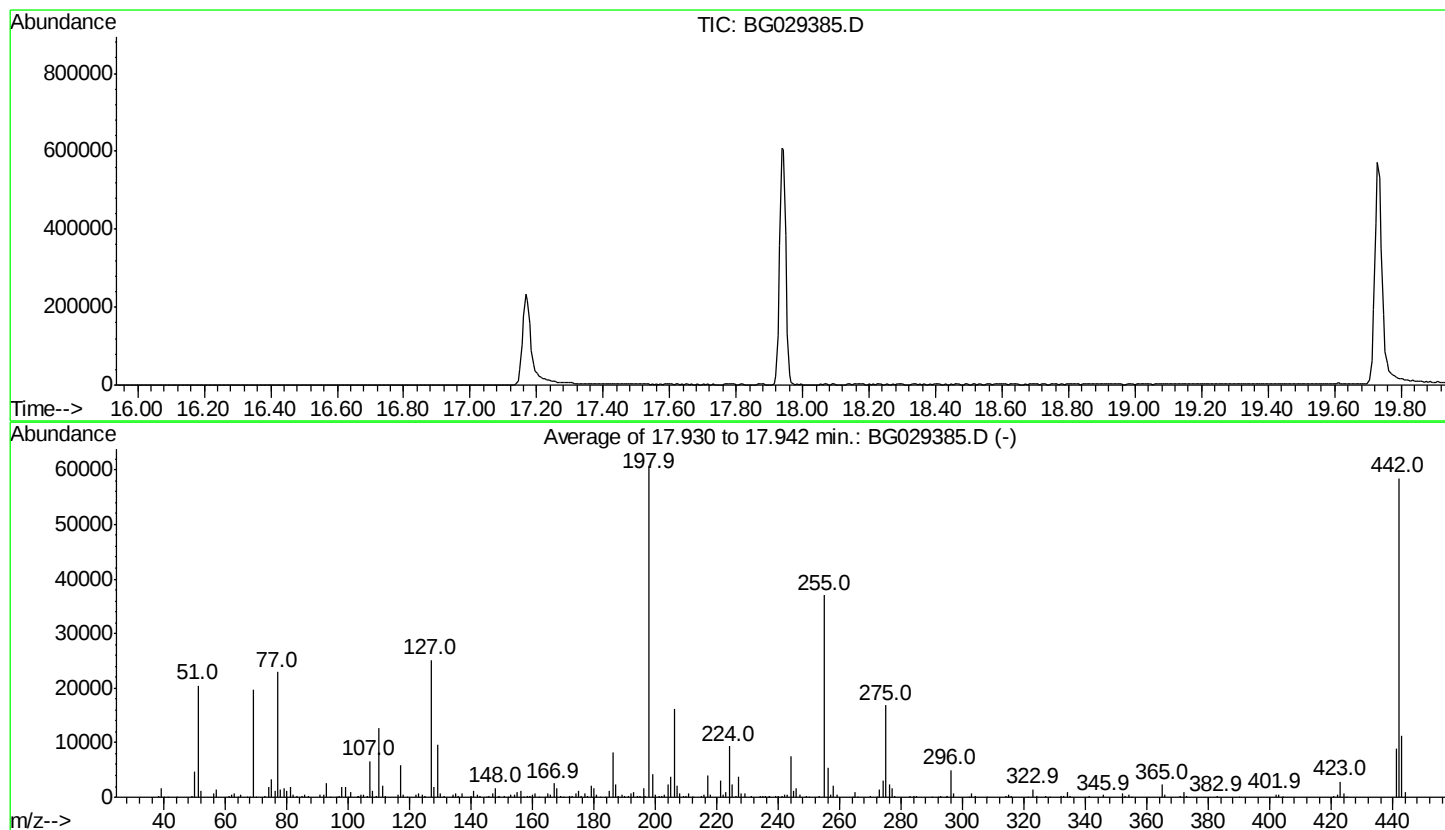

AutoFind: Scans 2492, 2493, 2494; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	20512	PASS
68	69	0.00	2	0.6	121	PASS
69	198	0.00	100	32.5	19723	PASS
70	69	0.00	2	0.5	106	PASS
127	198	10	80	41.3	25106	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	60773	PASS
199	198	5	9	7.1	4303	PASS
275	198	10	60	27.7	16804	PASS
365	198	1	100	3.7	2265	PASS
441	442	0.01	24	15.2	8883	PASS
442	198	50	100	96.3	58530	PASS
443	442	15	24	19.4	11368	PASS