
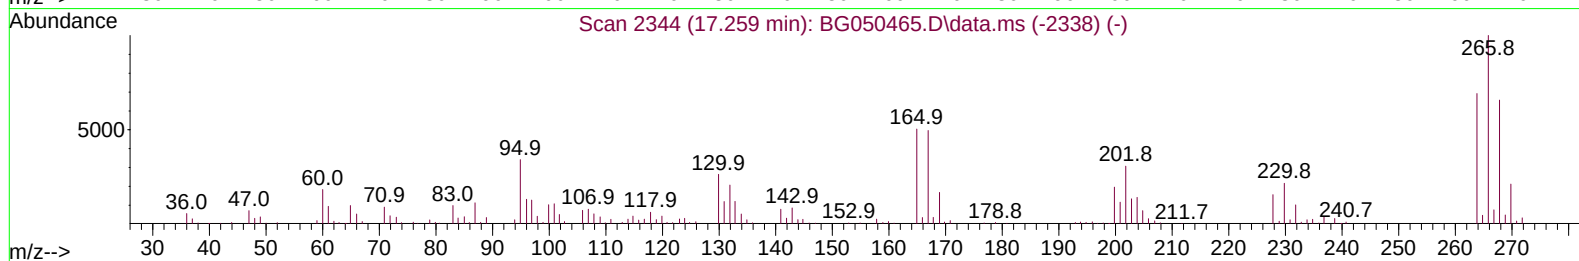
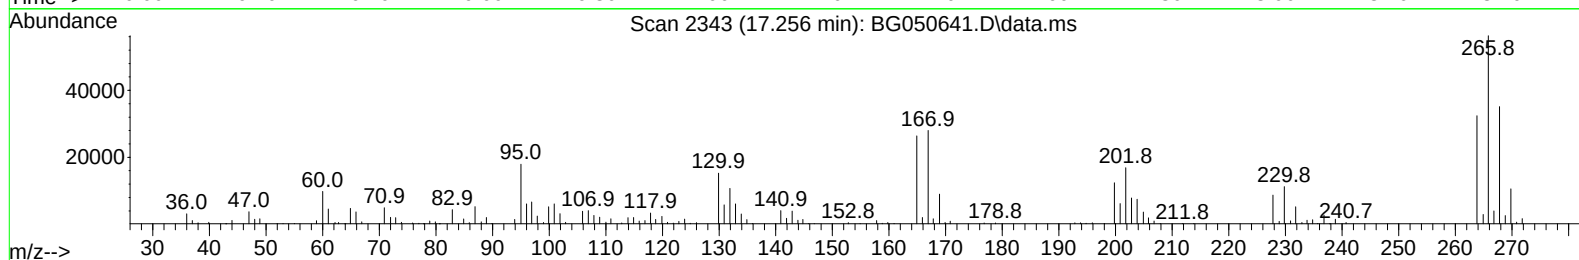


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102021\
Data File : BG050641.D
Acq On : 20 Oct 2021 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 13:51:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

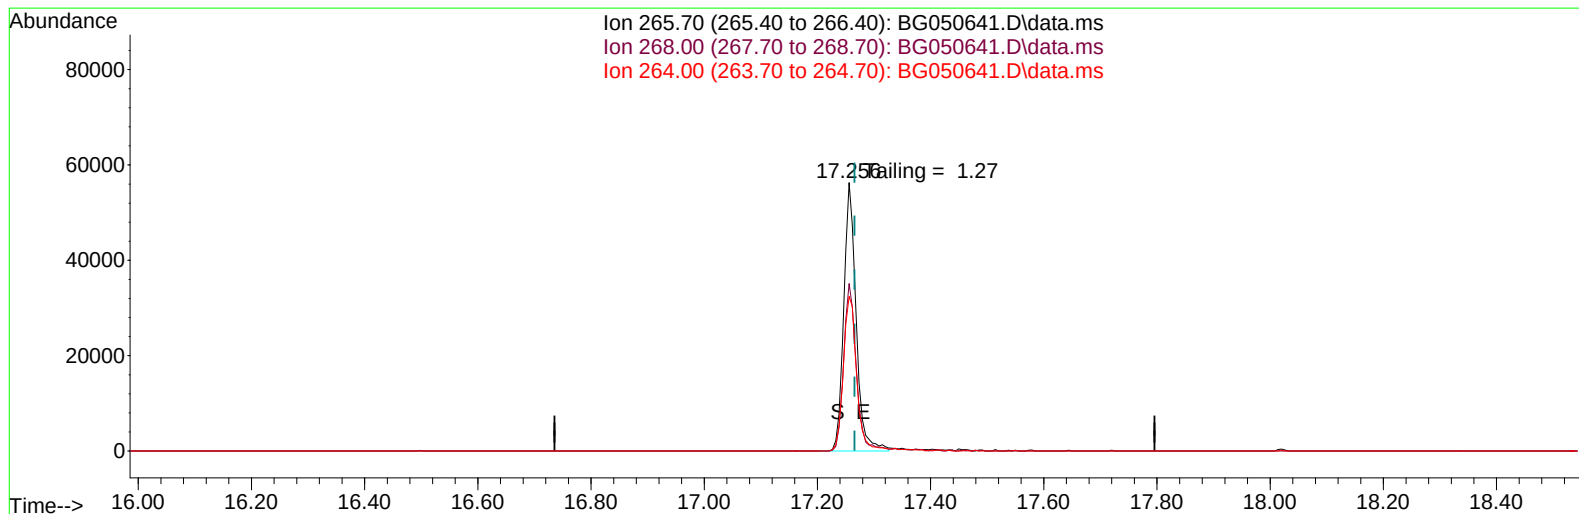

TIC: BG050641.D\data.ms

(70) Pentachlorophenol (C)




17.256min (-0.009) 20148.61 ng

response 86543

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.38
264.00	61.30	57.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102021\
Data File : BG050641.D
Acq On : 20 Oct 2021 11:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 20 13:51:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

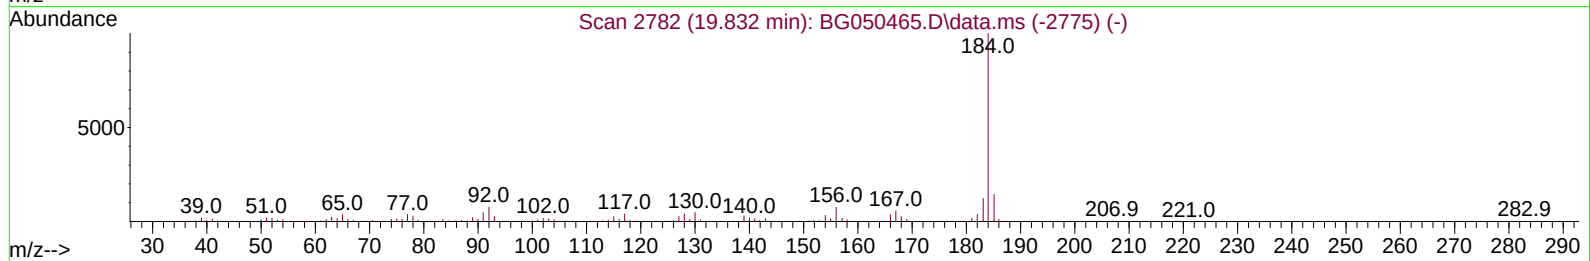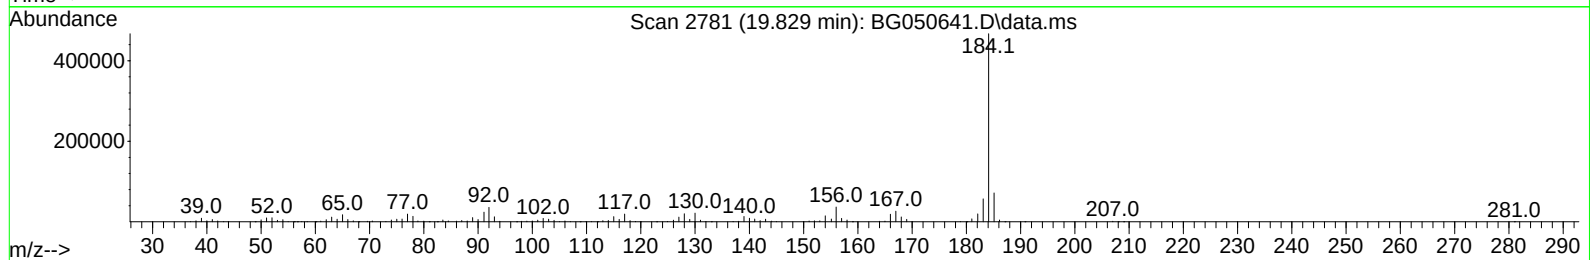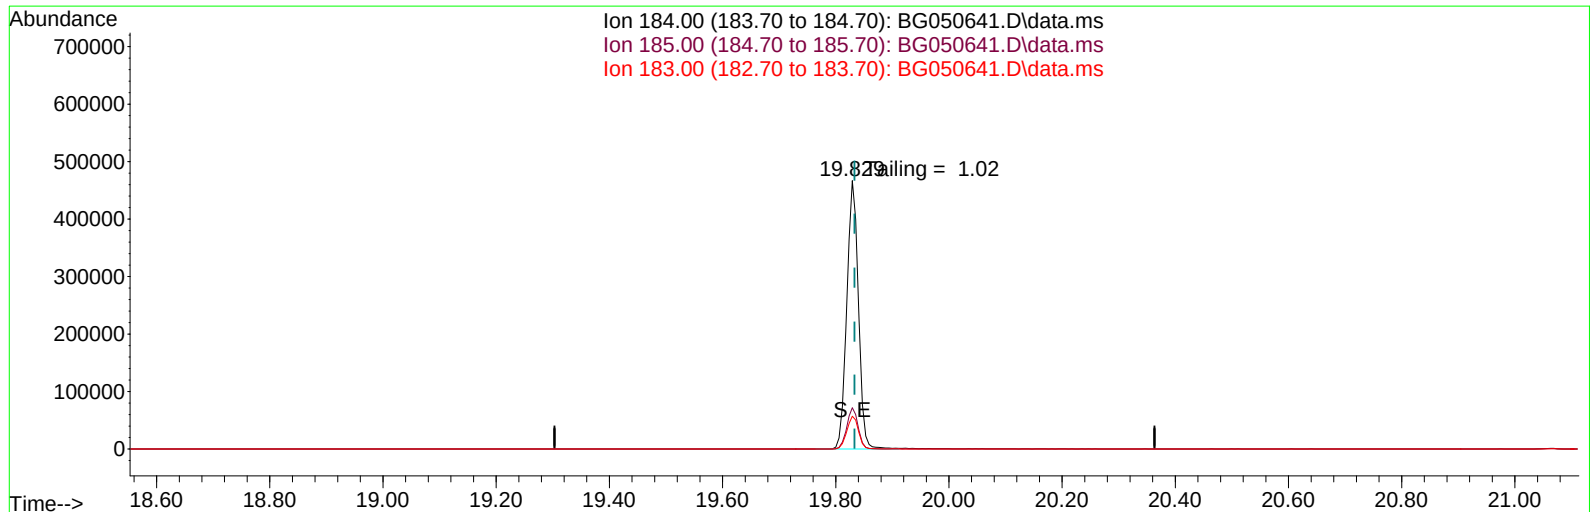

TIC: BG050641.D\data.ms

(77) Benzidine

19.829min (-0.004) 52833.05 ng

response 664404

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.38
183.00	11.70	12.25
0.00	0.00	0.00