

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102115\
 Data File : BG019279.D
 Acq On : 21 Oct 2015 13:36
 Operator : UM/NP
 Sample : G4074-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H3

Quant Time: Oct 21 14:16:19 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 12:55:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	19748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	92065	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	71694	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	166746	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	182723	20.00	ng/ul	0.00
86) Perylene-d12	24.82	264	187516	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	715	2.02	ng/uL	0.00
5) Phenol-d5	7.16	99	26804	15.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	16246	14.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	20891	16.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	20426	13.99	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	11245	15.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	13632	18.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	26292	17.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	9379	4.88	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	102998	16.43	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	113736	16.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	16305	14.46	ng/ul	0.00
58) Fluorene-d10	15.61	176	91651	17.10	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	18354	17.84	ng/ul	0.00
71) Anthracene-d10	17.47	188	143120	18.17	ng/ul	0.00
79) Pyrene-d10	19.75	212	155853	18.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.60	264	169246	17.87	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.07	163	45770	7.25	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102115\
Data File : BG019279.D
Acq On : 21 Oct 2015 13:36
Operator : UM/NP
Sample : G4074-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H3

Quant Time: Oct 21 14:16:19 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 12:55:56 2015
Response via : Initial Calibration

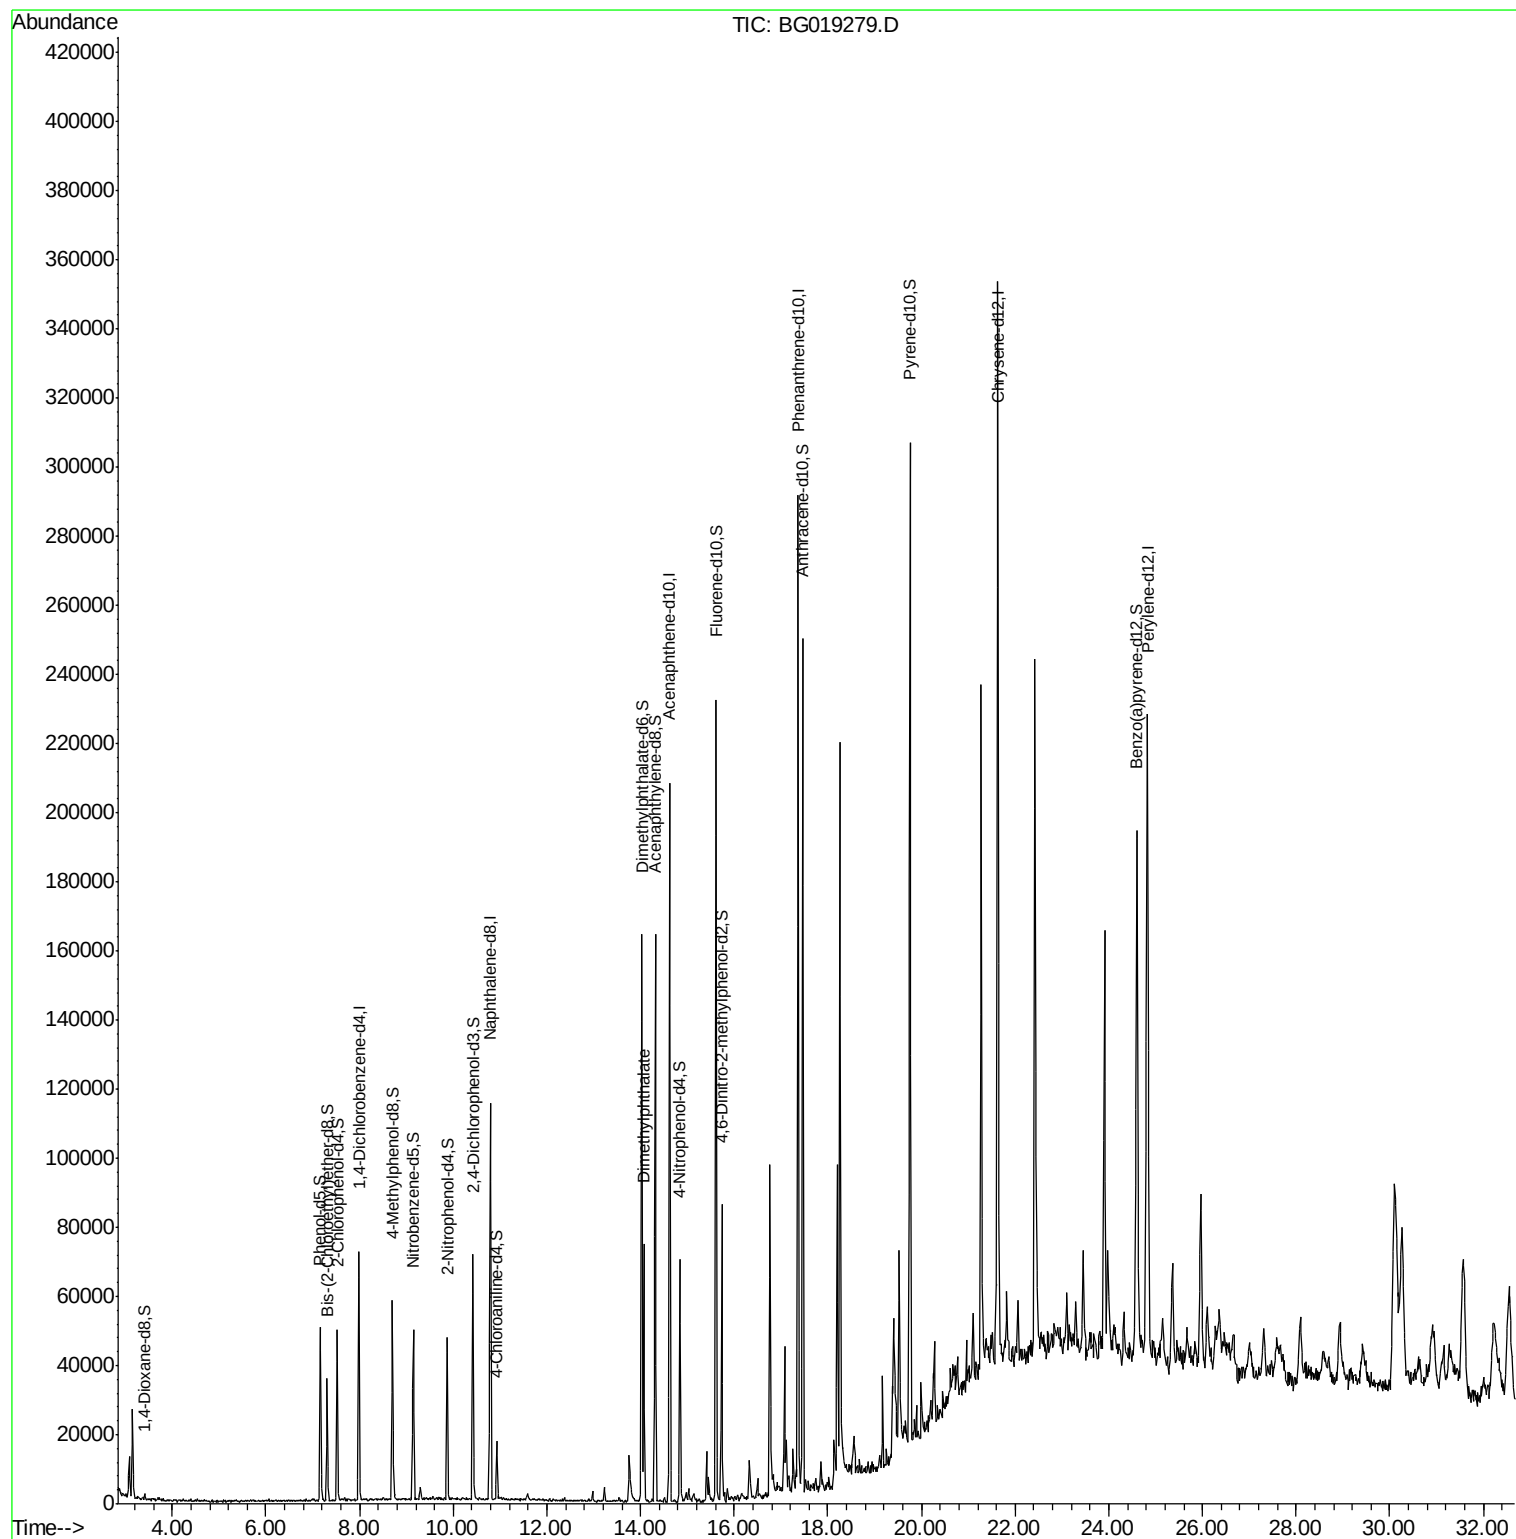

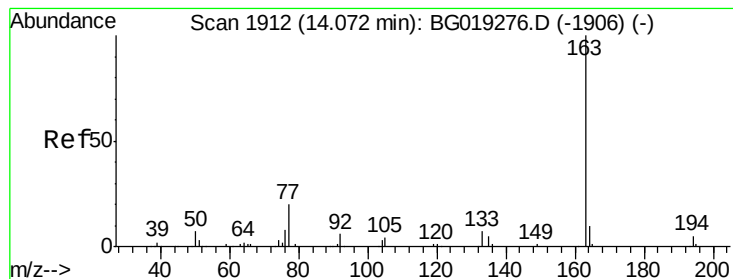

#45

Dimethylphthalate

Concen: 7.25 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BG019279.D

Acq: 21 Oct 2015 13:36

Instrument :

BNA_G

ClientSampleId :

JG9H3


Tgt Ion:163 Resp: 45770

Ion Ratio Lower Upper

163 100

194 3.3 3.3 4.9

164 9.5 8.1 12.1

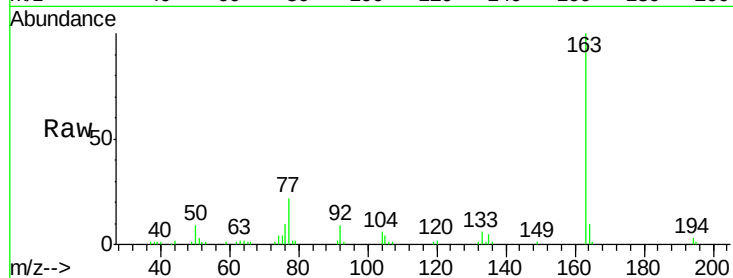

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

