

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102115\
 Data File : BG019282.D
 Acq On : 21 Oct 2015 15:30
 Operator : UM/NP
 Sample : G4074-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K4

Quant Time: Oct 21 16:06:40 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 12:55:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	24232	20.00	ng/ul	0.00
18) Naphthalene-d8	10.80	136	115494	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	80453	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	181426	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	205806	20.00	ng/ul	0.00
86) Perylene-d12	24.83	264	206777	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	606	1.39	ng/uL	0.00
5) Phenol-d5	7.17	99	24082	11.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	14214	10.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	18881	12.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	19748	11.02	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	9940	11.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	12071	12.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	23237	12.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	13811	5.73	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	85515	12.15	ng/ul	0.00
47) Acenaphthylene-d8	14.32	160	96893	12.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	11544	9.13	ng/ul	0.00
58) Fluorene-d10	15.61	176	75500	12.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	12401	11.08	ng/ul	0.00
71) Anthracene-d10	17.46	188	108992	12.72	ng/ul	0.00
79) Pyrene-d10	19.75	212	117346	12.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	128955	12.34	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.07	163	42882	6.05	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102115\
Data File : BG019282.D
Acq On : 21 Oct 2015 15:30
Operator : UM/NP
Sample : G4074-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K4

Quant Time: Oct 21 16:06:40 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 12:55:56 2015
Response via : Initial Calibration

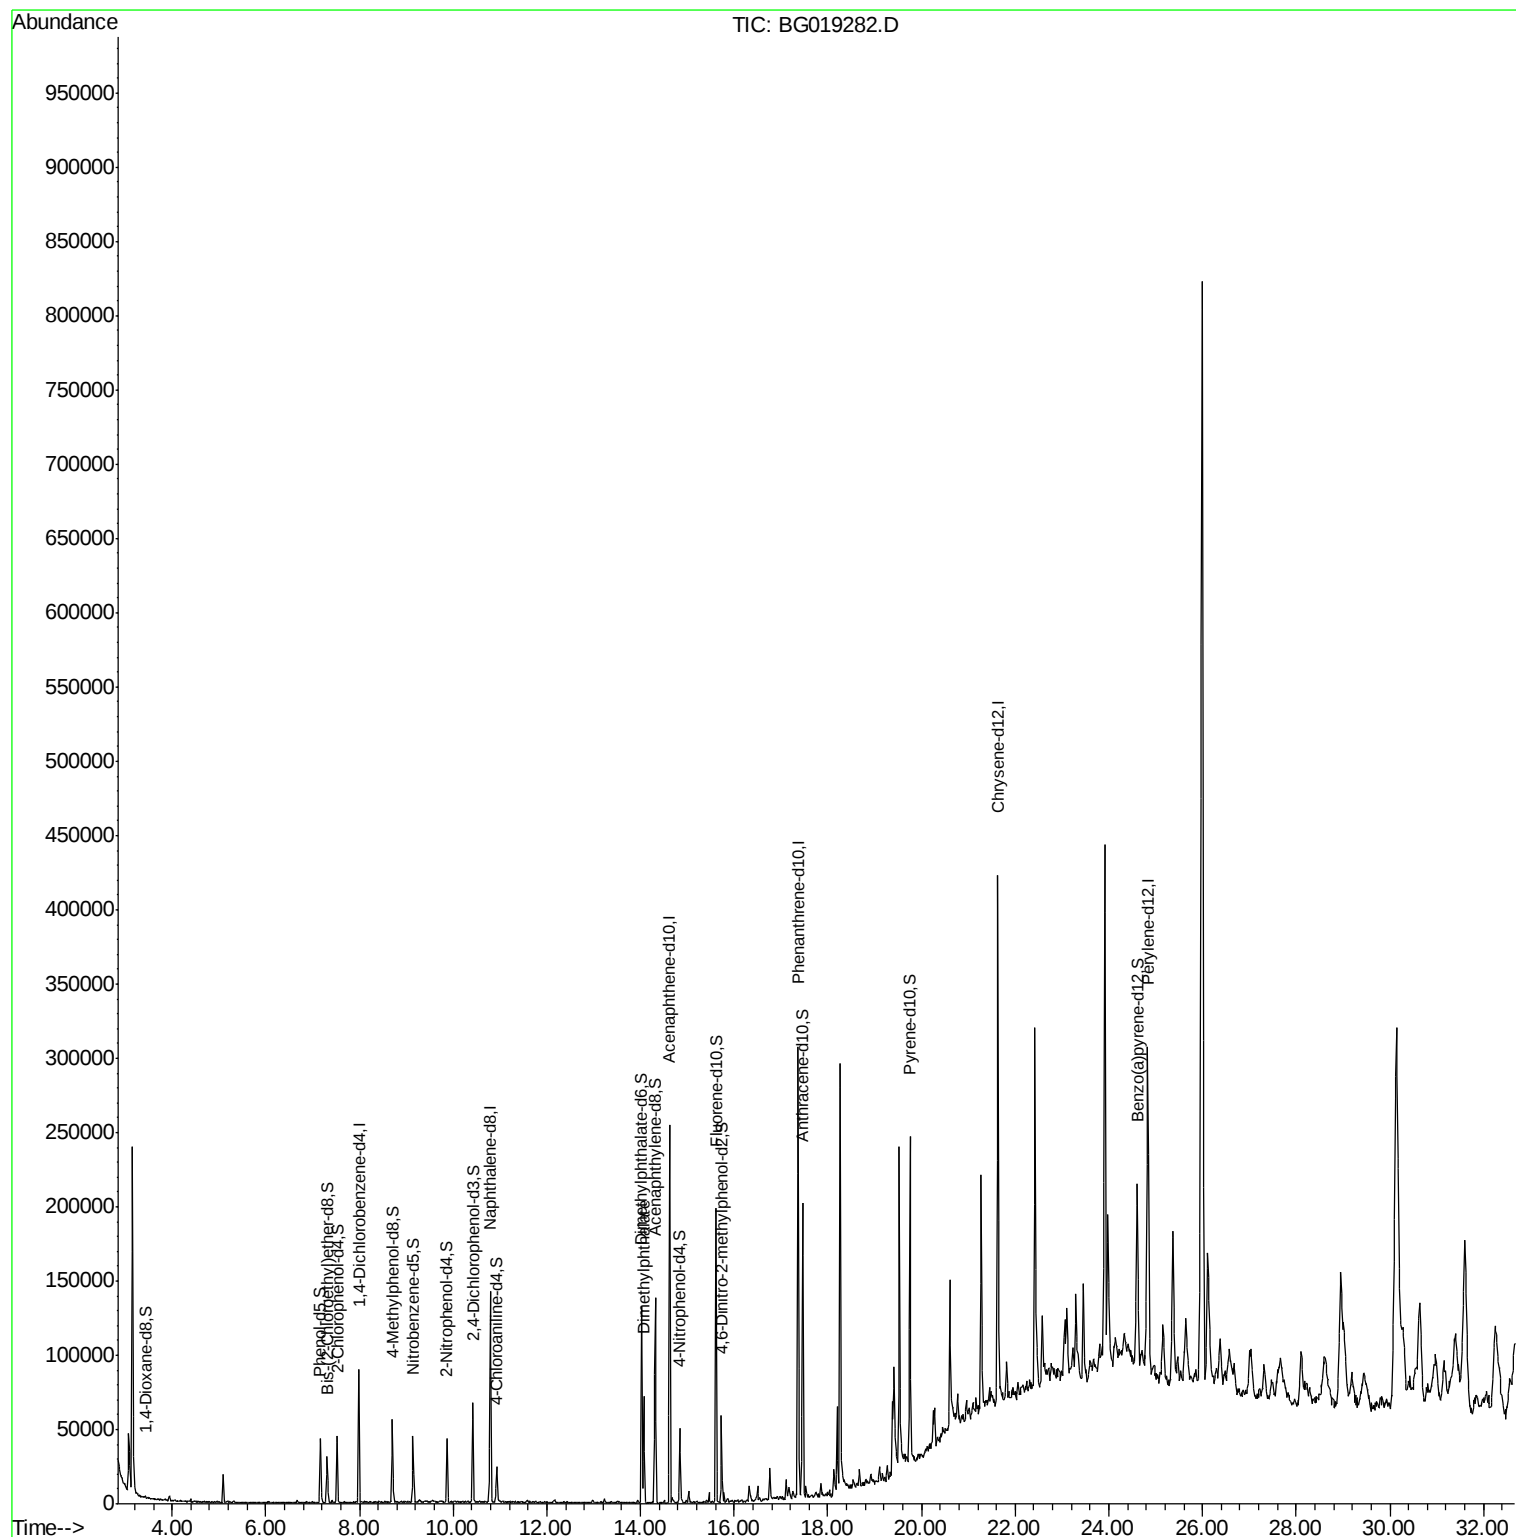

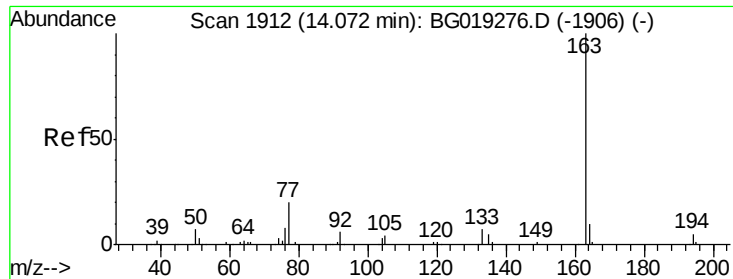

#45

Dimethylphthalate

Concen: 6.05 ng/ul

RT: 14.07 min Scan# 1911

Delta R.T. -0.00 min

Lab File: BG019282.D

Acq: 21 Oct 2015 15:30

Instrument :

BNA_G

ClientSampleId :

JG9K4


Tgt Ion:163 Resp: 42882

Ion Ratio Lower Upper

163 100

194 3.5 3.3 4.9

164 10.7 8.1 12.1

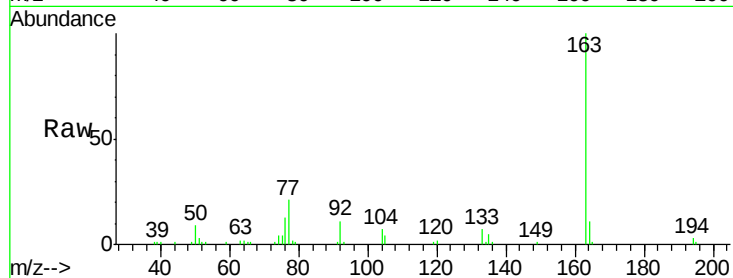

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

