

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
 Data File : BG019278.D
 Acq On : 21 Oct 2015 12:58
 Operator : UM/NP
 Sample : G4074-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H1

Quant Time: Oct 21 13:32:33 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 12:55:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	17230	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	77182	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	59626	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	146111	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	166095	20.00	ng/ul	0.00
86) Perylene-d12	24.82	264	171278	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	743	2.40	ng/uL	0.00
5) Phenol-d5	7.16	99	17396	11.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	11789	12.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	14394	13.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	13796	10.83	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	7401	12.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	8648	13.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	15551	12.44	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	6180	3.84	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	67603	12.96	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	71489	12.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	10251	10.93	ng/ul	0.00
58) Fluorene-d10	15.61	176	58526	13.13	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	11839	13.13	ng/ul	0.00
71) Anthracene-d10	17.46	188	91942	13.32	ng/ul	0.00
79) Pyrene-d10	19.75	212	103426	13.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.60	264	113701	13.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	25885	4.93	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
Data File : BG019278.D
Acq On : 21 Oct 2015 12:58
Operator : UM/NP
Sample : G4074-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H1

Quant Time: Oct 21 13:32:33 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 12:55:56 2015
Response via : Initial Calibration

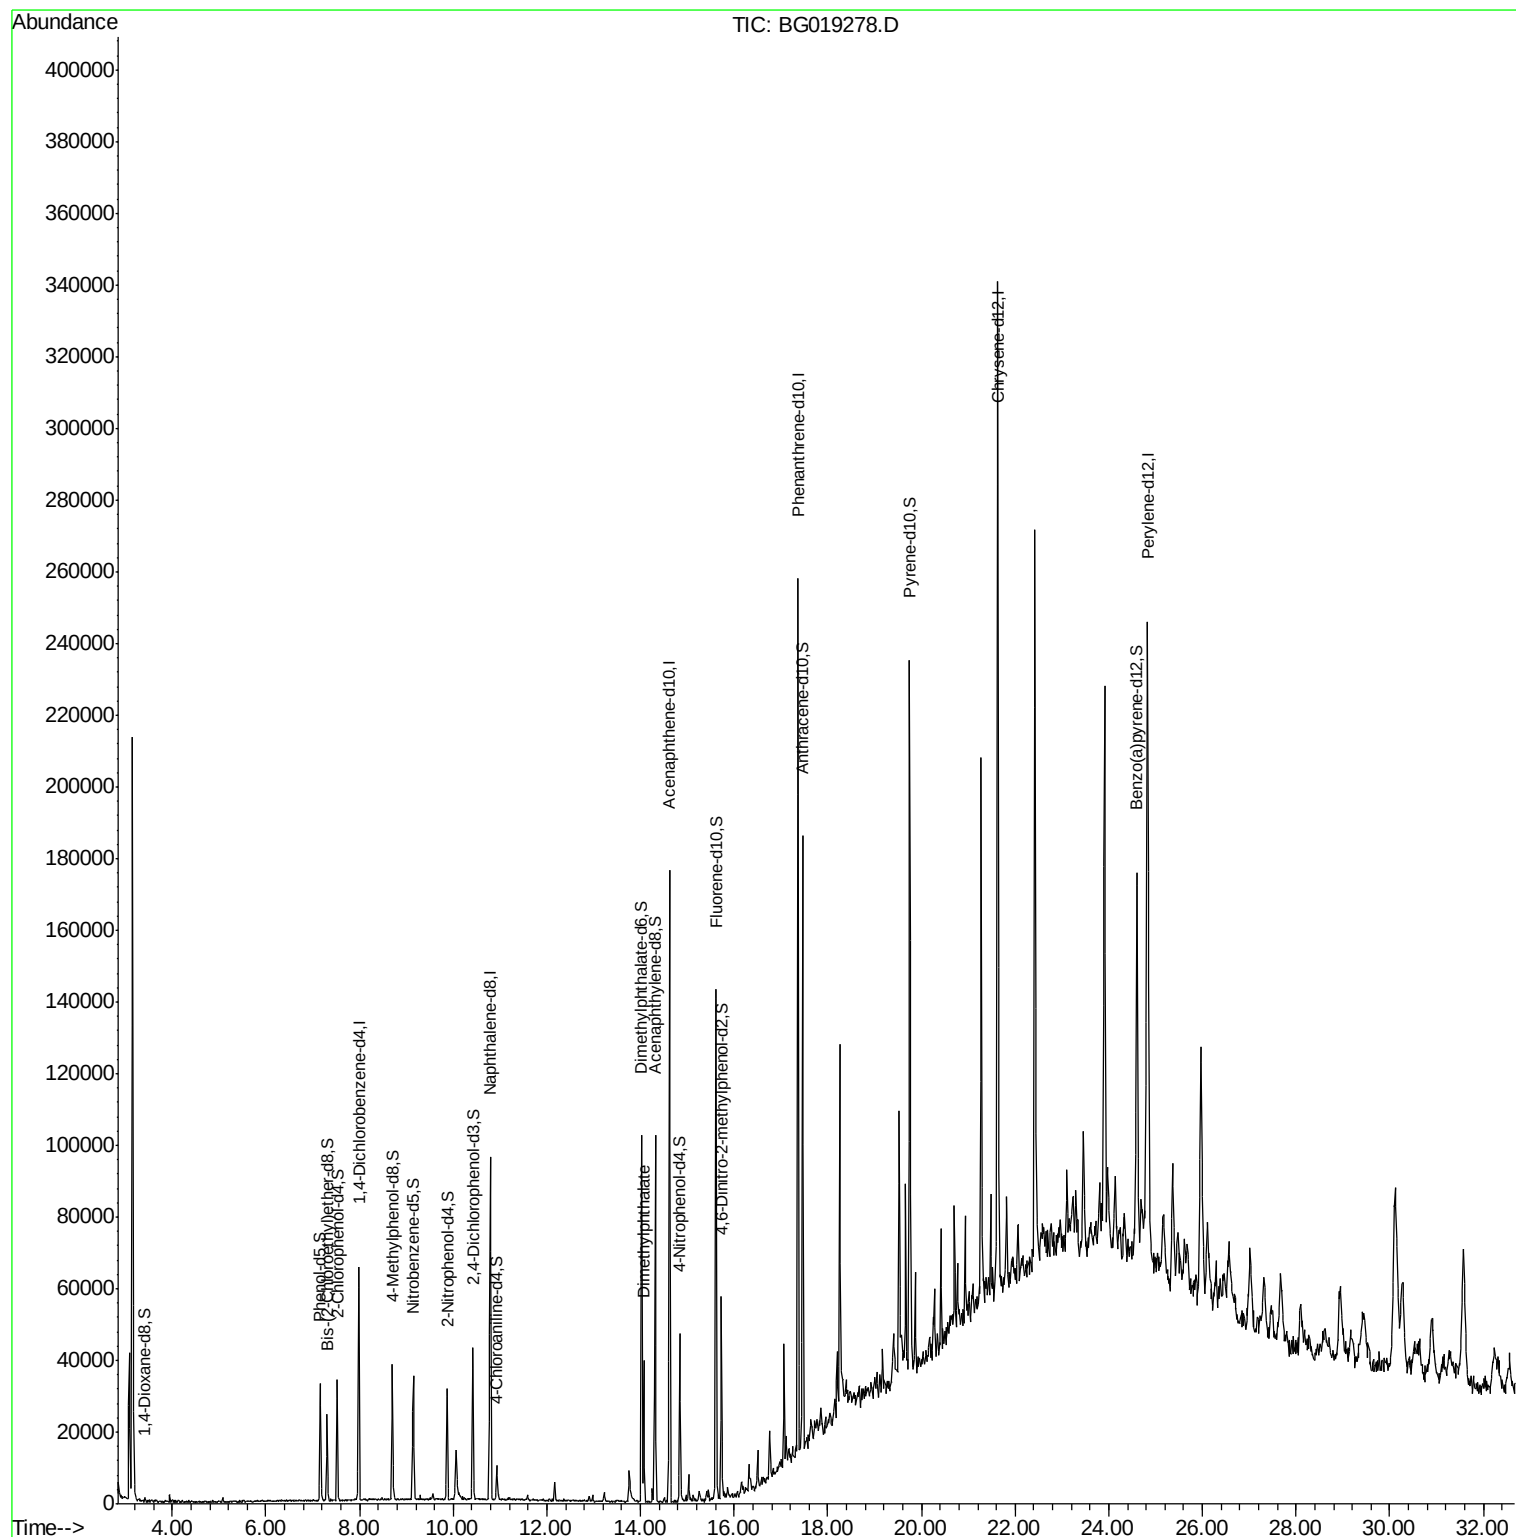

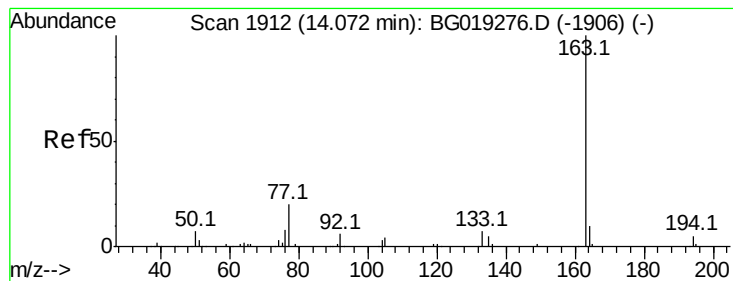

#45

Dimethylphthalate

Concen: 4.93 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. 0.00 min

Lab File: BG019278.D

Acq: 21 Oct 2015 12:58

Instrument :

BNA_G

ClientSampleId :

JG9H1


Tot Ion:163 Resp: 25885

Ion Ratio Lower Upper

163 100

194 3.4 3.3 4.9

164 9.4 8.1 12.1

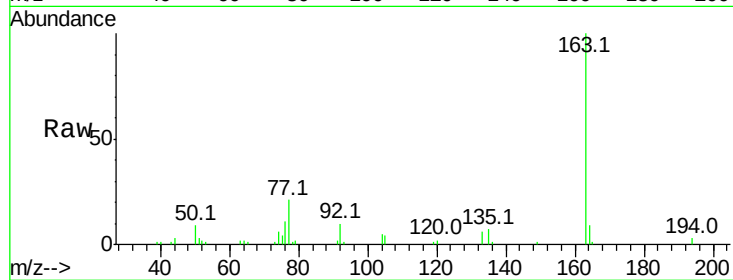

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

