

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
 Data File : BG019281.D
 Acq On : 21 Oct 2015 14:52
 Operator : UM/NP
 Sample : G4074-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K1

Quant Time: Oct 21 15:55:00 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 12:55:56 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	19158	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	90816	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	67266	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.37	188	151181	20.00	ng/ul	0.00
78) Chrysene-d12	21.63	240	168913	20.00	ng/ul	0.00
86) Perylene-d12	24.82	264	170239	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	966	2.81	ng/uL	0.00
5) Phenol-d5	7.16	99	33797	20.22	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	20108	18.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	26024	21.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	28690	20.25	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	13958	19.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	16442	22.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.42	165	31867	21.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	31560	16.66	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	113489	19.29	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	132421	20.82	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	17838	16.87	ng/ul	0.00
58) Fluorene-d10	15.61	176	100659	20.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	18324	19.65	ng/ul	0.00
71) Anthracene-d10	17.47	188	153973	21.56	ng/ul	0.00
79) Pyrene-d10	19.75	212	170805	22.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	185566	21.58	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	46354	7.82	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
Data File : BG019281.D
Acq On : 21 Oct 2015 14:52
Operator : UM/NP
Sample : G4074-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K1

Quant Time: Oct 21 15:55:00 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 12:55:56 2015
Response via : Initial Calibration

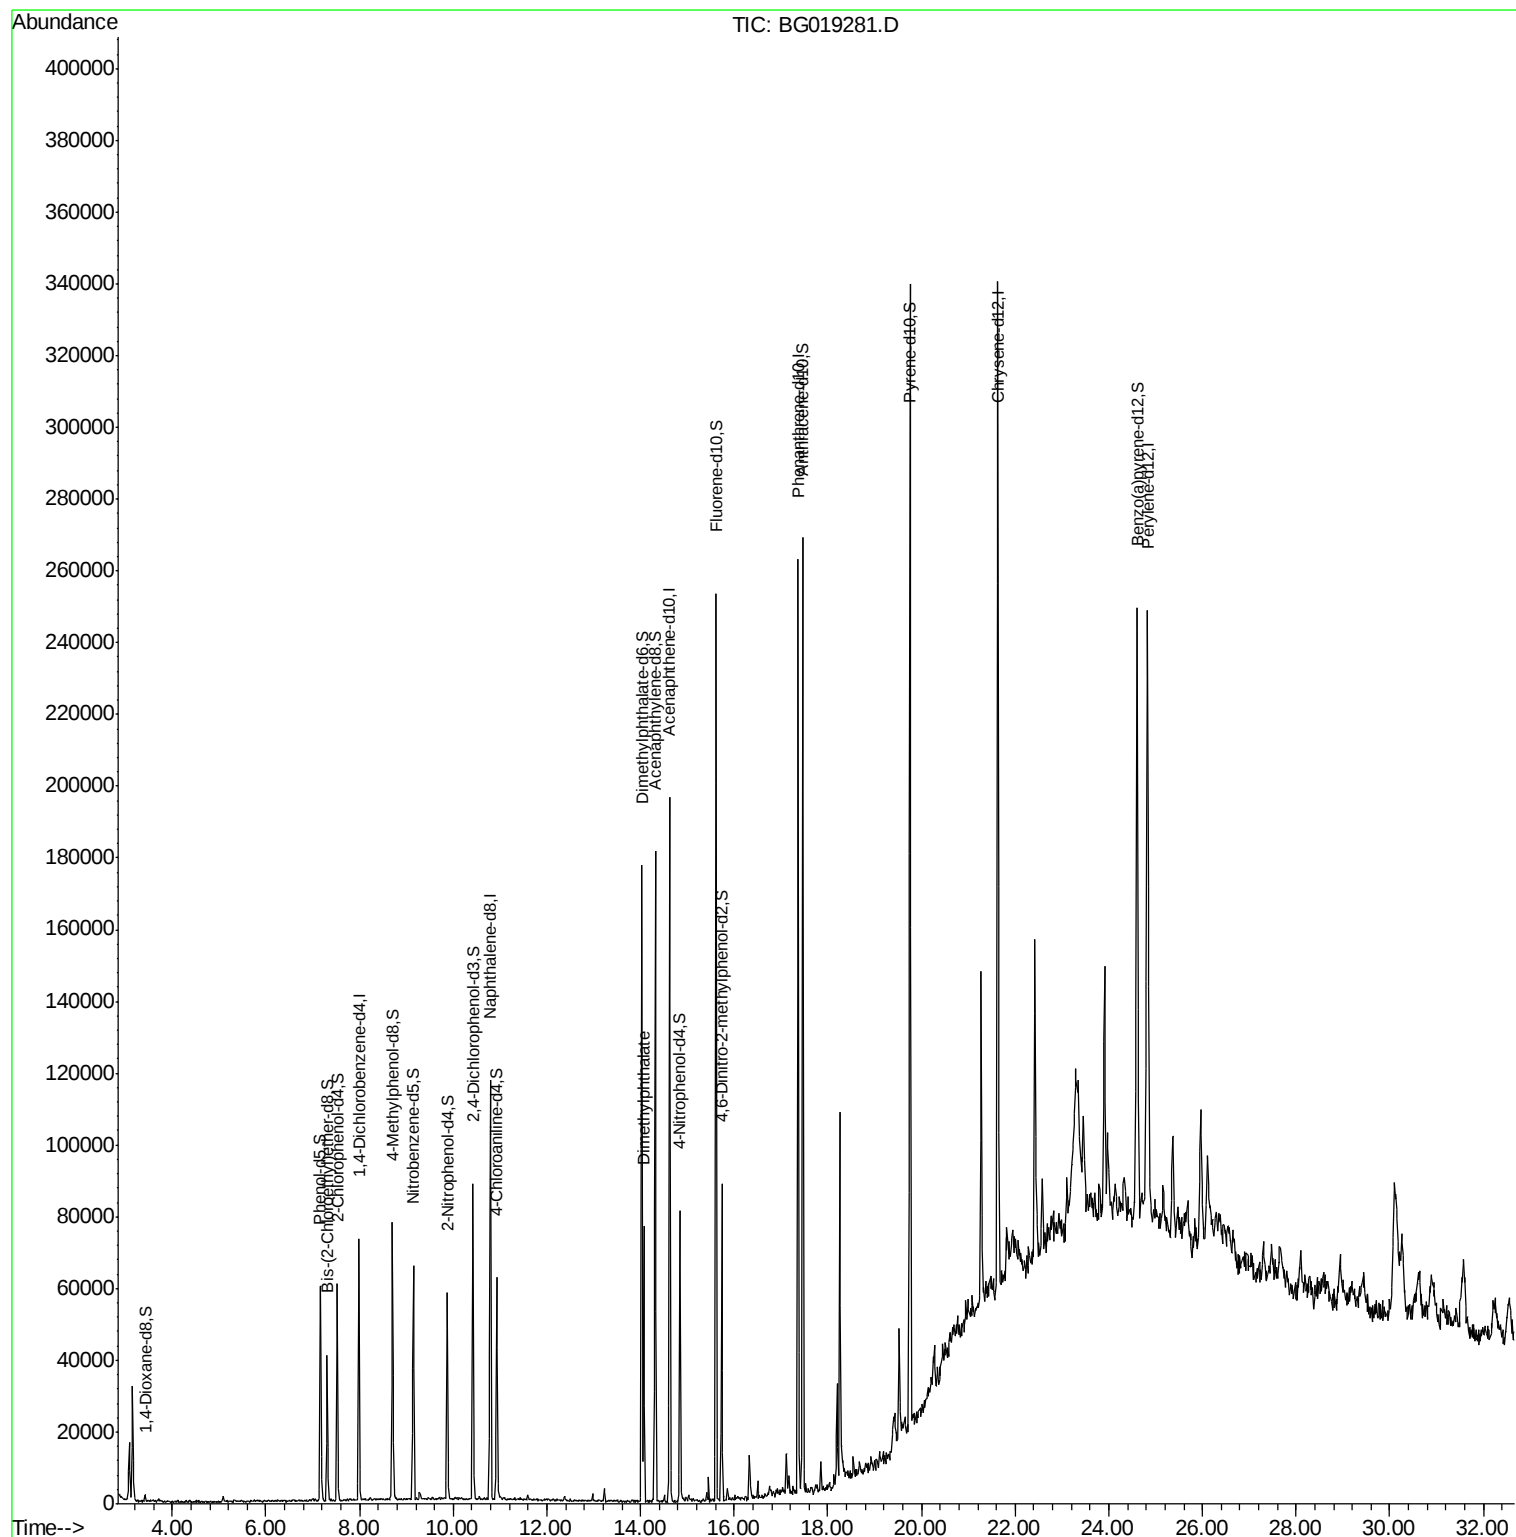

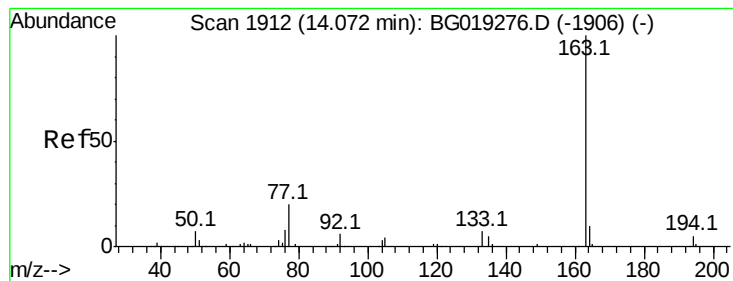

#45

Dimethylphthalate

Concen: 7.82 ng/ul

RT: 14.07 min Scan# 1912

Delta R.T. -0.00 min

Lab File: BG019281.D

Acq: 21 Oct 2015 14:52

Instrument :

BNA_G

ClientSampleId :

JG9K1


Tot Ion:163 Resp: 46354

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 10.3 8.1 12.1

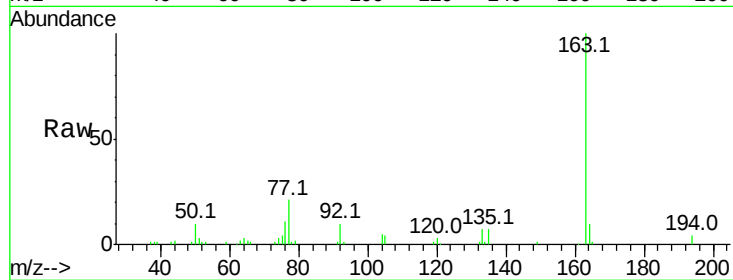

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

