

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
 Data File : BG019302.D
 Acq On : 22 Oct 2015 4:56
 Operator : UM/NP
 Sample : G4074-14
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H2

Quant Time: Oct 22 10:12:46 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 21 01:23:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	23835	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	113579	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.62	164	81663	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	177921	20.00	ng/ul	-0.01
78) Chrysene-d12	21.63	240	200065	20.00	ng/ul	-0.01
86) Perylene-d12	24.83	264	203998	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.41	96	1187	2.77	ng/uL	-0.01
5) Phenol-d5	7.16	99	34711	16.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	21614	16.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	28182	18.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	28097	15.94	ng/ul	0.00
19) Nitrobenzene-d5	9.14	128	15543	17.76	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.87	143	17825	19.19	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.42	165	35640	19.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	11129	4.70	ng/ul	-0.01
44) Dimethylphthalate-d6	14.02	166	121026	16.95	ng/ul	-0.01
47) Acenaphthylene-d8	14.31	160	136470	17.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	16020	12.48	ng/ul	0.00
58) Fluorene-d10	15.61	176	104621	17.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	20163	18.37	ng/ul	0.00
71) Anthracene-d10	17.46	188	150638	17.92	ng/ul	0.00
79) Pyrene-d10	19.75	212	162468	17.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.61	264	175454	17.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.07	163	50723	7.05	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102115\
Data File : BG019302.D
Acq On : 22 Oct 2015 4:56
Operator : UM/NP
Sample : G4074-14
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H2

Quant Time: Oct 22 10:12:46 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG101515.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 21 01:23:32 2015
Response via : Initial Calibration

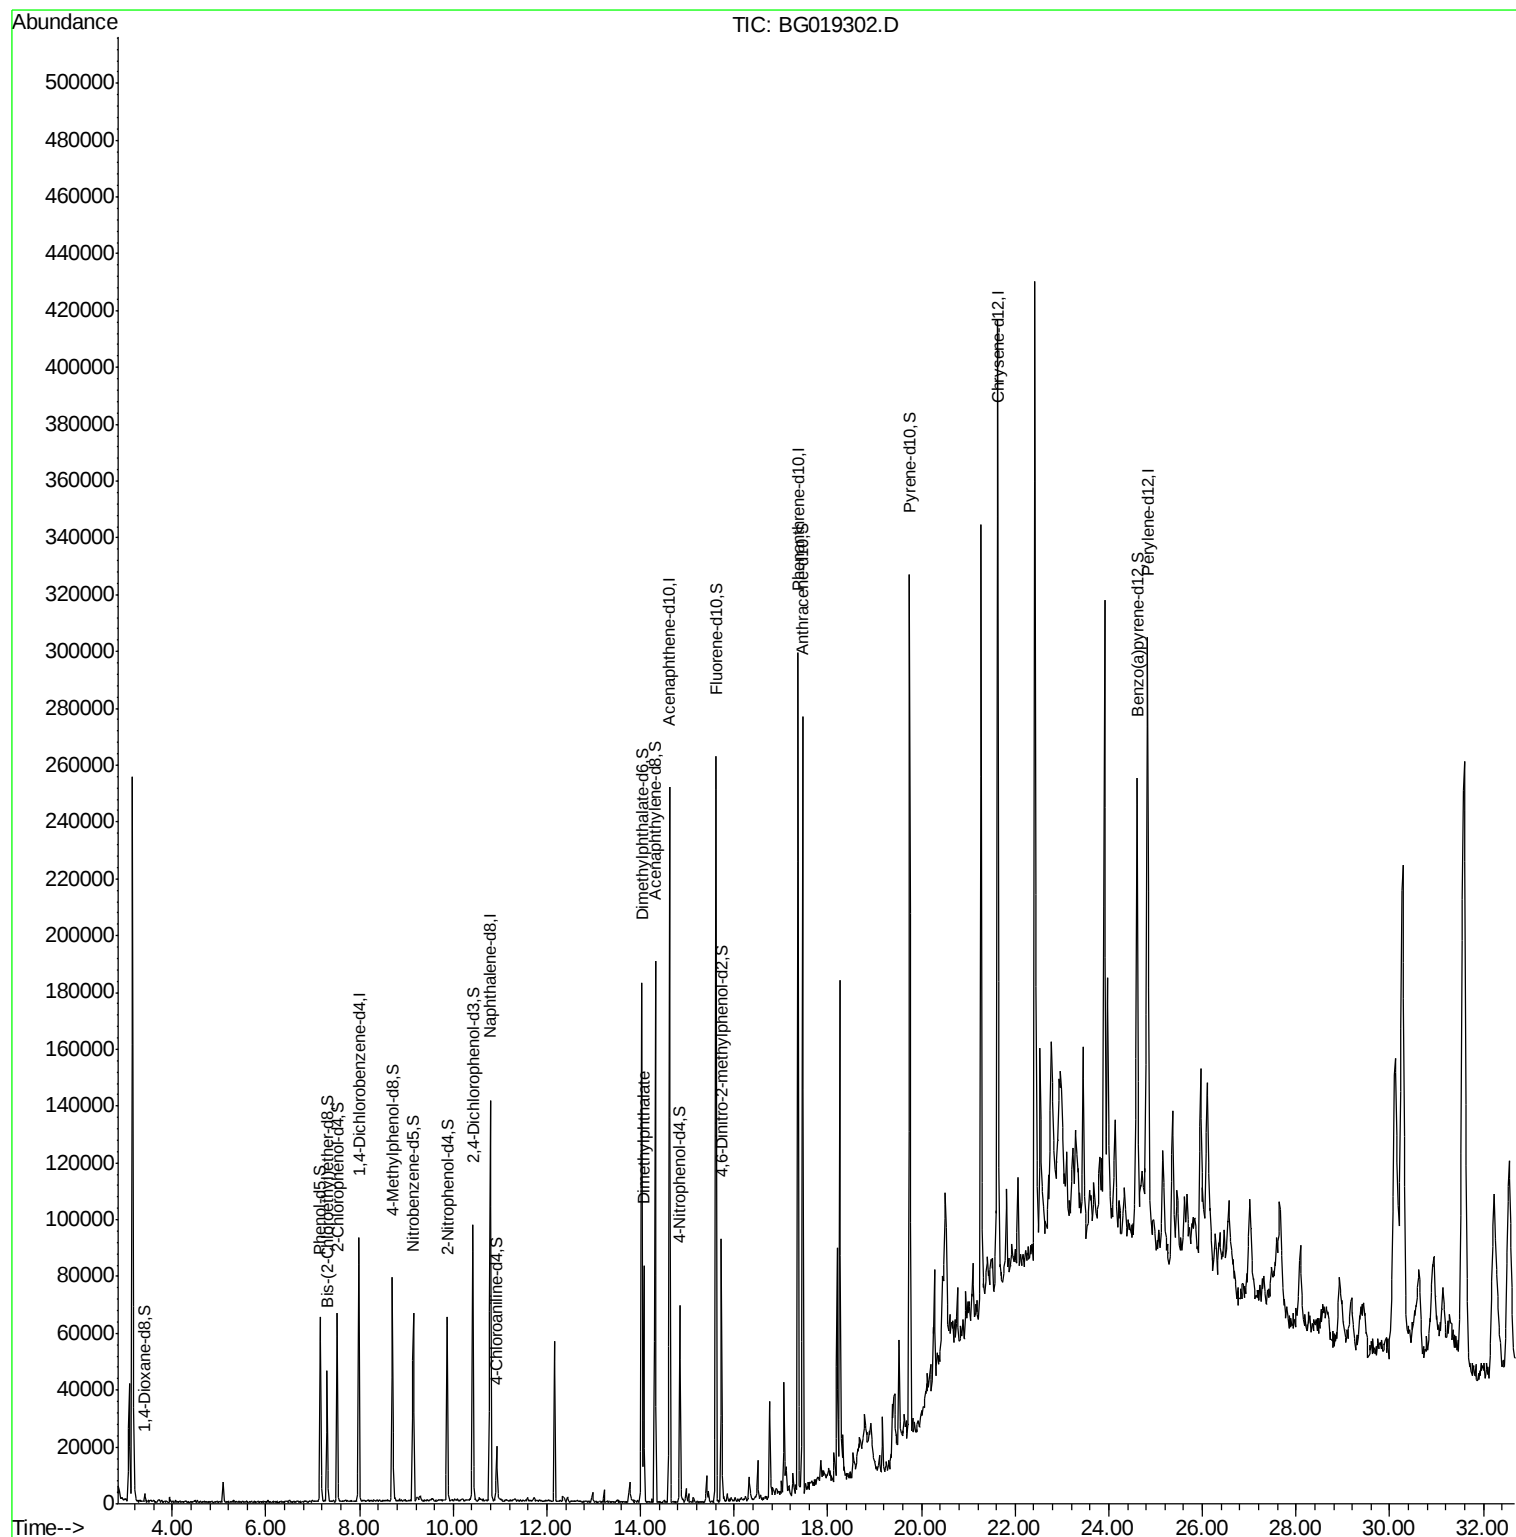

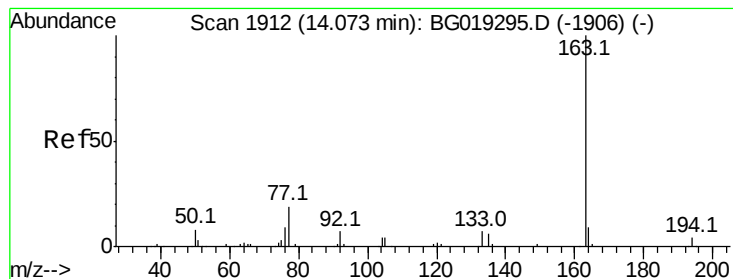

#45

Dimethylphthalate

Concen: 7.05 ng/ul

RT: 14.07 min Scan# 1911

Delta R.T. -0.01 min

Lab File: BG019302.D

Acq: 22 Oct 2015 4:56

Instrument :

BNA_G

ClientSampleId :

JG9H2


Tot Ion:163 Resp: 50723

Ion Ratio Lower Upper

163 100

194 3.5 3.3 4.9

164 11.6 8.1 12.1

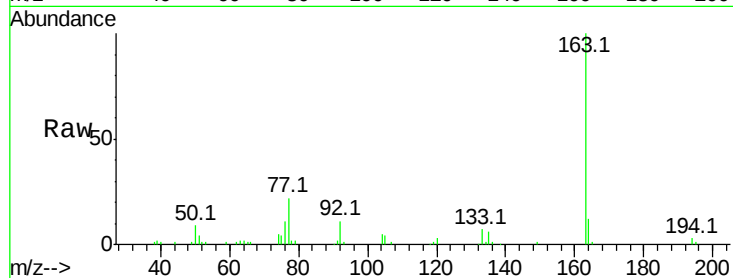

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

