
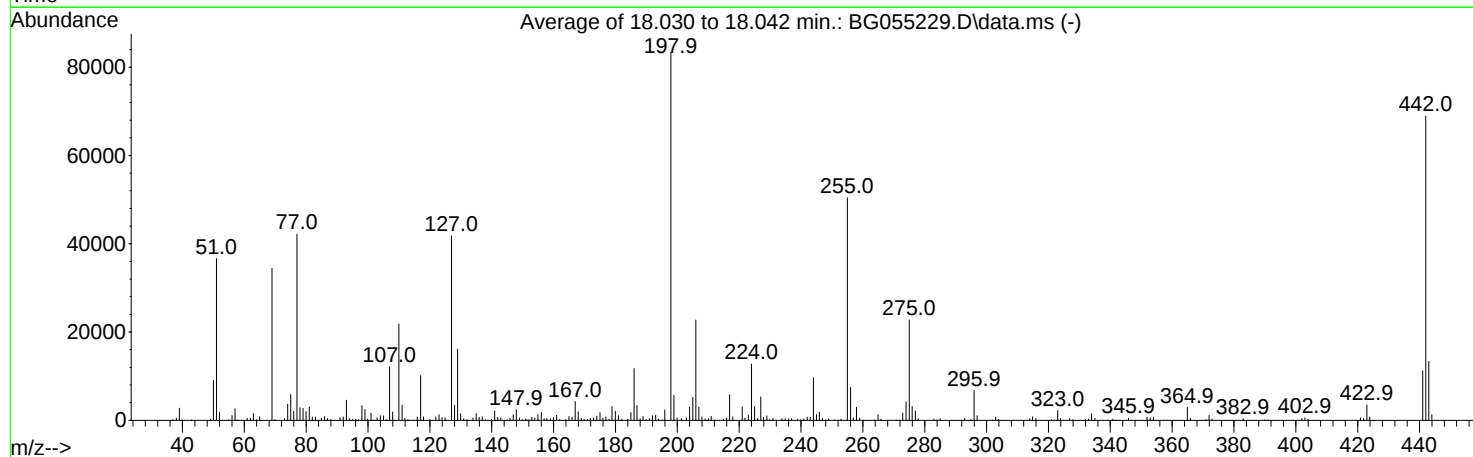


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102122\
Data File : BG055229.D
Acq On : 21 Oct 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 20 09:21:42 2022

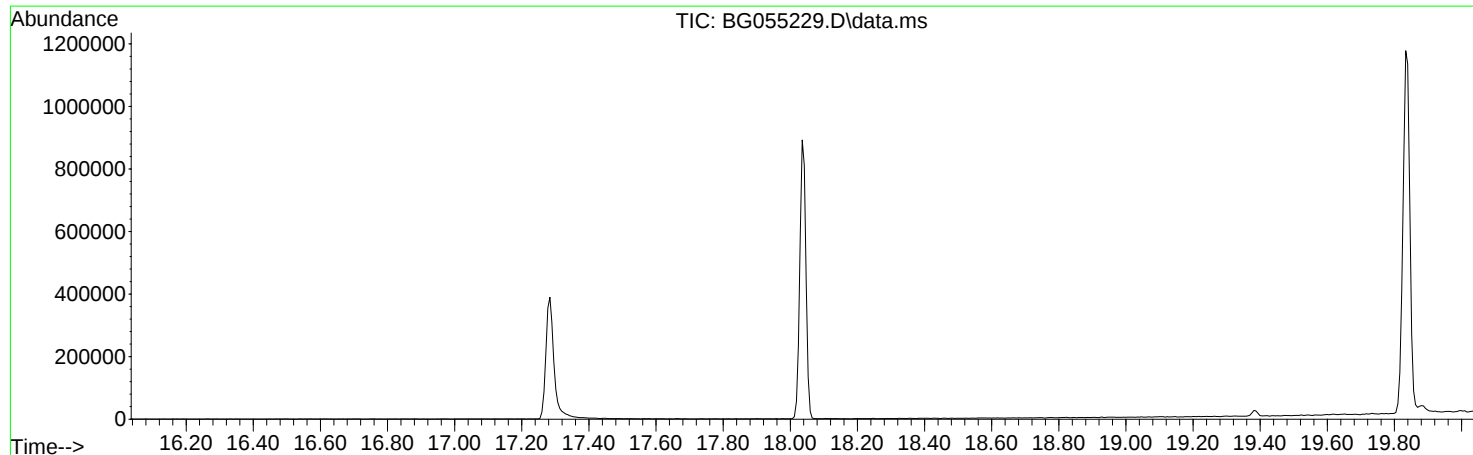




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	36645	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.3	34448	PASS
70	69	0.00	2	0.3	92	PASS
127	198	10	80	50.1	41789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83355	PASS
199	198	5	9	6.8	5634	PASS
275	198	10	60	27.3	22744	PASS
365	198	1	100	3.5	2936	PASS
441	198	0.01	100	13.4	11205	PASS
442	442	50	100	100.0	68933	PASS
443	442	15	24	19.4	13352	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102122\
Data File : BG055229.D
Acq On : 21 Oct 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 03:37:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 09:21:42 2022
Response via : Initial Calibration

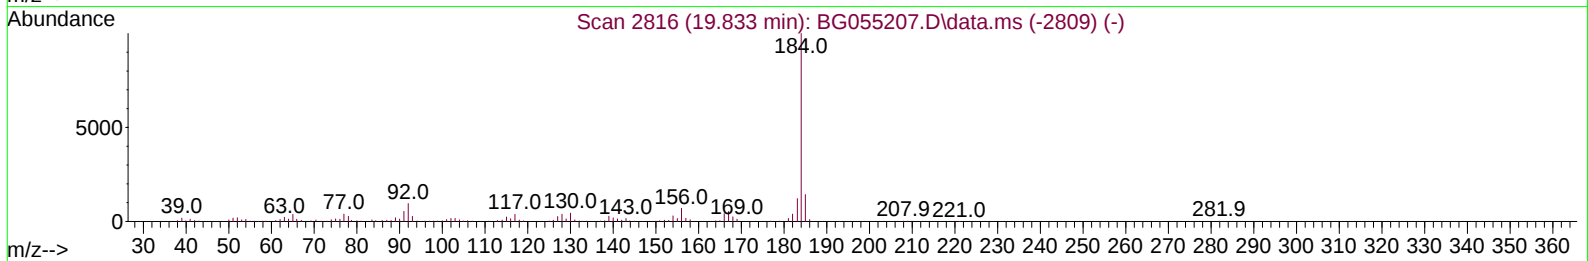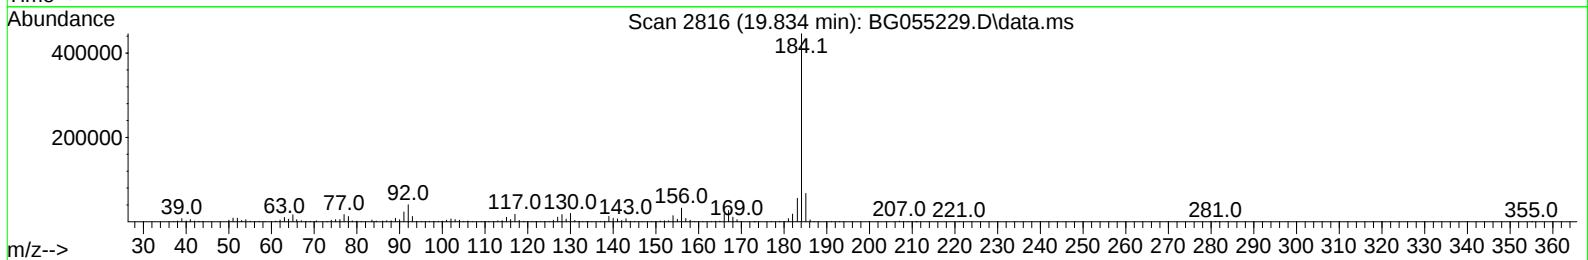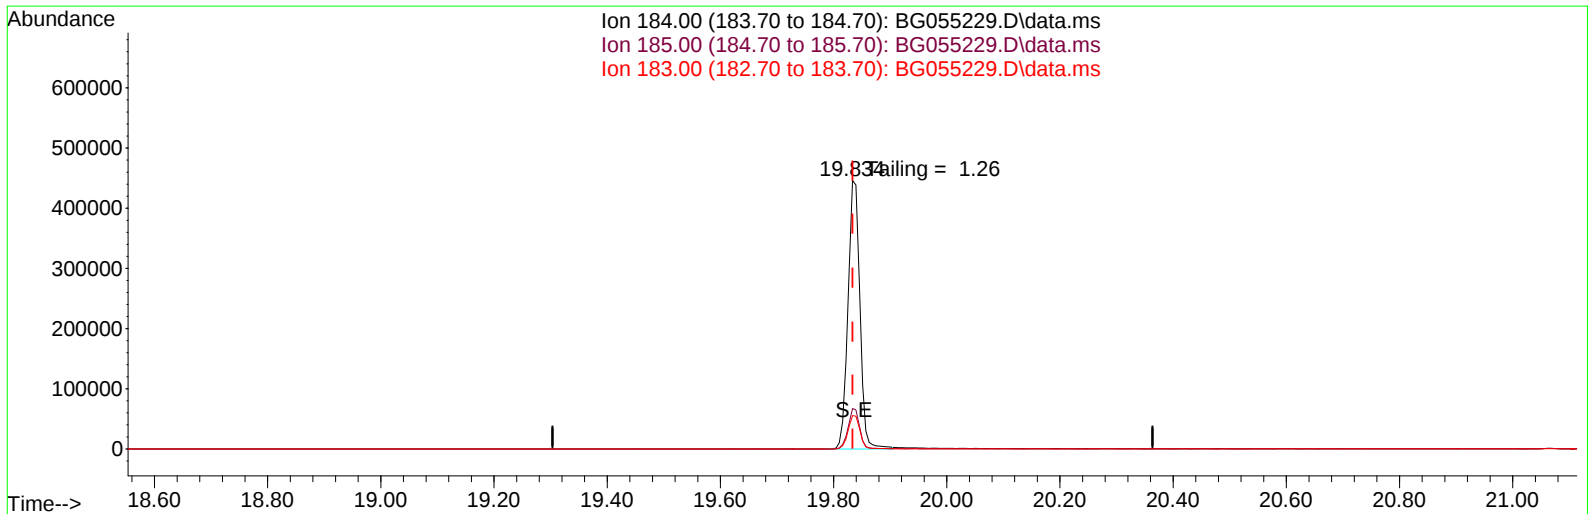

TIC: BG055229.D\data.ms

(77) Benzidine

19.834min (+ 0.000) 420709.12 ng




response 663301

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	15.07
183.00	12.20	12.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102122\
Data File : BG055229.D
Acq On : 21 Oct 2022 10:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 22 03:37:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 20 09:21:42 2022
Response via : Initial Calibration

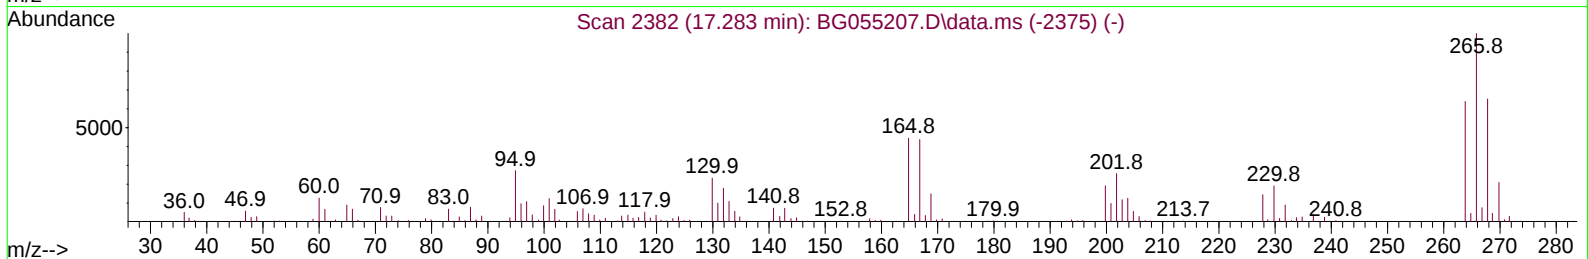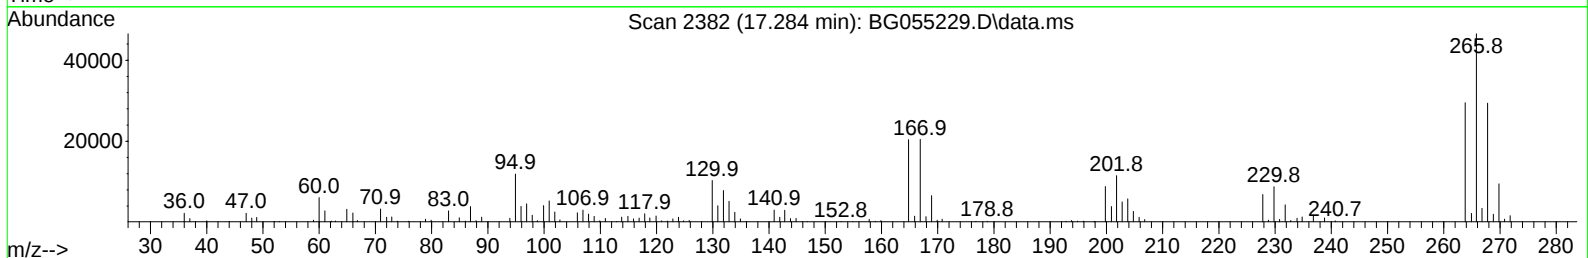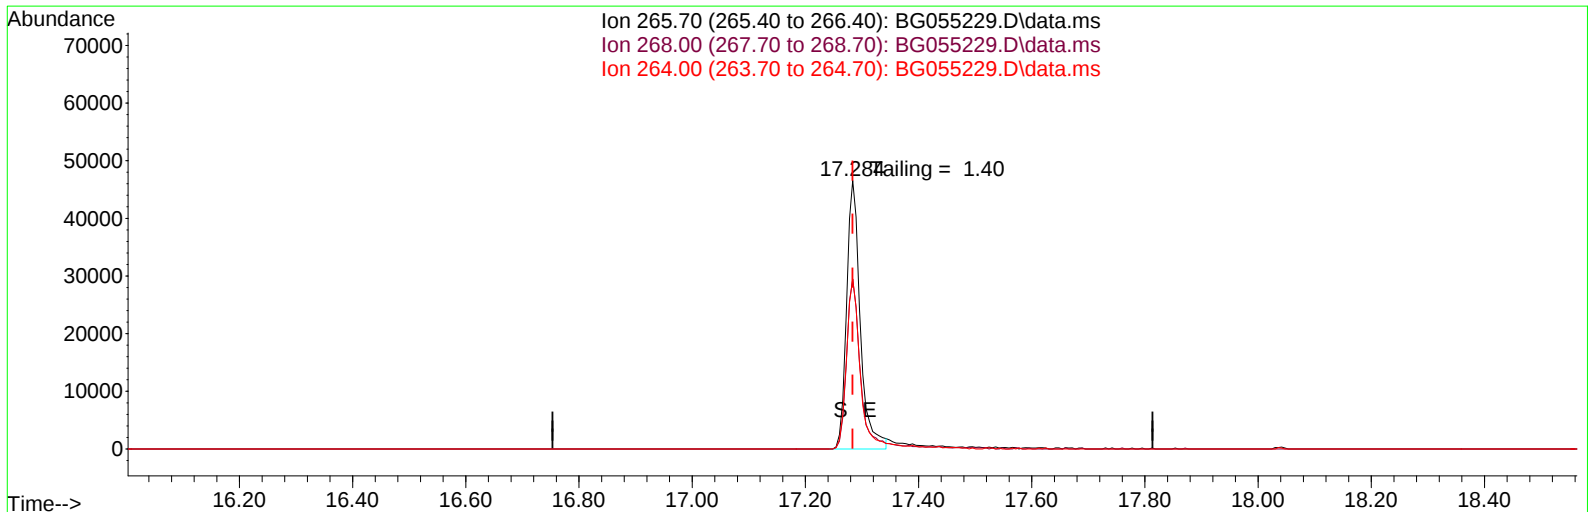

TIC: BG055229.D\data.ms

(70) Pentachlorophenol (C)

17.284min (+ 0.001) 32753.50 ng

response 83346

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	69.70	63.16
264.00	63.90	63.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/21/2022	BNA_G	BG055229.D
Compound Name	Response	Retention Time
DDT	281735	21.068
DDD	7169	20.615
DDE	327	20.122
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7496	289231	2.59

Instrument :
BNA_G
ClientSampleId :
DFTPP