

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019316.D
 Acq On : 24 Oct 2015 2:15
 Operator : UM/NP
 Sample : PB86228BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK28

Quant Time: Oct 25 01:26:40 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 01:11:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	37969	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	150450	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	124217	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	344121	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	474403	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	423536	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.56	96	5359	7.84	ng/uL	0.00
5) Phenol-d5	7.37	99	112940	33.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	71853	36.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	73882	34.26	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	95142	36.53	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	42282	37.01	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	50002	38.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	97497	34.25	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	62110	21.97	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	400793	38.92	ng/ul	0.00
47) Acenaphthylene-d8	14.56	160	415165	36.42	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	64335	38.42	ng/ul	0.00
58) Fluorene-d10	15.85	176	340893	35.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	87199	38.49	ng/ul	0.00
71) Anthracene-d10	17.70	188	621974	39.47	ng/ul	0.00
79) Pyrene-d10	19.97	212	746690	35.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	863650	39.97	ng/ul	0.00


Target Compounds						Qvalue
15) N-Nitroso-di-n-propylamine	8.94	70	3321	1.23	ng/ul#	1
21) Isophorone	10.14	82	8552	1.20	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019316.D
Acq On : 24 Oct 2015 2:15
Operator : UM/NP
Sample : PB86228BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK28

Quant Time: Oct 25 01:26:40 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 01:11:12 2015
Response via : Initial Calibration




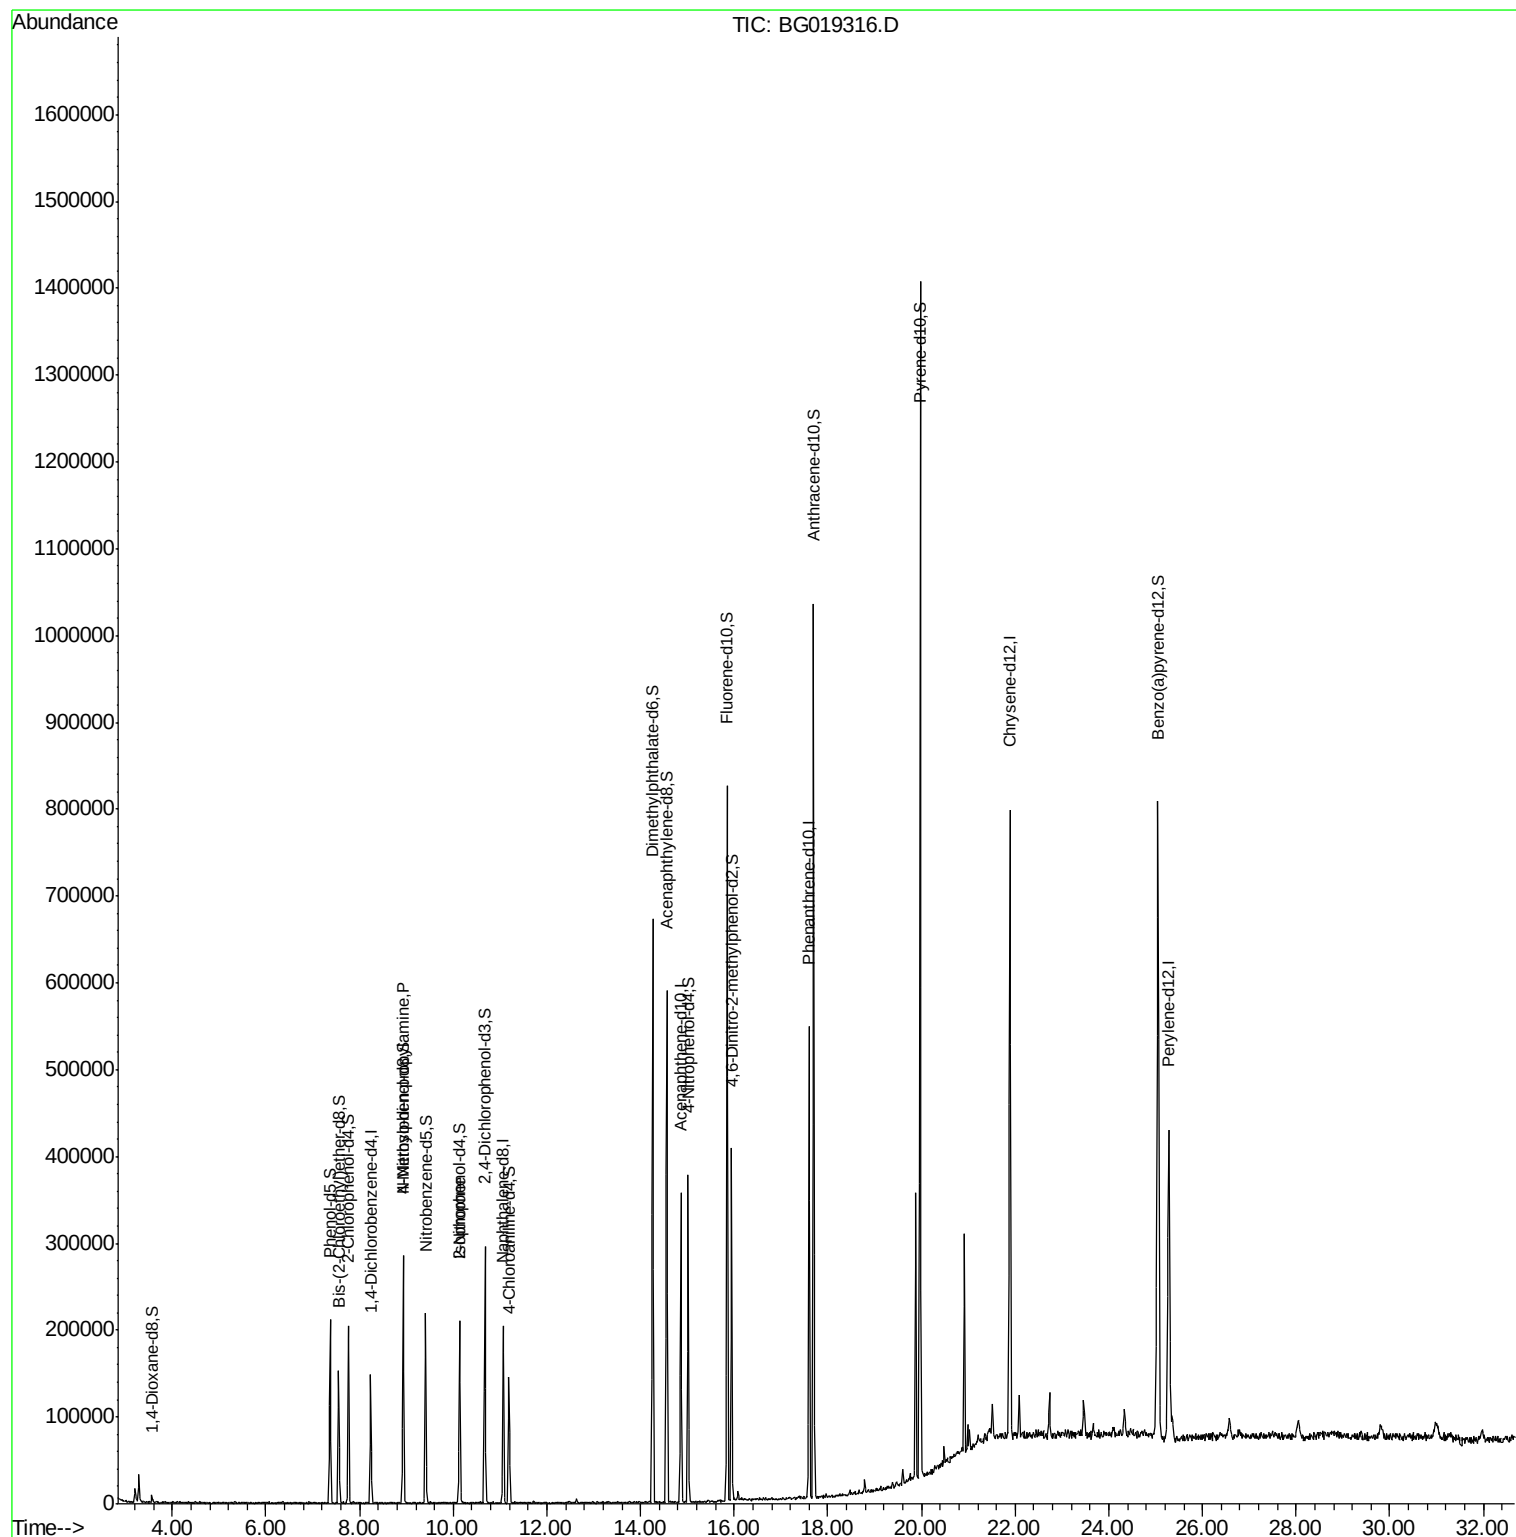


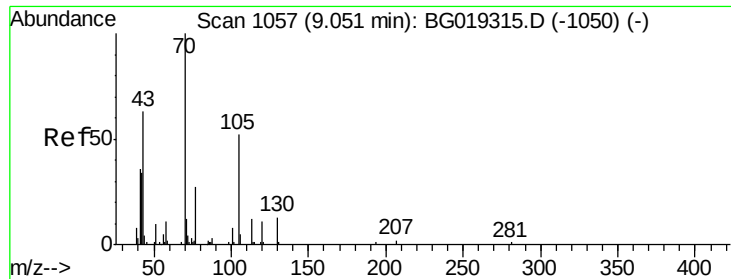

#15
N-Nitroso-di-n-propylamine
Concen: 1.23 ng/ul
RT: 8.94 min Scan# 1038
Delta R.T. -0.11 min
Lab File: BG019316.D
Acq: 24 Oct 2015 2:15

Instrument :
BNA_G
ClientSampleId :
SBLK28

Tgt Ion:	70	Resp:	3321
Ion	Ratio	Lower	Upper
70	100		
42	180.0	36.6	55.0#
101	0.0	5.8	8.8#
130	0.0	14.6	22.0#

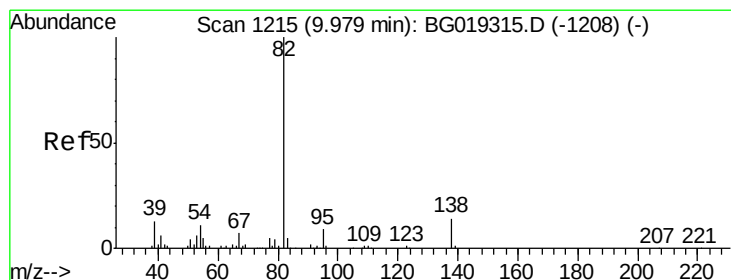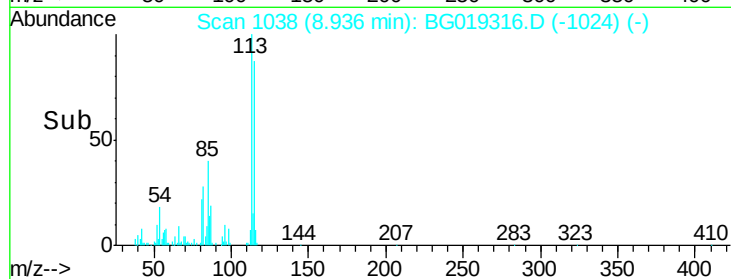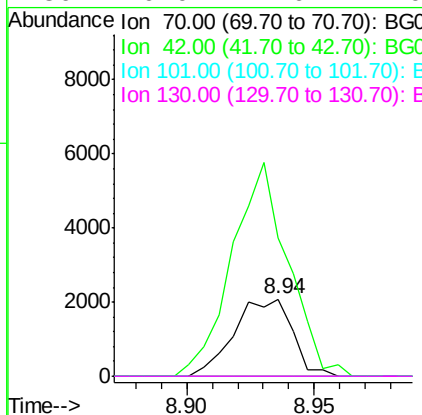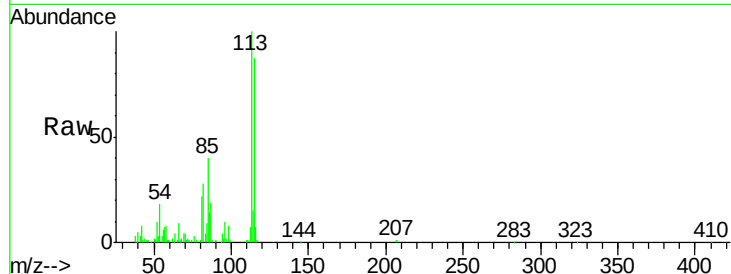

#21
Isophorone
Concen: 1.20 ng/ul
RT: 10.14 min Scan# 1243
Delta R.T. 0.16 min
Lab File: BG019316.D
Acq: 24 Oct 2015 2:15

Tgt Ion:	82	Resp:	8552
Ion	Ratio	Lower	Upper
82	100		
95	5.3	6.7	10.1#
138	0.0	10.8	16.2#

