

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019320.D
 Acq On : 24 Oct 2015 4:46
 Operator : UM/NP
 Sample : G4058-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LL6

Quant Time: Oct 25 01:27:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 01:11:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	26871	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	100884	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	82447	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	234491	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	331602	20.00	ng/ul	0.00
86) Perylene-d12	25.27	264	327462	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.57	96	2465	5.09	ng/uL	0.00
5) Phenol-d5	7.37	99	62741	26.53	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	40697	28.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	42298	27.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	51783	28.09	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	21950	28.65	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	25747	29.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	54365	28.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	59571	31.42	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	210706	30.82	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	227318	30.05	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	33154	29.83	ng/ul	0.00
58) Fluorene-d10	15.85	176	194904	30.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	42715	27.67	ng/ul	0.00
71) Anthracene-d10	17.70	188	330815	30.81	ng/ul	0.00
79) Pyrene-d10	19.96	212	433122	29.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.04	264	519638	31.11	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.30	163	79341	11.62	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019320.D
Acq On : 24 Oct 2015 4:46
Operator : UM/NP
Sample : G4058-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LL6

Quant Time: Oct 25 01:27:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 01:11:12 2015
Response via : Initial Calibration

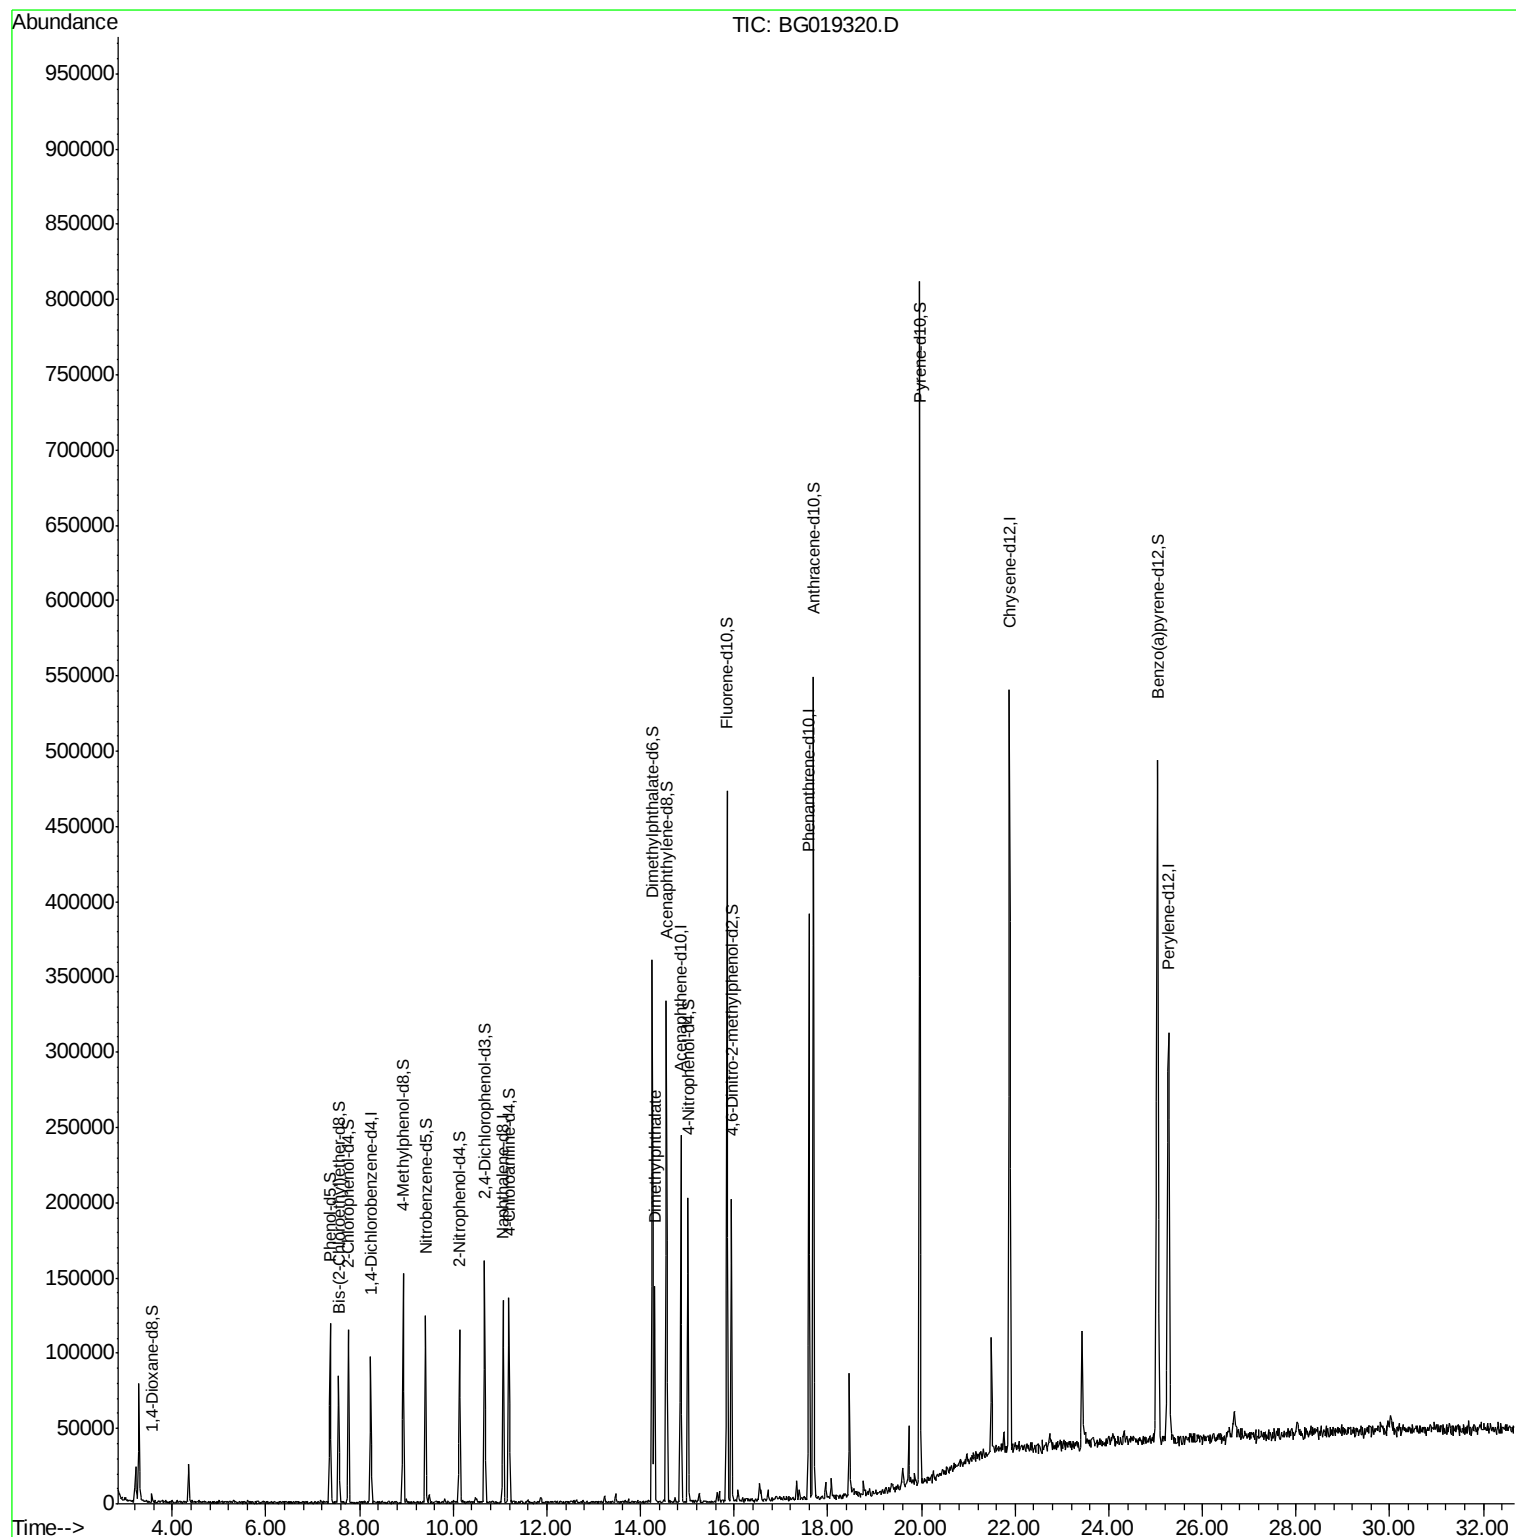

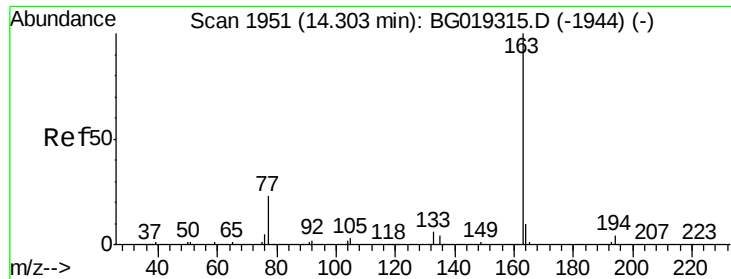

#45

Dimethylphthalate

Concen: 11.62 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. -0.00 min

Lab File: BG019320.D

Acq: 24 Oct 2015 4:46

Instrument :

BNA_G

ClientSampleId :

E5LL6


Tgt Ion:163 Resp: 79341

Ion Ratio Lower Upper

163 100

194 4.0 4.3 6.5#

164 9.7 7.5 11.3

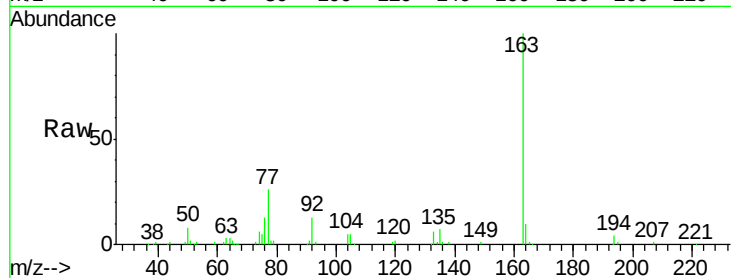

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

