

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019327.D
 Acq On : 24 Oct 2015 9:11
 Operator : UM/NP
 Sample : G4075-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K8

Quant Time: Oct 25 02:39:18 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 02:37:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	46173	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	187516	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	143756	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.59	188	397321	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	507381	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	481144	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.56	96	2733	3.29	ng/uL	0.00
5) Phenol-d5	7.37	99	83621	20.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	52236	21.53	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	52818	20.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	65747	20.76	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	27664	19.43	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	32782	20.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	70192	19.79	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	67420	19.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	236768	19.87	ng/ul	0.00
47) Acenaphthylene-d8	14.56	160	272981	20.69	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	36545	18.86	ng/ul	0.00
58) Fluorene-d10	15.84	176	218808	19.57	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.94	200	43425	16.60	ng/ul	0.00
71) Anthracene-d10	17.69	188	355424	19.54	ng/ul	0.00
79) Pyrene-d10	19.96	212	431654	19.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.03	264	485402	19.78	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.30	163	60151	5.05	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019327.D
Acq On : 24 Oct 2015 9:11
Operator : UM/NP
Sample : G4075-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K8

Quant Time: Oct 25 02:39:18 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 02:37:52 2015
Response via : Initial Calibration

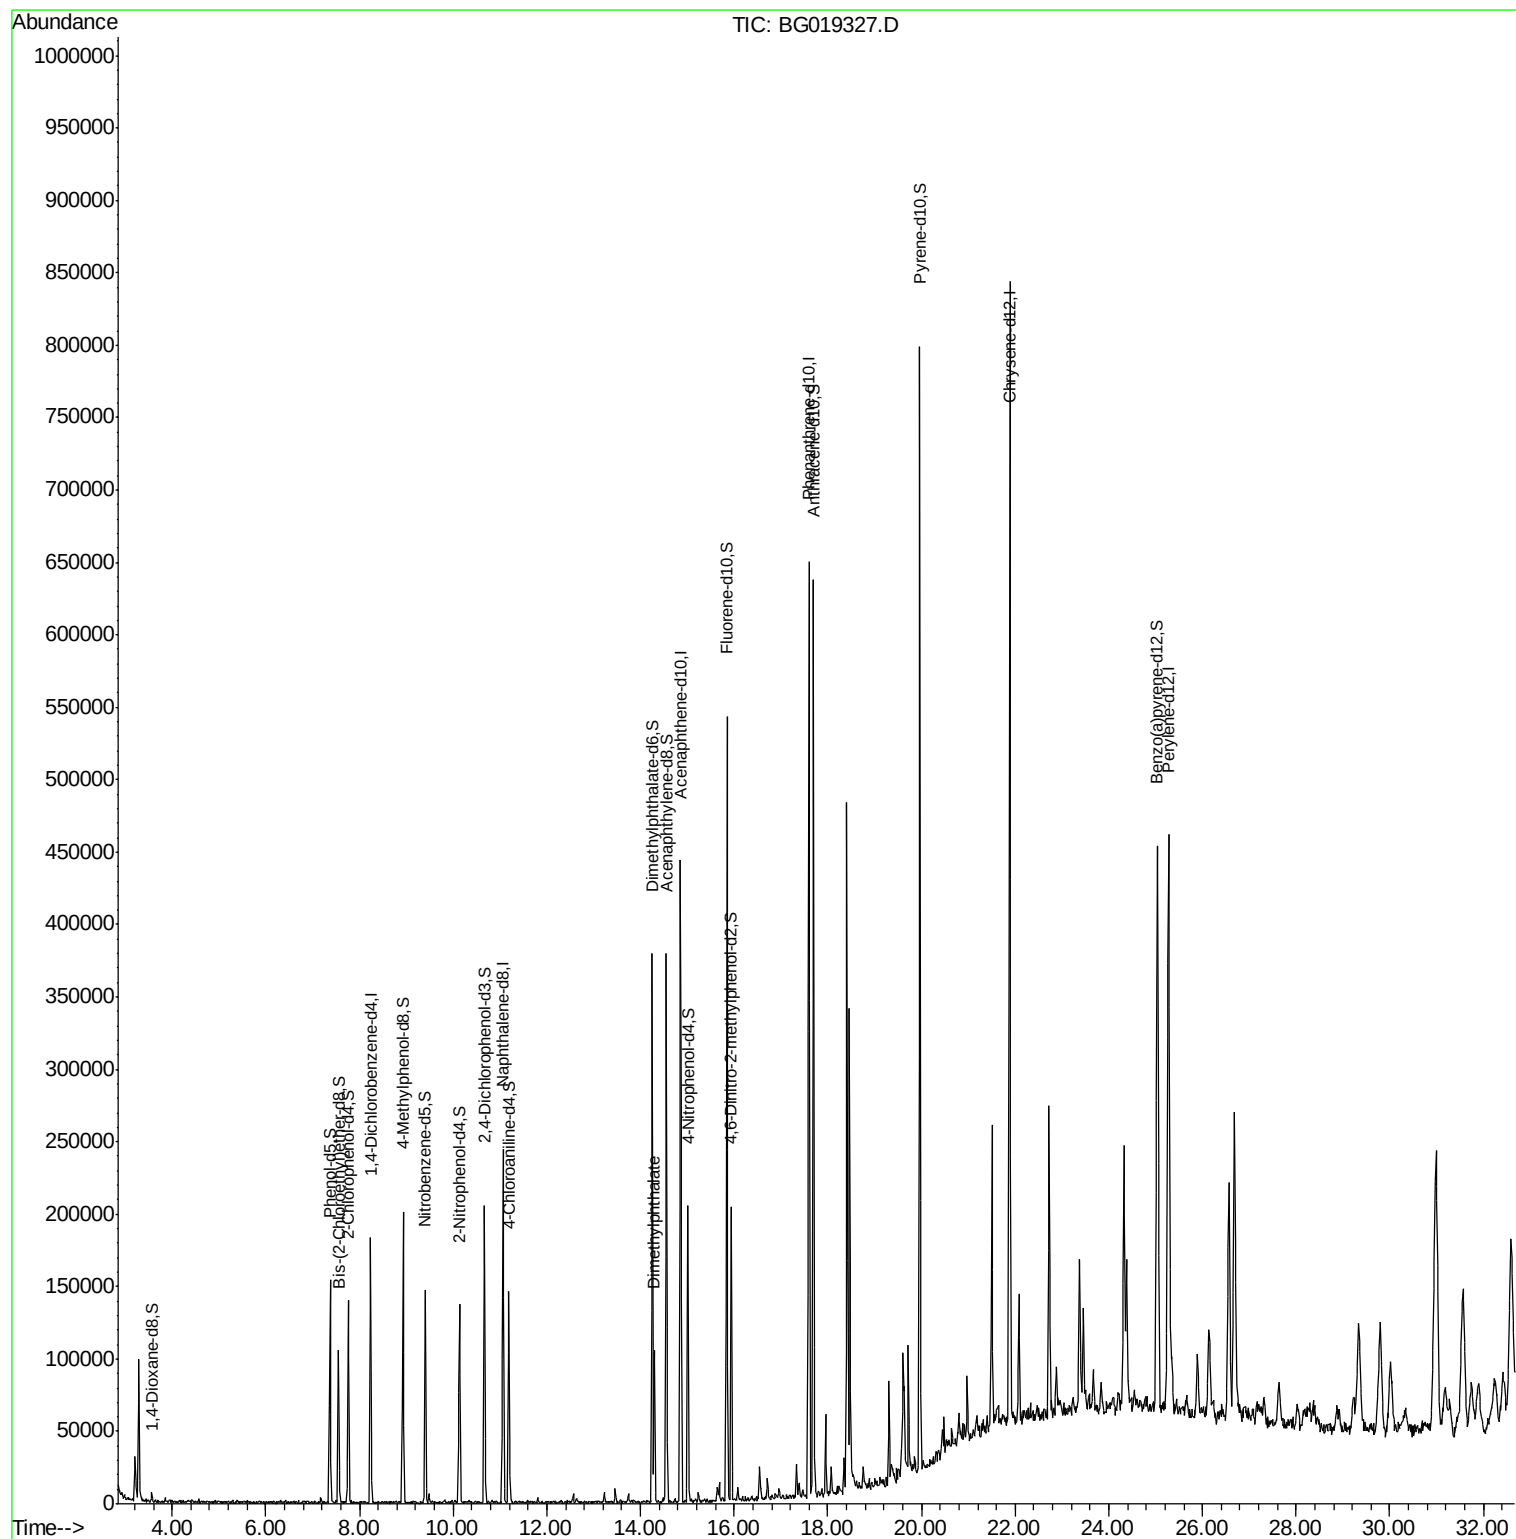

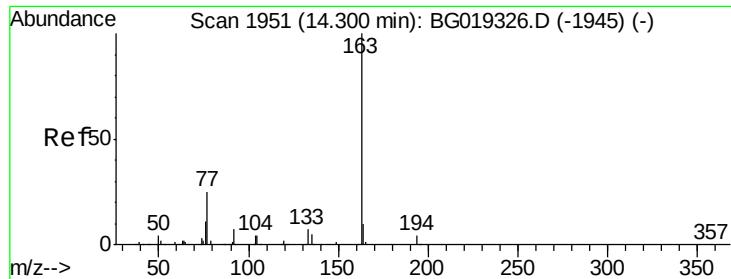

#45

Dimethylphthalate

Concen: 5.05 ng/ul

RT: 14.30 min Scan# 1950

Delta R.T. -0.00 min

Lab File: BG019327.D

Acq: 24 Oct 2015 9:11

Instrument :

BNA_G

ClientSampleId :

JG9K8


Tgt Ion:163 Resp: 60151

Ion Ratio Lower Upper

163 100

194 3.1 4.3 6.5#

164 9.6 7.5 11.3

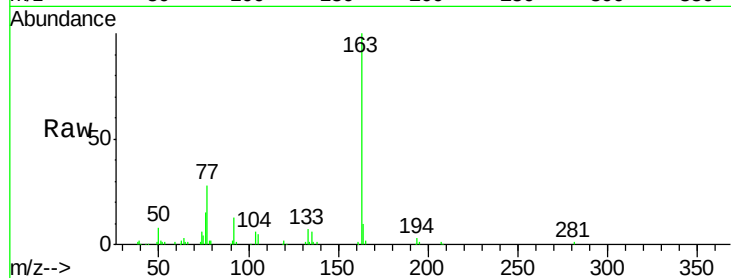

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

