

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019332.D
 Acq On : 24 Oct 2015 12:20
 Operator : UM/NP
 Sample : G4075-15
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9J3

Quant Time: Oct 25 02:40:05 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 02:37:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	40789	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	157730	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	128969	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	343426	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	462494	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	441787	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.56	96	4055	5.52	ng/uL	0.00
5) Phenol-d5	7.37	99	107471	29.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	66765	31.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	65810	28.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	87643	31.32	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	36028	30.08	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	41144	30.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	88415	29.63	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	93893	31.68	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	305953	28.61	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	347757	29.39	ng/ul	0.00
52) 4-Nitrophenol-d4	15.01	143	48900	28.12	ng/ul	0.00
58) Fluorene-d10	15.85	176	280796	27.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.94	200	65766	29.09	ng/ul	0.00
71) Anthracene-d10	17.69	188	483035	30.72	ng/ul	0.00
79) Pyrene-d10	19.97	212	590991	29.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.04	264	679063	30.13	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.30	163	164328	15.39	ng/ul	99
84) Bis(2-ethylhexyl)phthalate	21.76	149	13080	1.19	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019332.D
Acq On : 24 Oct 2015 12:20
Operator : UM/NP
Sample : G4075-15
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9J3

Quant Time: Oct 25 02:40:05 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 02:37:52 2015
Response via : Initial Calibration




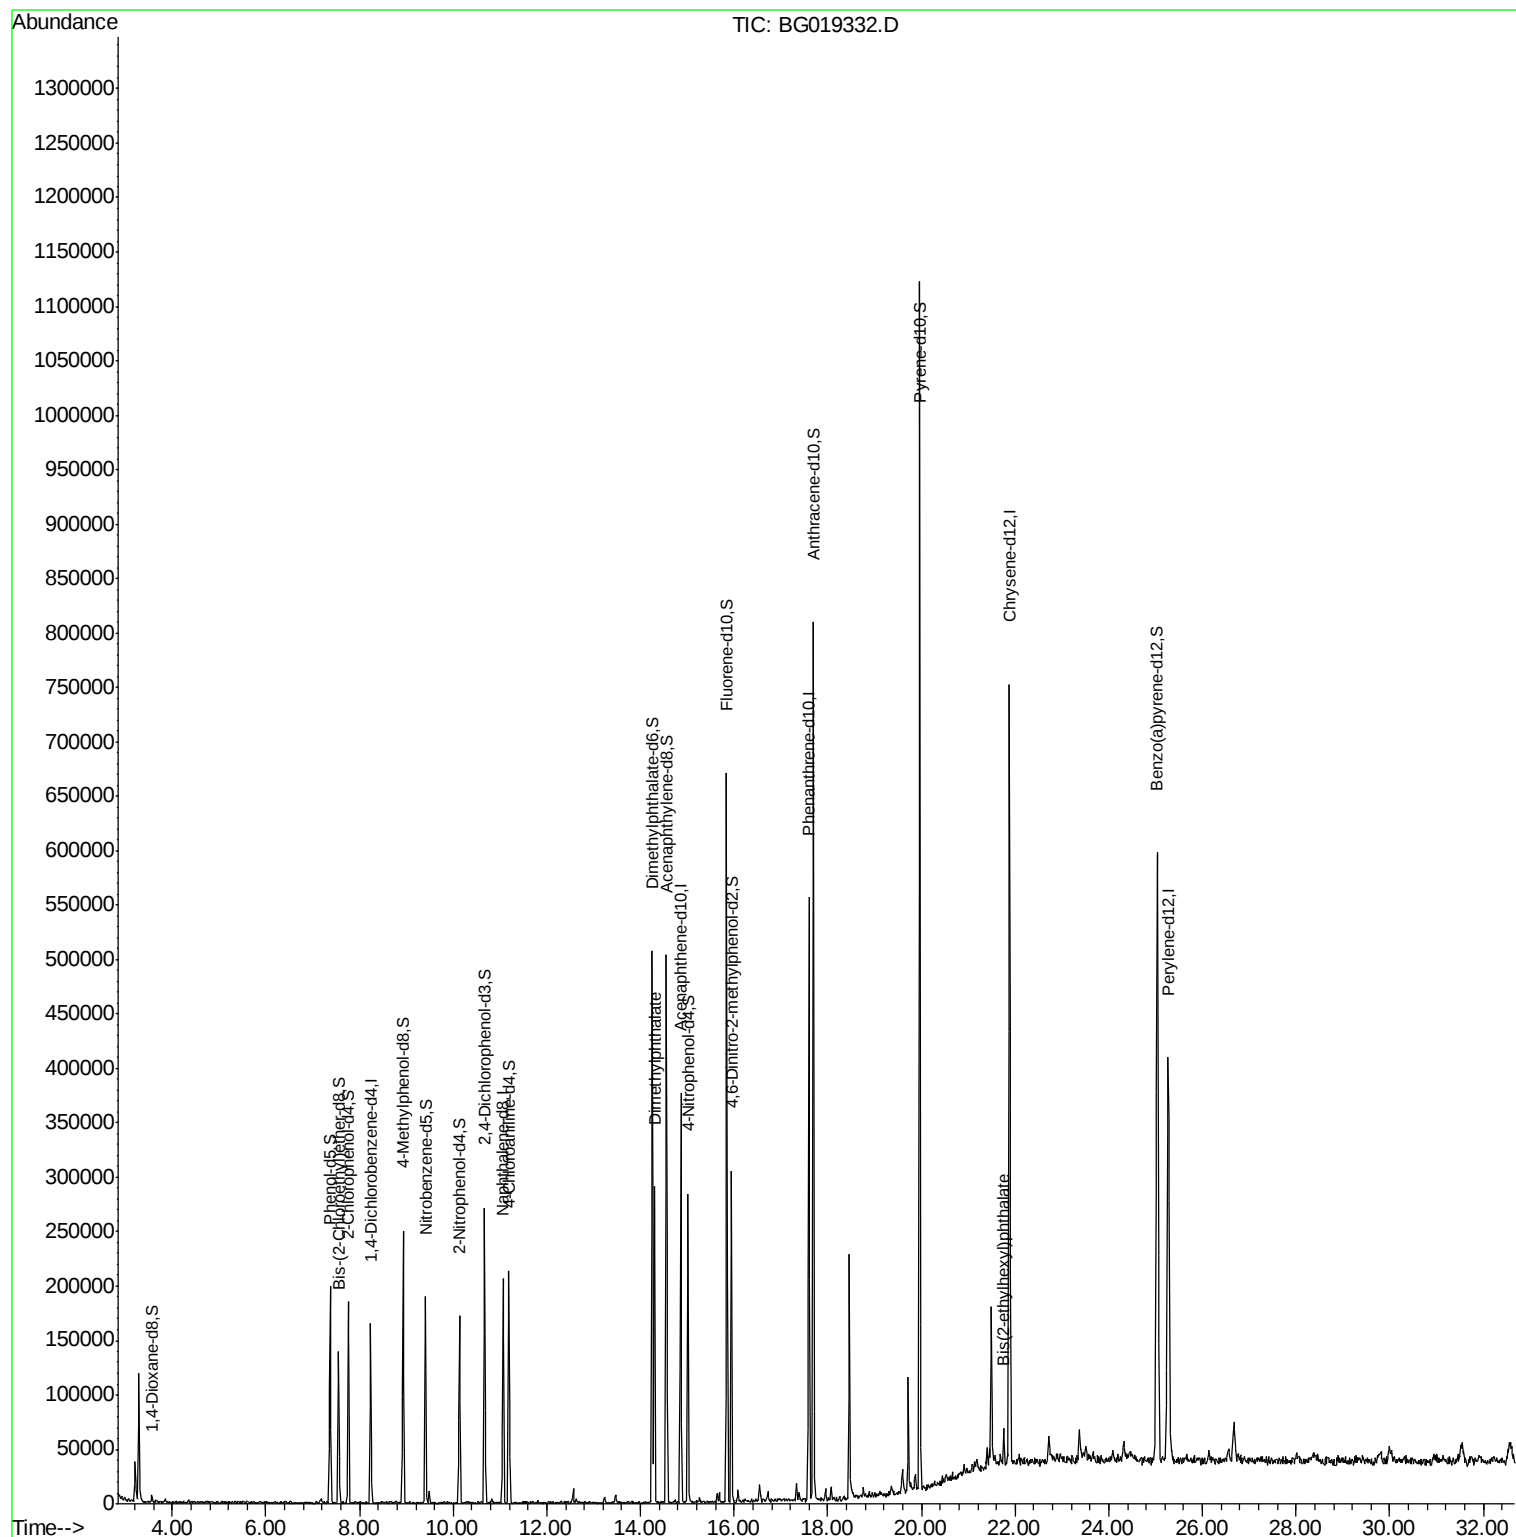


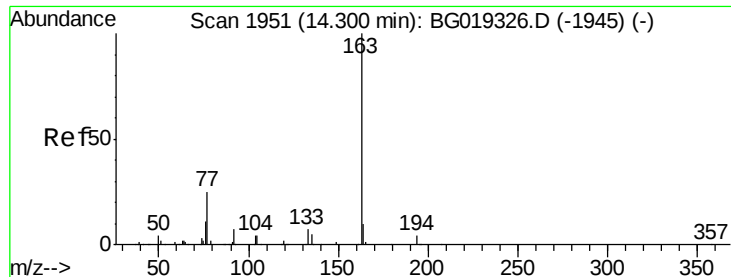

#45
 Dimethylphthalate
 Concen: 15.39 ng/ul
 RT: 14.30 min Scan# 1951
 Delta R.T. 0.00 min
 Lab File: BG019332.D
 Acq: 24 Oct 2015 12:20

Instrument :
 BNA_G
 ClientSampleId :
 JG9J3

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.5	4.3	6.5
164	9.5	7.5	11.3

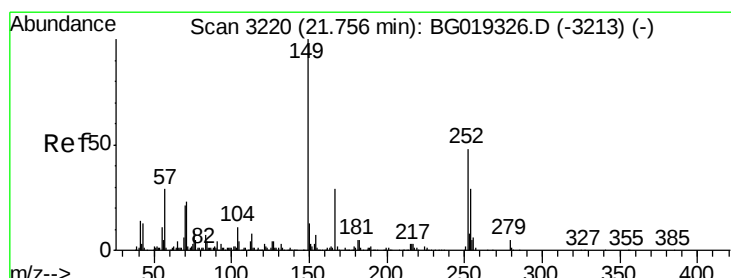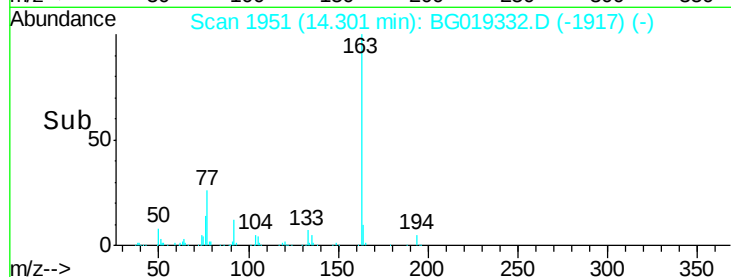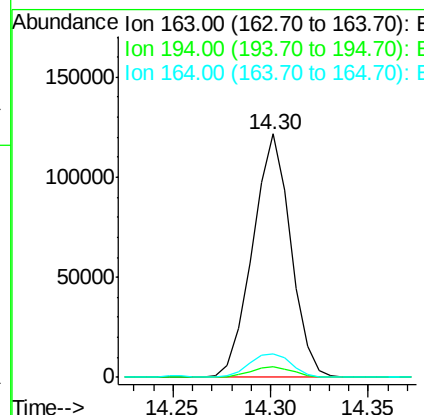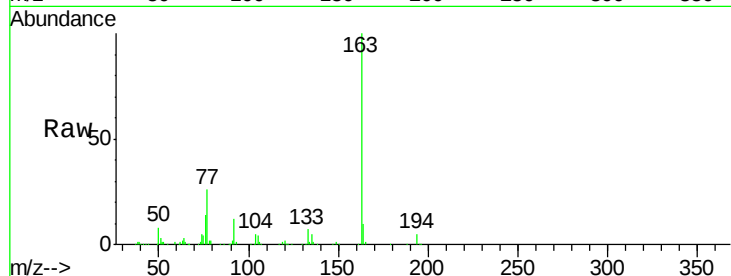

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 1.19 ng/ul
 RT: 21.76 min Scan# 3220
 Delta R.T. 0.00 min
 Lab File: BG019332.D
 Acq: 24 Oct 2015 12:20

Tgt Ion	Ratio	Lower	Upper
149	100		
167	38.1	23.2	34.8#
279	5.5	5.0	7.4

