

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019346.D
 Acq On : 24 Oct 2015 21:38
 Operator : UM/NP
 Sample : G4075-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H8

Quant Time: Oct 25 03:31:08 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 03:28:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	53366	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	219822	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	175405	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	487348	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	591072	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	566813	20.00	ng/ul	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.56	96	4214	4.38	ng/uL	0.00
5) Phenol-d5	7.38	99	155954	33.21	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.55	67	87181	31.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	98057	32.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.94	113	124604	34.04	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	50542	30.28	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	58874	30.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	129392	31.11	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	89411	21.64	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	412255	28.35	ng/ul	0.00
47) Acenaphthylene-d8	14.56	160	475558	29.55	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	74024	31.30	ng/ul	0.01
58) Fluorene-d10	15.85	176	383025	28.07	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	89744	27.97	ng/ul	0.00
71) Anthracene-d10	17.70	188	650548	29.15	ng/ul	0.00
79) Pyrene-d10	19.97	212	742818	28.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	837718	28.97	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.30	163	250683	17.26	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019346.D
Acq On : 24 Oct 2015 21:38
Operator : UM/NP
Sample : G4075-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H8

Quant Time: Oct 25 03:31:08 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 03:28:11 2015
Response via : Initial Calibration

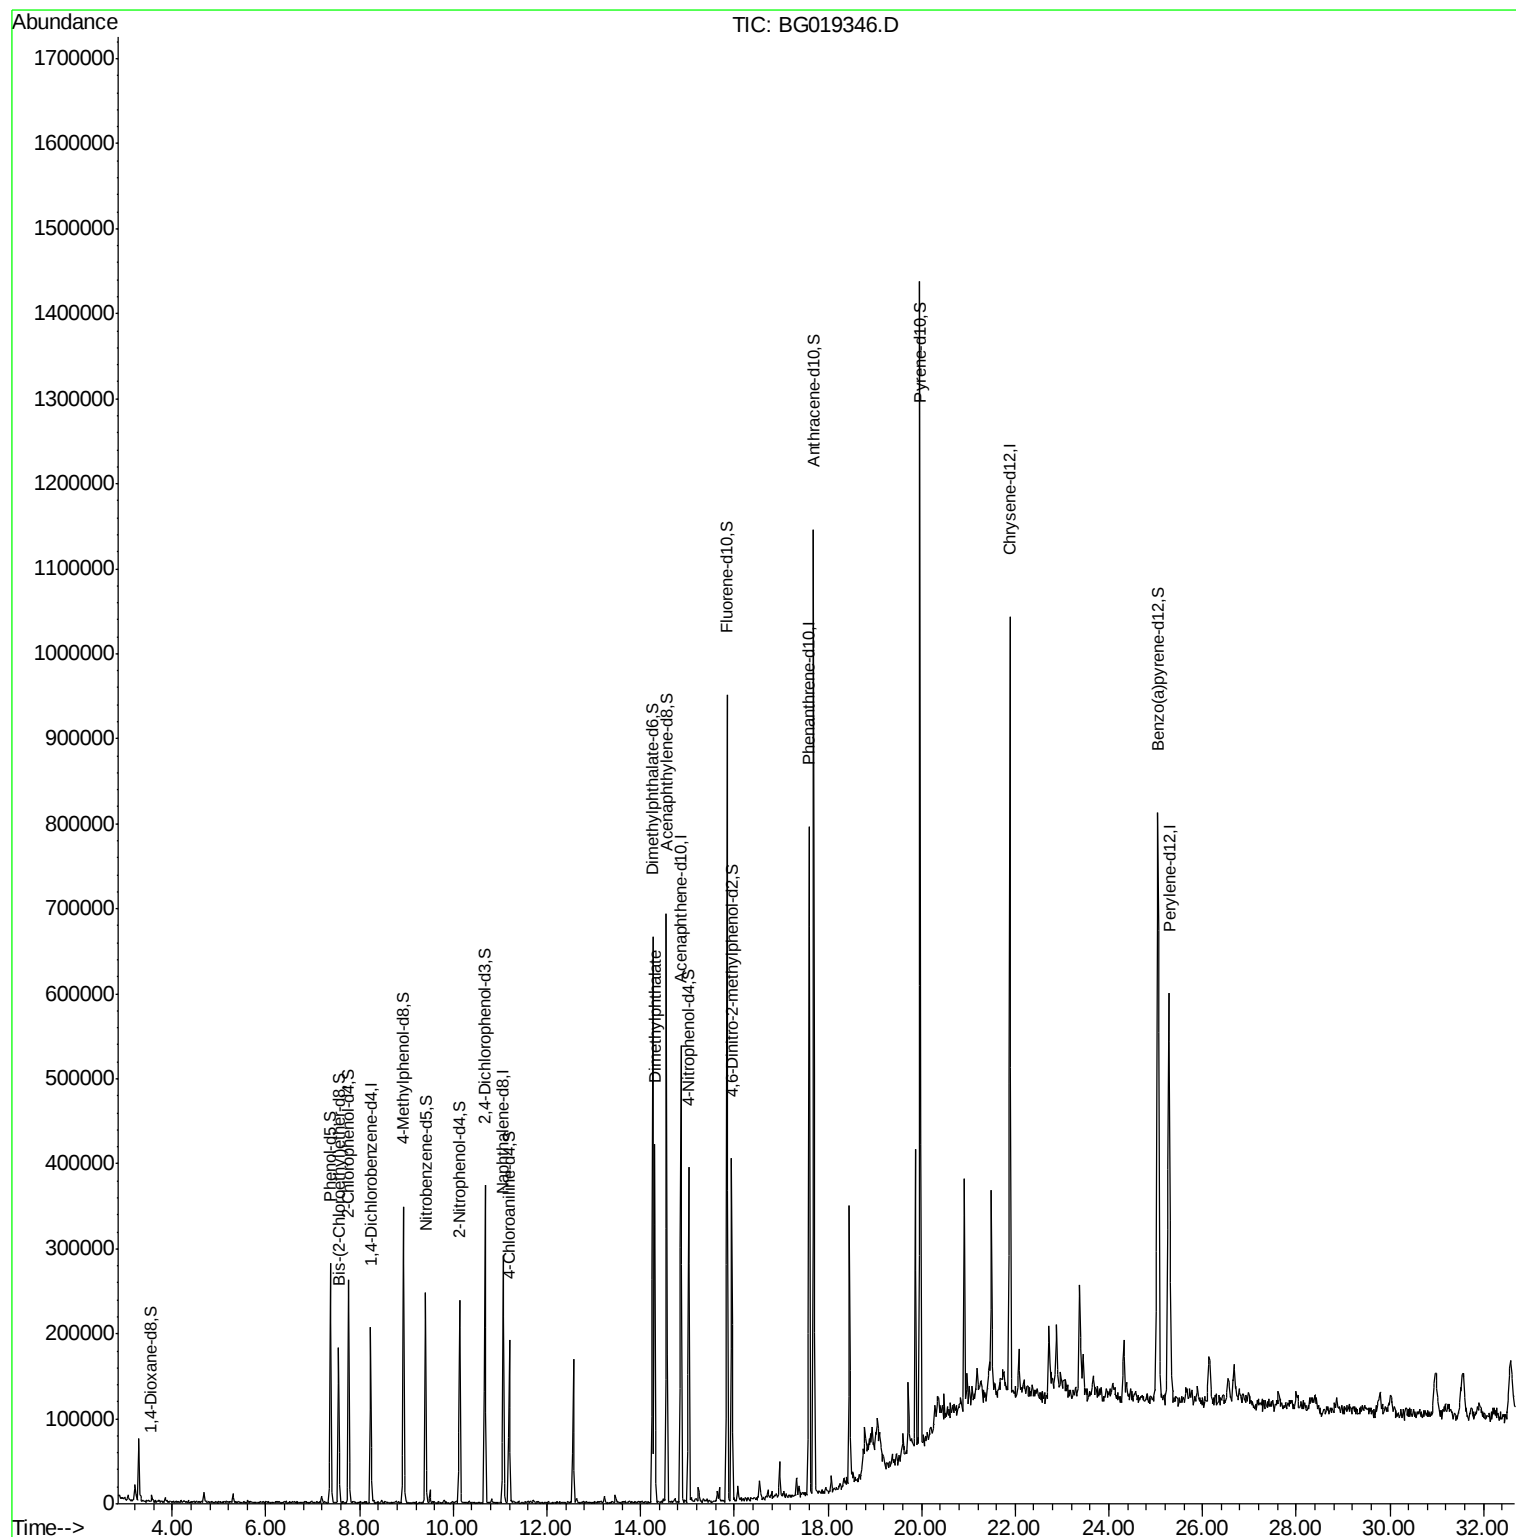

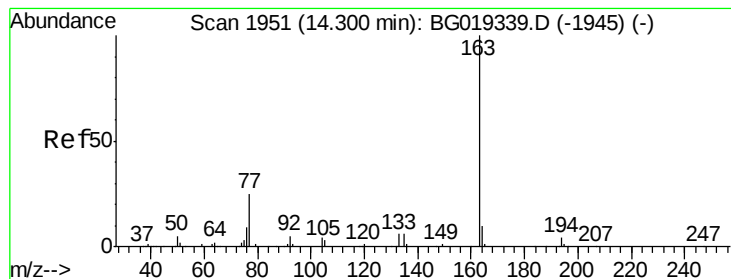

#45

Dimethylphthalate

Concen: 17.26 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. 0.00 min

Lab File: BG019346.D

Acq: 24 Oct 2015 21:38

Instrument :

BNA_G

ClientSampleId :

JG9H8


Tgt Ion:163 Resp: 250683

Ion Ratio Lower Upper

163 100

194 4.1 4.3 6.5#

164 10.9 7.5 11.3

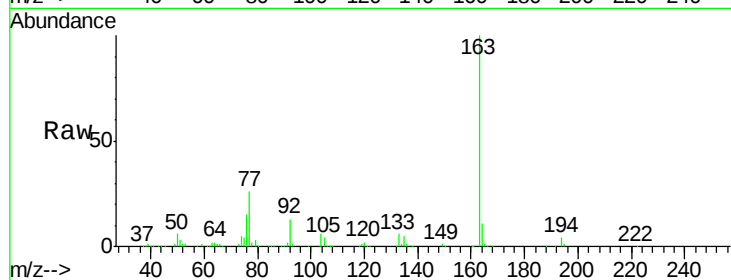

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

