

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
 Data File : BG019353.D
 Acq On : 25 Oct 2015 2:03
 Operator : UM/NP
 Sample : G4075-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9L1

Quant Time: Oct 25 03:32:27 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 03:28:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	87736	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	345316	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	257115	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	629868	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	716739	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	705108	20.00	ng/ul	0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.57	96	4777	3.02	ng/uL	0.00
5) Phenol-d5	7.39	99	163476	21.17	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.56	67	97961	21.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	101467	20.36	ng/ul	0.01
13) 4-Methylphenol-d8	8.95	113	118495	19.69	ng/ul	0.02
19) Nitrobenzene-d5	9.41	128	54193	20.67	ng/ul	0.00
22) 2-Nitrophenol-d4	10.15	143	63624	21.24	ng/ul	0.01
26) 2,4-Dichlorophenol-d3	10.69	165	137931	21.11	ng/ul	0.02
29) 4-Chloroaniline-d4	11.20	131	113848	17.54	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	429290	20.14	ng/ul	0.00
47) Acenaphthylene-d8	14.56	160	509094	21.58	ng/ul	0.01
52) 4-Nitrophenol-d4	15.04	143	66753	19.26	ng/ul	0.02
58) Fluorene-d10	15.85	176	403489	20.17	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	72908	17.58	ng/ul	0.00
71) Anthracene-d10	17.70	188	624020	21.64	ng/ul	0.00
79) Pyrene-d10	19.97	212	685278	21.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	756448	21.03	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.31	163	97892	4.60	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102315\
Data File : BG019353.D
Acq On : 25 Oct 2015 2:03
Operator : UM/NP
Sample : G4075-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9L1

Quant Time: Oct 25 03:32:27 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 03:28:11 2015
Response via : Initial Calibration

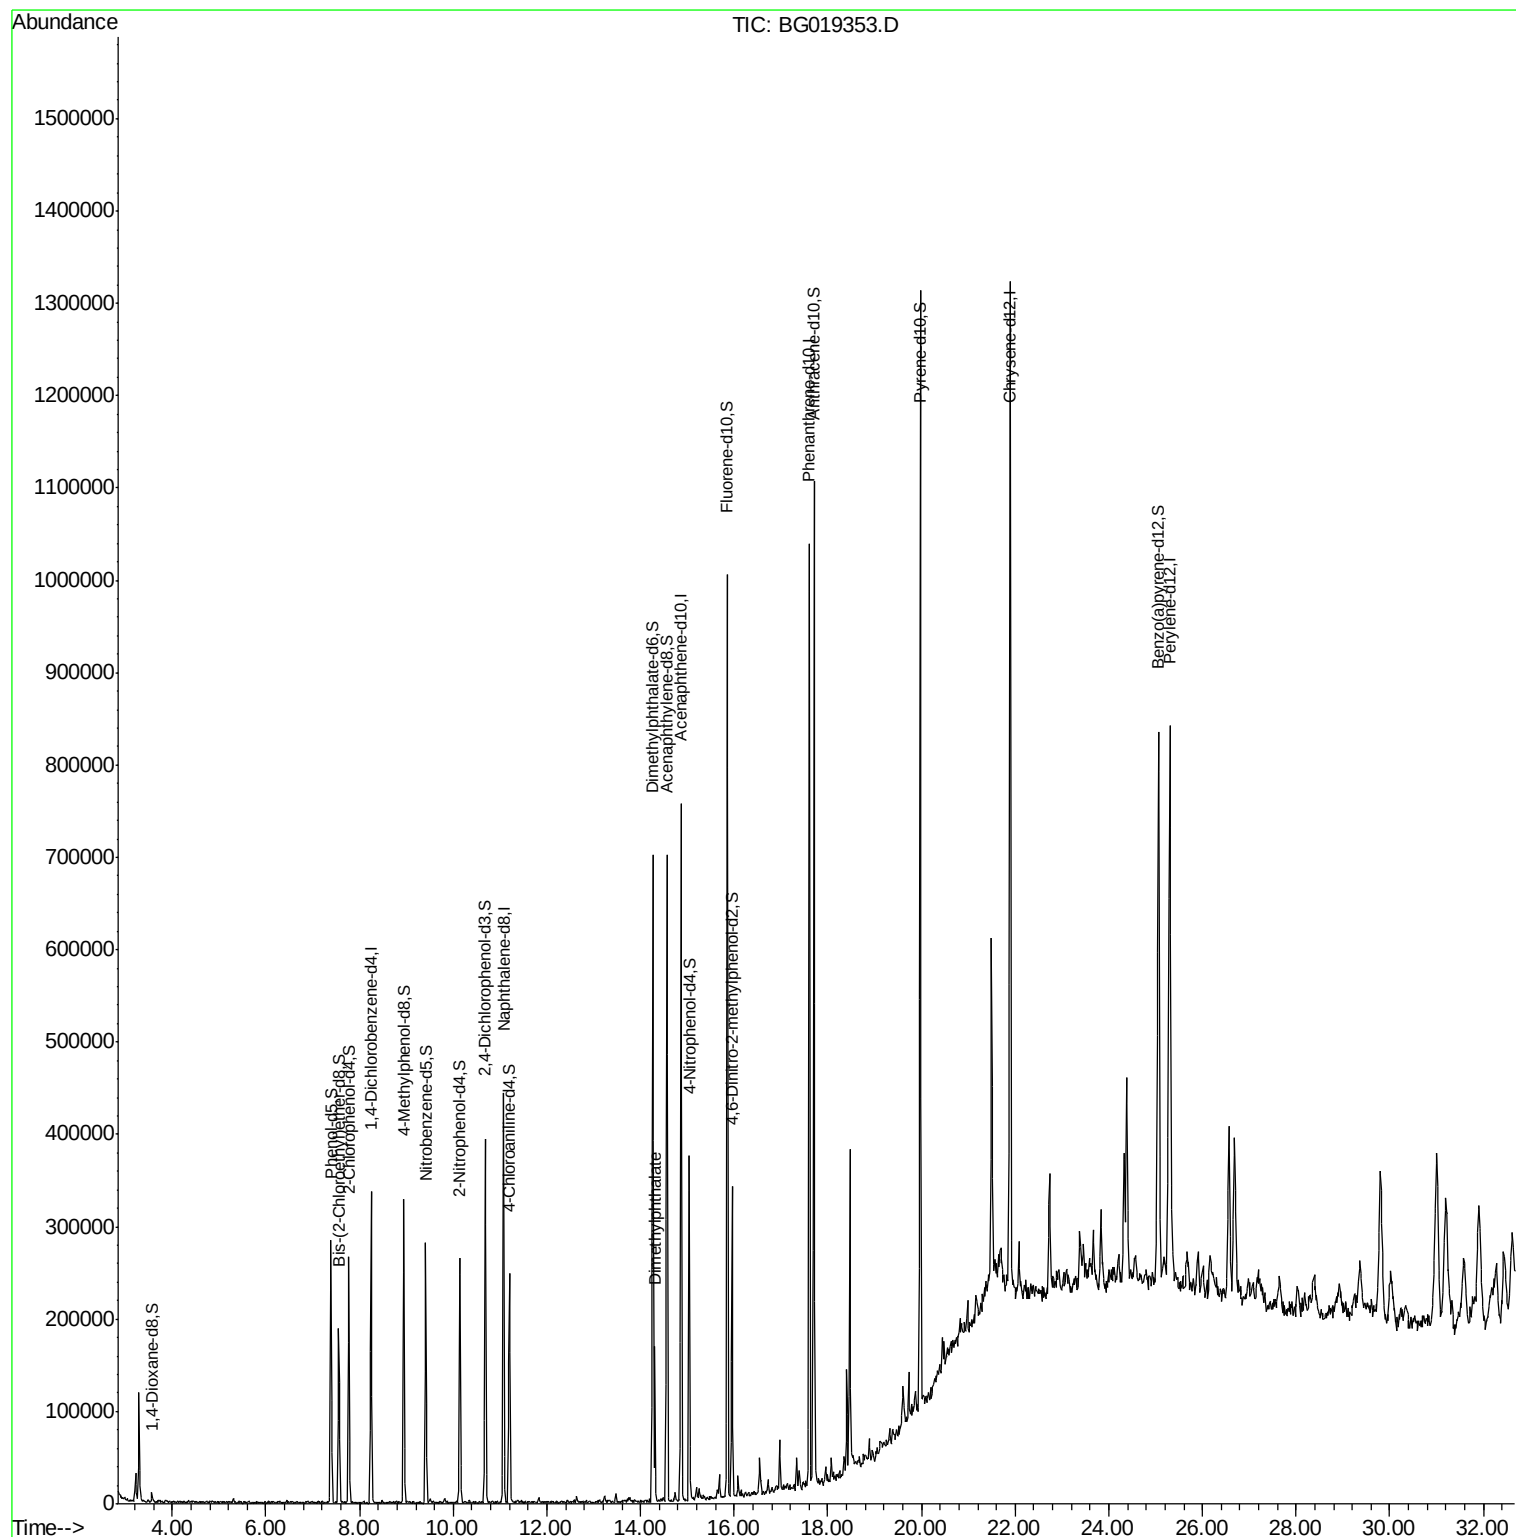

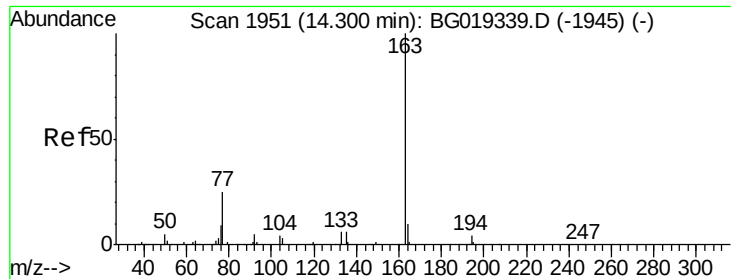

#45

Dimethylphthalate

Concen: 4.60 ng/ul

RT: 14.31 min Scan# 1952

Delta R.T. 0.01 min

Lab File: BG019353.D

Acq: 25 Oct 2015 2:03

Instrument :

BNA_G

ClientSampleId :

JG9L1


Tgt Ion:163 Resp: 97892

Ion Ratio Lower Upper

163 100

194 5.0 4.3 6.5

164 10.7 7.5 11.3

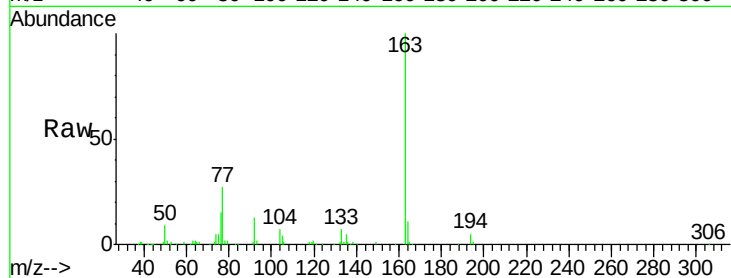

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

