

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
 Data File : BG019325.D
 Acq On : 24 Oct 2015 7:55
 Operator : UM/NP
 Sample : G4058-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LN9

Quant Time: Oct 25 01:28:05 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 01:11:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	29161	20.00	ng/ul	0.00
18) Naphthalene-d8	11.06	136	116594	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	97610	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.59	188	265687	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	379907	20.00	ng/ul	0.00
86) Perylene-d12	25.27	264	359810	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.57	96	2621	4.99	ng/uL	0.00
5) Phenol-d5	7.37	99	65131	25.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	41901	27.34	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	42058	25.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	51442	25.72	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	22327	25.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	26492	26.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	55059	24.96	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	60347	27.54	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	205240	25.36	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	224754	25.09	ng/ul	0.00
52) 4-Nitrophenol-d4	15.01	143	26250	19.95	ng/ul	0.00
58) Fluorene-d10	15.84	176	188993	24.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.94	200	36383	20.80	ng/ul	0.00
71) Anthracene-d10	17.69	188	322217	26.49	ng/ul	0.00
79) Pyrene-d10	19.96	212	423753	25.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.04	264	487760	26.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.30	163	128249	15.86	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
Data File : BG019325.D
Acq On : 24 Oct 2015 7:55
Operator : UM/NP
Sample : G4058-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LN9

Quant Time: Oct 25 01:28:05 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 01:11:12 2015
Response via : Initial Calibration

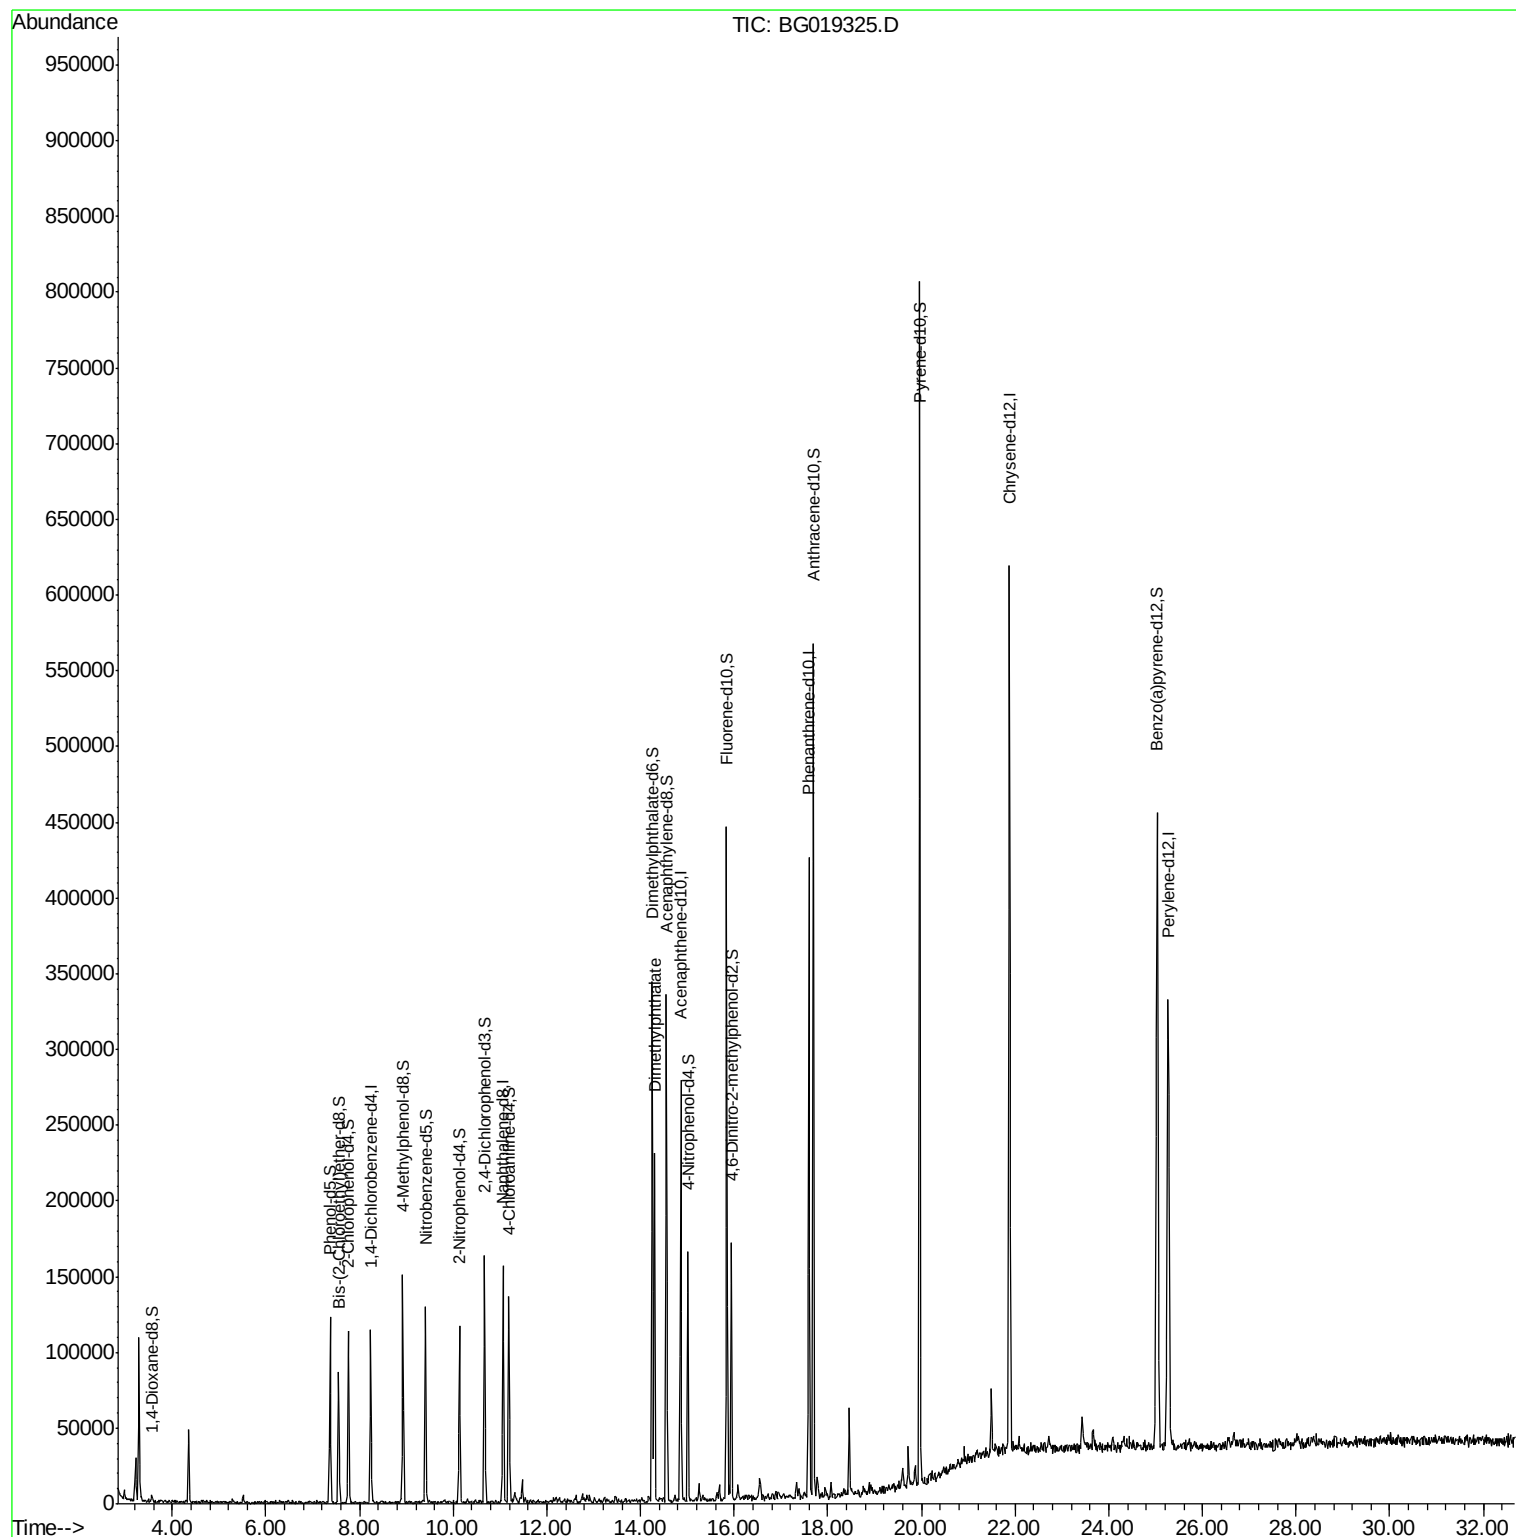

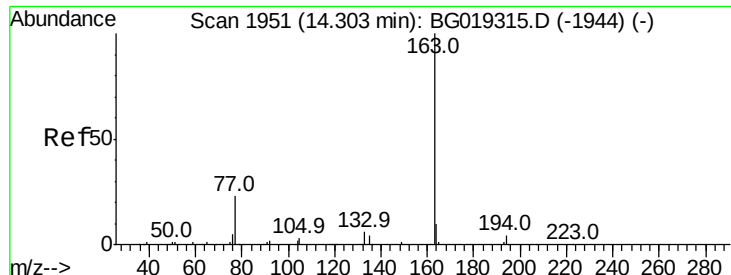

#45

Dimethylphthalate

Concen: 15.86 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. -0.00 min

Lab File: BG019325.D

Acq: 24 Oct 2015 7:55

Instrument :

BNA_G

ClientSampleId :

E5LN9


Tot Ion:163 Resp: 128249

Ion Ratio Lower Upper

163 100

194 3.7 4.3 6.5#

164 10.2 7.5 11.3

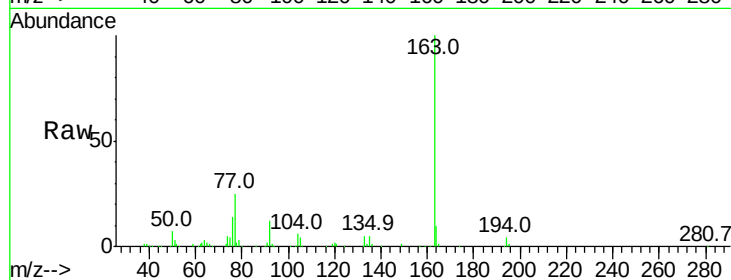

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

