

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
 Data File : BG019328.D
 Acq On : 24 Oct 2015 9:49
 Operator : UM/NP
 Sample : G4075-09
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K9

Quant Time: Oct 25 02:39:26 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 02:37:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	49008	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	195607	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	151936	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	409937	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	513653	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	490740	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.57	96	3139	3.56	ng/uL	0.00
5) Phenol-d5	7.37	99	84074	19.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.56	67	52576	20.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	53227	19.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	66813	19.87	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	28641	19.28	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	33053	19.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	71711	19.38	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	74832	20.36	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	245390	19.48	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	288187	20.67	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	40594	19.82	ng/ul	0.00
58) Fluorene-d10	15.85	176	226641	19.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.94	200	46672	17.29	ng/ul	0.00
71) Anthracene-d10	17.69	188	376355	20.05	ng/ul	0.00
79) Pyrene-d10	19.96	212	453794	20.16	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.04	264	512660	20.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.30	163	70520	5.60	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
Data File : BG019328.D
Acq On : 24 Oct 2015 9:49
Operator : UM/NP
Sample : G4075-09
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K9

Quant Time: Oct 25 02:39:26 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 02:37:52 2015
Response via : Initial Calibration

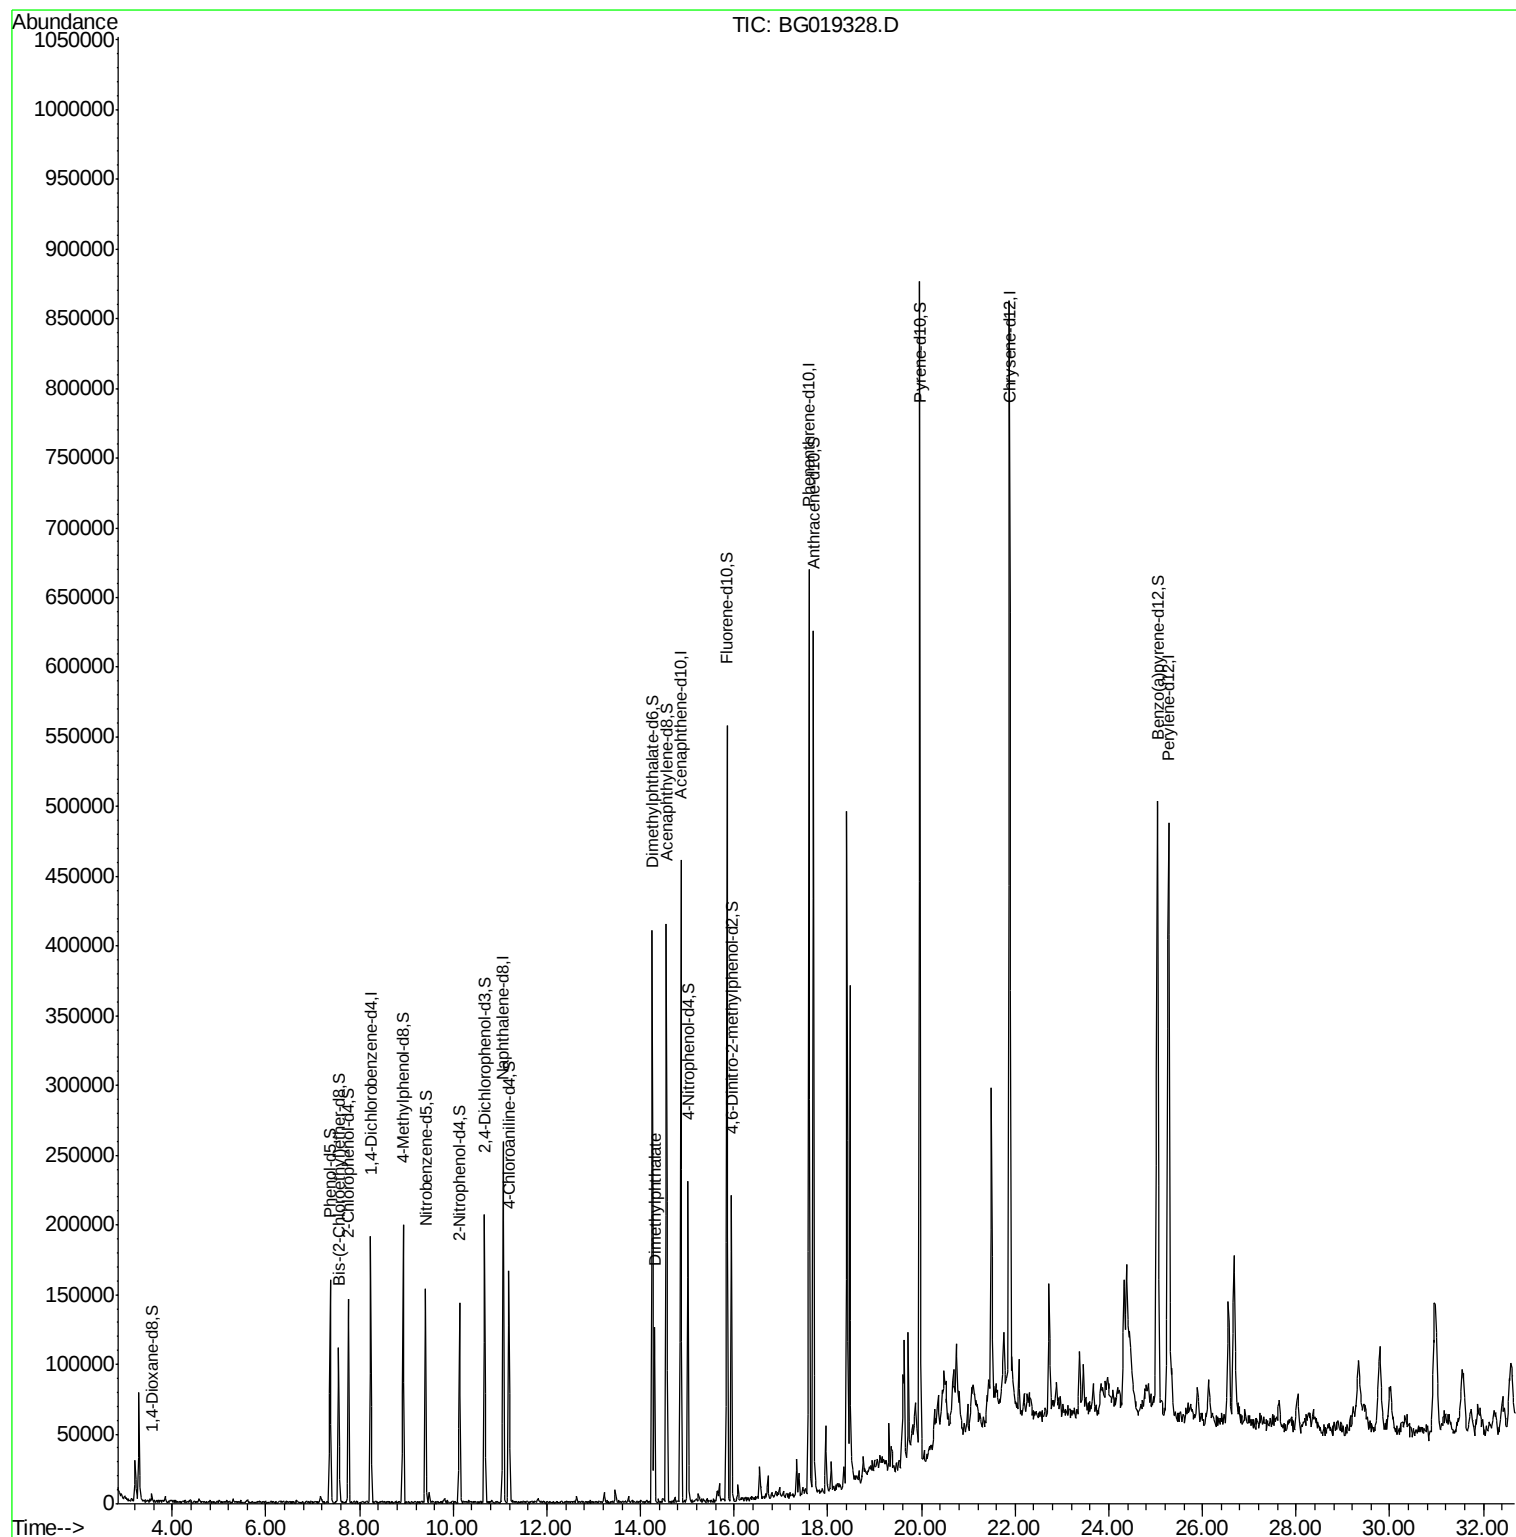

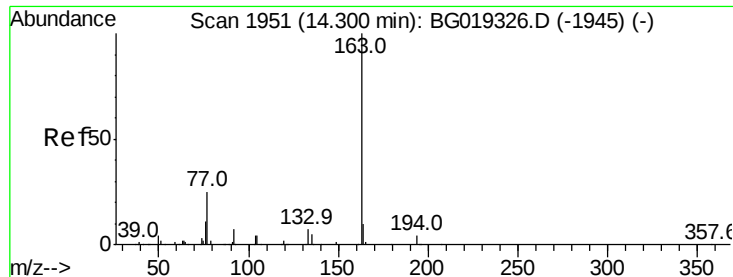

#45

Dimethylphthalate

Concen: 5.60 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. 0.00 min

Lab File: BG019328.D

Acq: 24 Oct 2015 9:49

Instrument :

BNA_G

ClientSampleId :

JG9K9


Tot Ion:163 Resp: 70520

Ion Ratio Lower Upper

163 100

194 4.4 4.3 6.5

164 10.7 7.5 11.3

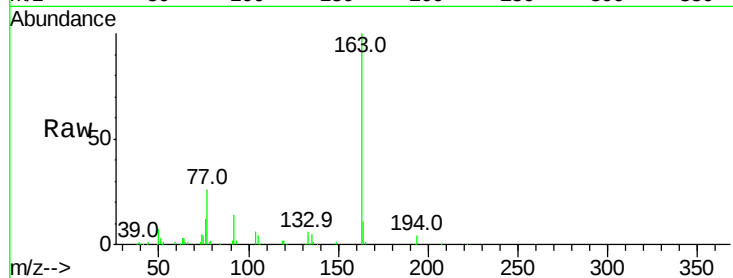

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

