

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
 Data File : BG019329.D
 Acq On : 24 Oct 2015 10:27
 Operator : UM/NP
 Sample : G4075-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H9

Quant Time: Oct 25 02:39:36 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 02:37:52 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	55975	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	226916	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	177006	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	473200	20.00	ng/ul	0.00
78) Chrysene-d12	21.88	240	601917	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	581158	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.57	96	5644	5.60	ng/uL	0.00
5) Phenol-d5	7.37	99	156870	31.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	98985	33.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	98420	30.96	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	128030	33.34	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	54377	31.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	63834	32.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	136005	31.68	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	144202	33.82	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	487254	33.20	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	522466	32.17	ng/ul	0.00
52) 4-Nitrophenol-d4	15.02	143	76796	32.18	ng/ul	0.00
58) Fluorene-d10	15.85	176	433080	31.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	99645	31.99	ng/ul	0.00
71) Anthracene-d10	17.70	188	736895	34.01	ng/ul	0.00
79) Pyrene-d10	19.96	212	899267	34.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	1007692	33.99	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.30	163	247073	16.85	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
Data File : BG019329.D
Acq On : 24 Oct 2015 10:27
Operator : UM/NP
Sample : G4075-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H9

Quant Time: Oct 25 02:39:36 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 02:37:52 2015
Response via : Initial Calibration

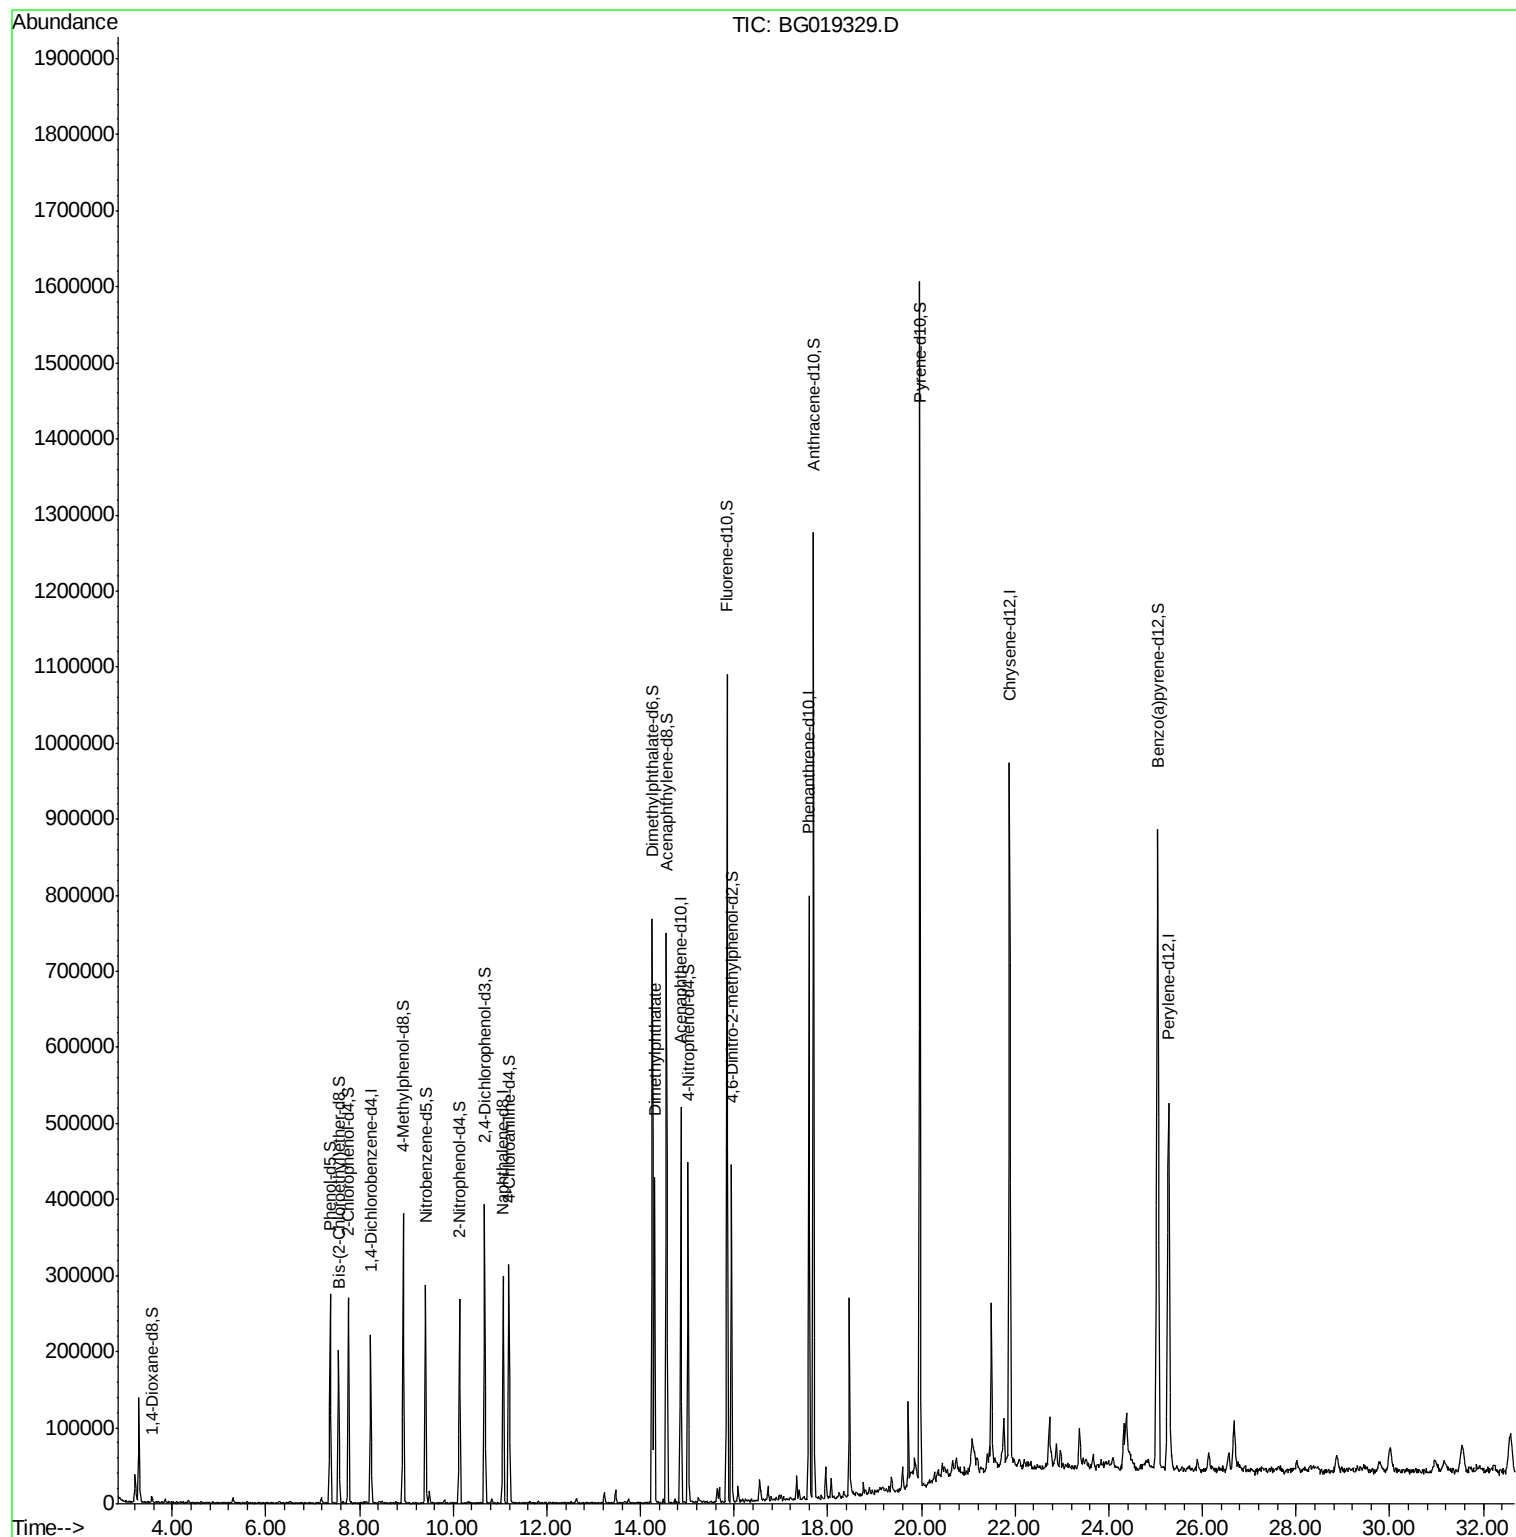

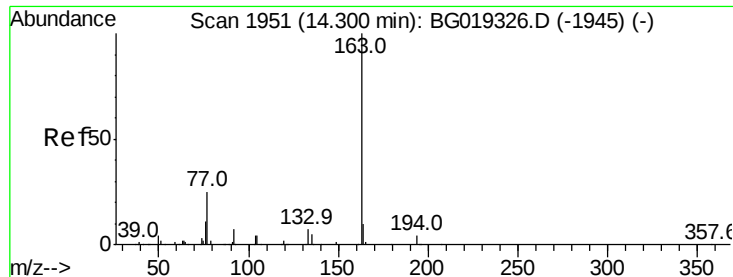

#45

Dimethylphthalate

Concen: 16.85 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. 0.00 min

Lab File: BG019329.D

Acq: 24 Oct 2015 10:27

Instrument :

BNA_G

ClientSampleId :

JG9H9


Tot Ion:163 Resp: 247073

Ion Ratio Lower Upper

163 100

194 4.3 4.3 6.5#

164 9.5 7.5 11.3

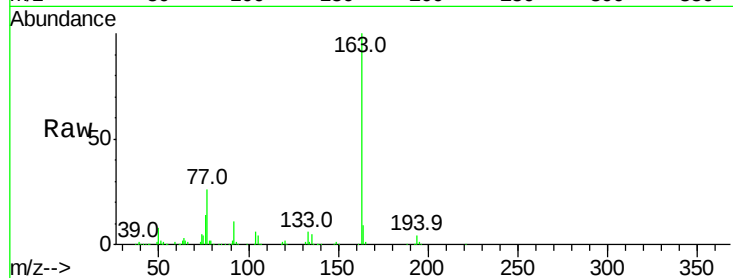

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

