

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
 Data File : BG019351.D
 Acq On : 25 Oct 2015 00:48
 Operator : UM/NP
 Sample : G4075-07
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9K7

Quant Time: Oct 25 03:32:09 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 25 03:28:11 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	102709	20.00	ng/ul	0.00
18) Naphthalene-d8	11.07	136	408845	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	309840	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	741329	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	875406	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	840549	20.00	ng/ul	0.03

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.57	96	4676	2.53	ng/uL	0.00
5) Phenol-d5	7.38	99	165922	18.36	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.56	67	98604	18.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.77	132	105513	18.09	ng/ul	0.01
13) 4-Methylphenol-d8	8.94	113	132718	18.84	ng/ul	0.01
19) Nitrobenzene-d5	9.41	128	52765	16.99	ng/ul	0.00
22) 2-Nitrophenol-d4	10.14	143	65869	18.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	141678	18.32	ng/ul	0.01
29) 4-Chloroaniline-d4	11.20	131	117099	15.24	ng/ul	0.00
44) Dimethylphthalate-d6	14.26	166	447414	17.42	ng/ul	0.00
47) Acenaphthylene-d8	14.56	160	521440	18.34	ng/ul	0.00
52) 4-Nitrophenol-d4	15.04	143	67305	16.11	ng/ul	0.02
58) Fluorene-d10	15.85	176	411067	17.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	79294	16.25	ng/ul	0.00
71) Anthracene-d10	17.70	188	644953	19.00	ng/ul	0.00
79) Pyrene-d10	19.97	212	701601	18.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	786799	18.35	ng/ul	0.02


Target Compounds					Ovalue
45) Dimethylphthalate	14.31	163	135311	5.27 ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102315\
Data File : BG019351.D
Acq On : 25 Oct 2015 00:48
Operator : UM/NP
Sample : G4075-07
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9K7

Quant Time: Oct 25 03:32:09 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 25 03:28:11 2015
Response via : Initial Calibration

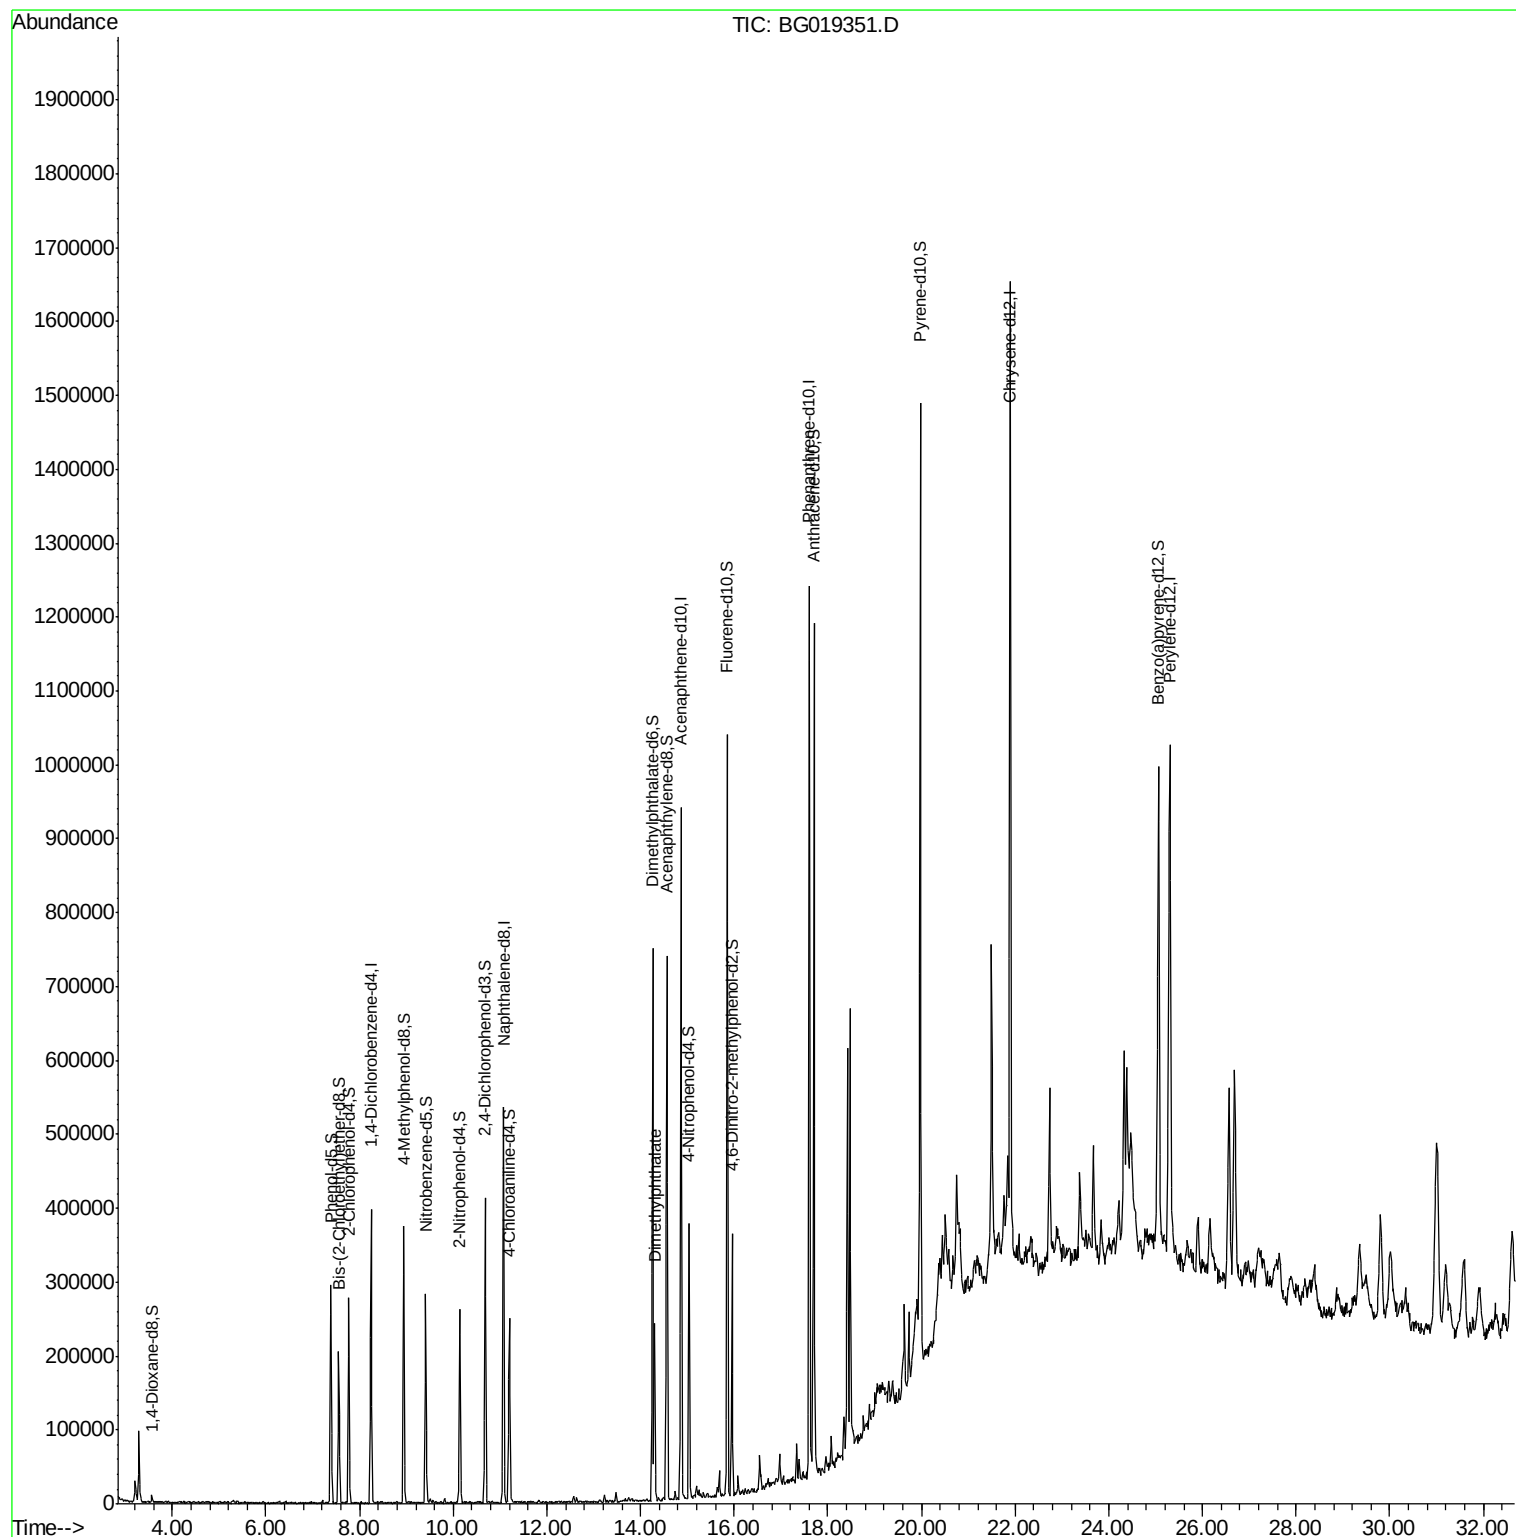

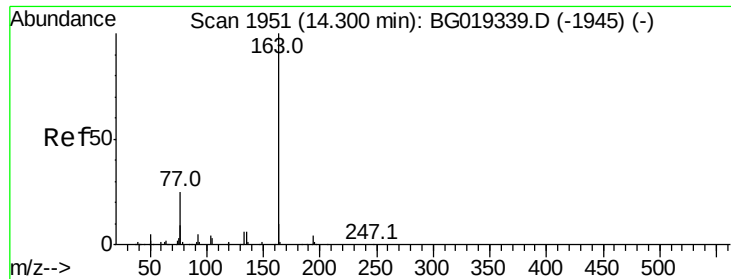

#45

Dimethylphthalate

Concen: 5.27 ng/ul

RT: 14.31 min Scan# 1952

Delta R.T. 0.01 min

Lab File: BG019351.D

Acq: 25 Oct 2015 00:48

Instrument :

BNA_G

ClientSampleId :

JG9K7


Tot Ion:163 Resp: 135311

Ion Ratio Lower Upper

163 100

194 4.7 4.3 6.5

164 10.9 7.5 11.3

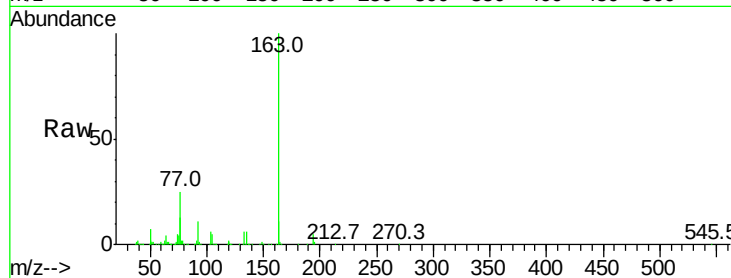

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

