
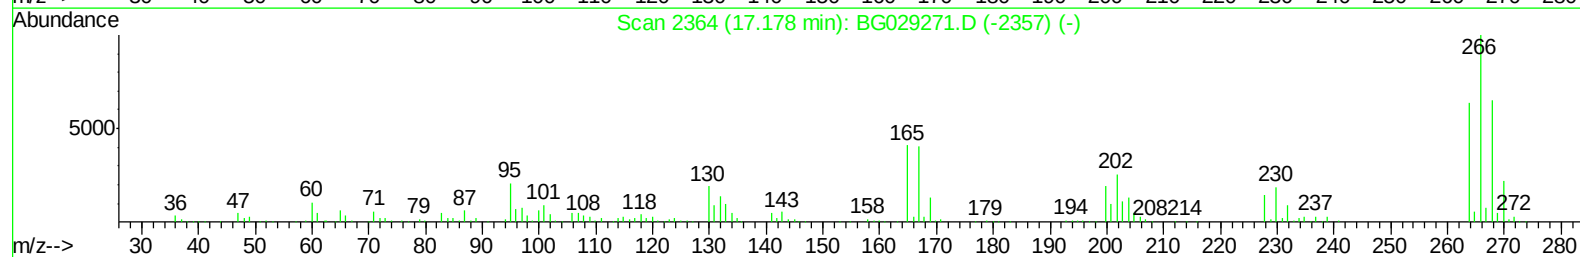
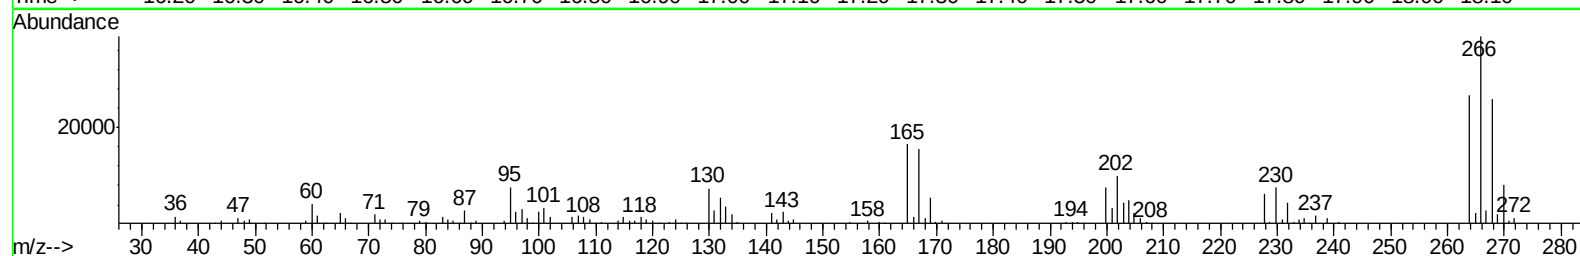


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102317\
Data File : BG029400.D
Acq On : 23 Oct 2017 15:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 07:30:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

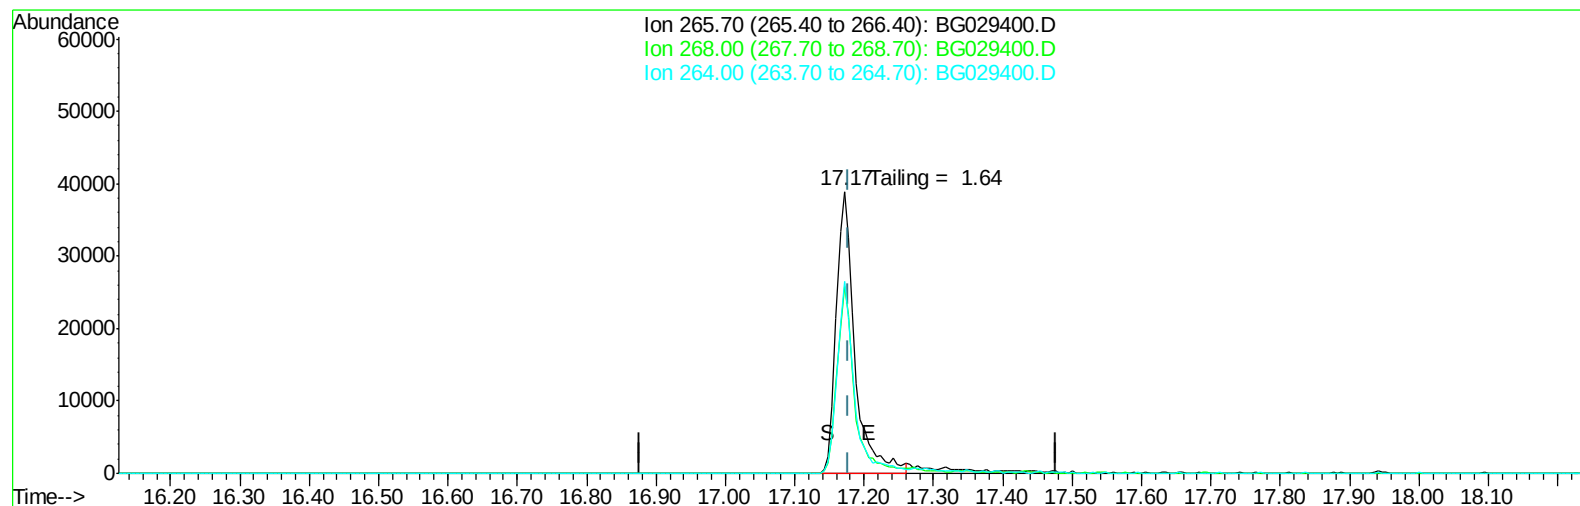

TIC: BG029400.D

(69) Pentachlorophenol (C)




17.171min (-0.006) 0.00ng

response 71042

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.28
264.00	62.00	68.38
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102317\
Data File : BG029400.D
Acq On : 23 Oct 2017 15:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 07:30:48 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

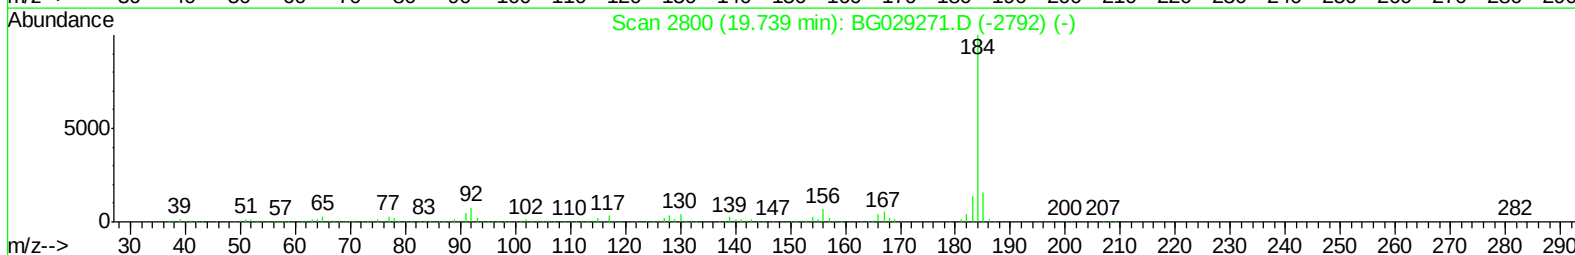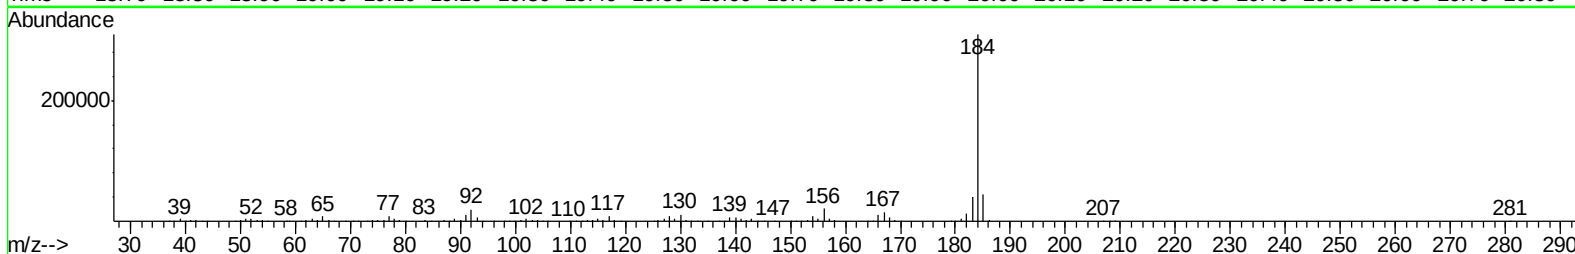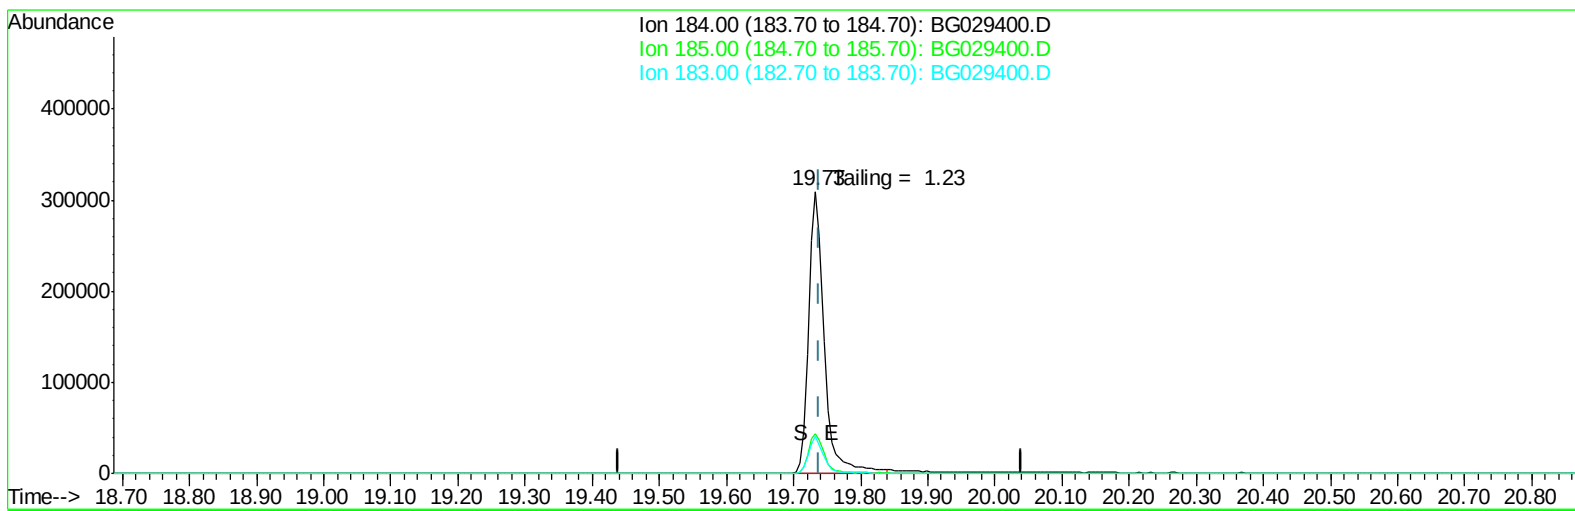

TIC: BG029400.D

(76) Benzidine

19.733min (-0.006) 0.00ng

response 493644

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.24
183.00	13.30	13.36
0.00	0.00	0.00