

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102317\
 Data File : BG029410.D
 Acq On : 23 Oct 2017 22:11
 Operator : SJ/JU
 Sample : I6028-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 15-40-RT4651

Quant Time: Oct 24 05:54:20 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 16 17:32:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	62493	20.00	ng	0.00
21) Naphthalene-d8	10.98	136	273334	20.00	ng	0.00
38) Acenaphthene-d10	14.78	164	183232	20.00	ng	-0.01
63) Phenanthrene-d10	17.52	188	504096	20.00	ng	-0.01
75) Chrysene-d12	21.79	240	586059	20.00	ng	-0.01
86) Perylene-d12	25.10	264	574765	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	485193	129.70	ng	0.00
7) Phenol-d6	7.32	99	588455	112.07	ng	0.00
23) Nitrobenzene-d5	9.33	82	401953	93.45	ng	0.00
41) 2,4,6-Tribromophenol	16.27	330	372894	157.62	ng	0.00
44) 2-Fluorobiphenyl	13.41	172	1070434	85.68	ng	0.00
78) Terphenyl-d14	20.11	244	2035489	79.01	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102317\
Data File : BG029410.D
Acq On : 23 Oct 2017 22:11
Operator : SJ/JU
Sample : I6028-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
15-40-RT4651

Quant Time: Oct 24 05:54:20 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101617.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 16 17:32:15 2017
Response via : Initial Calibration

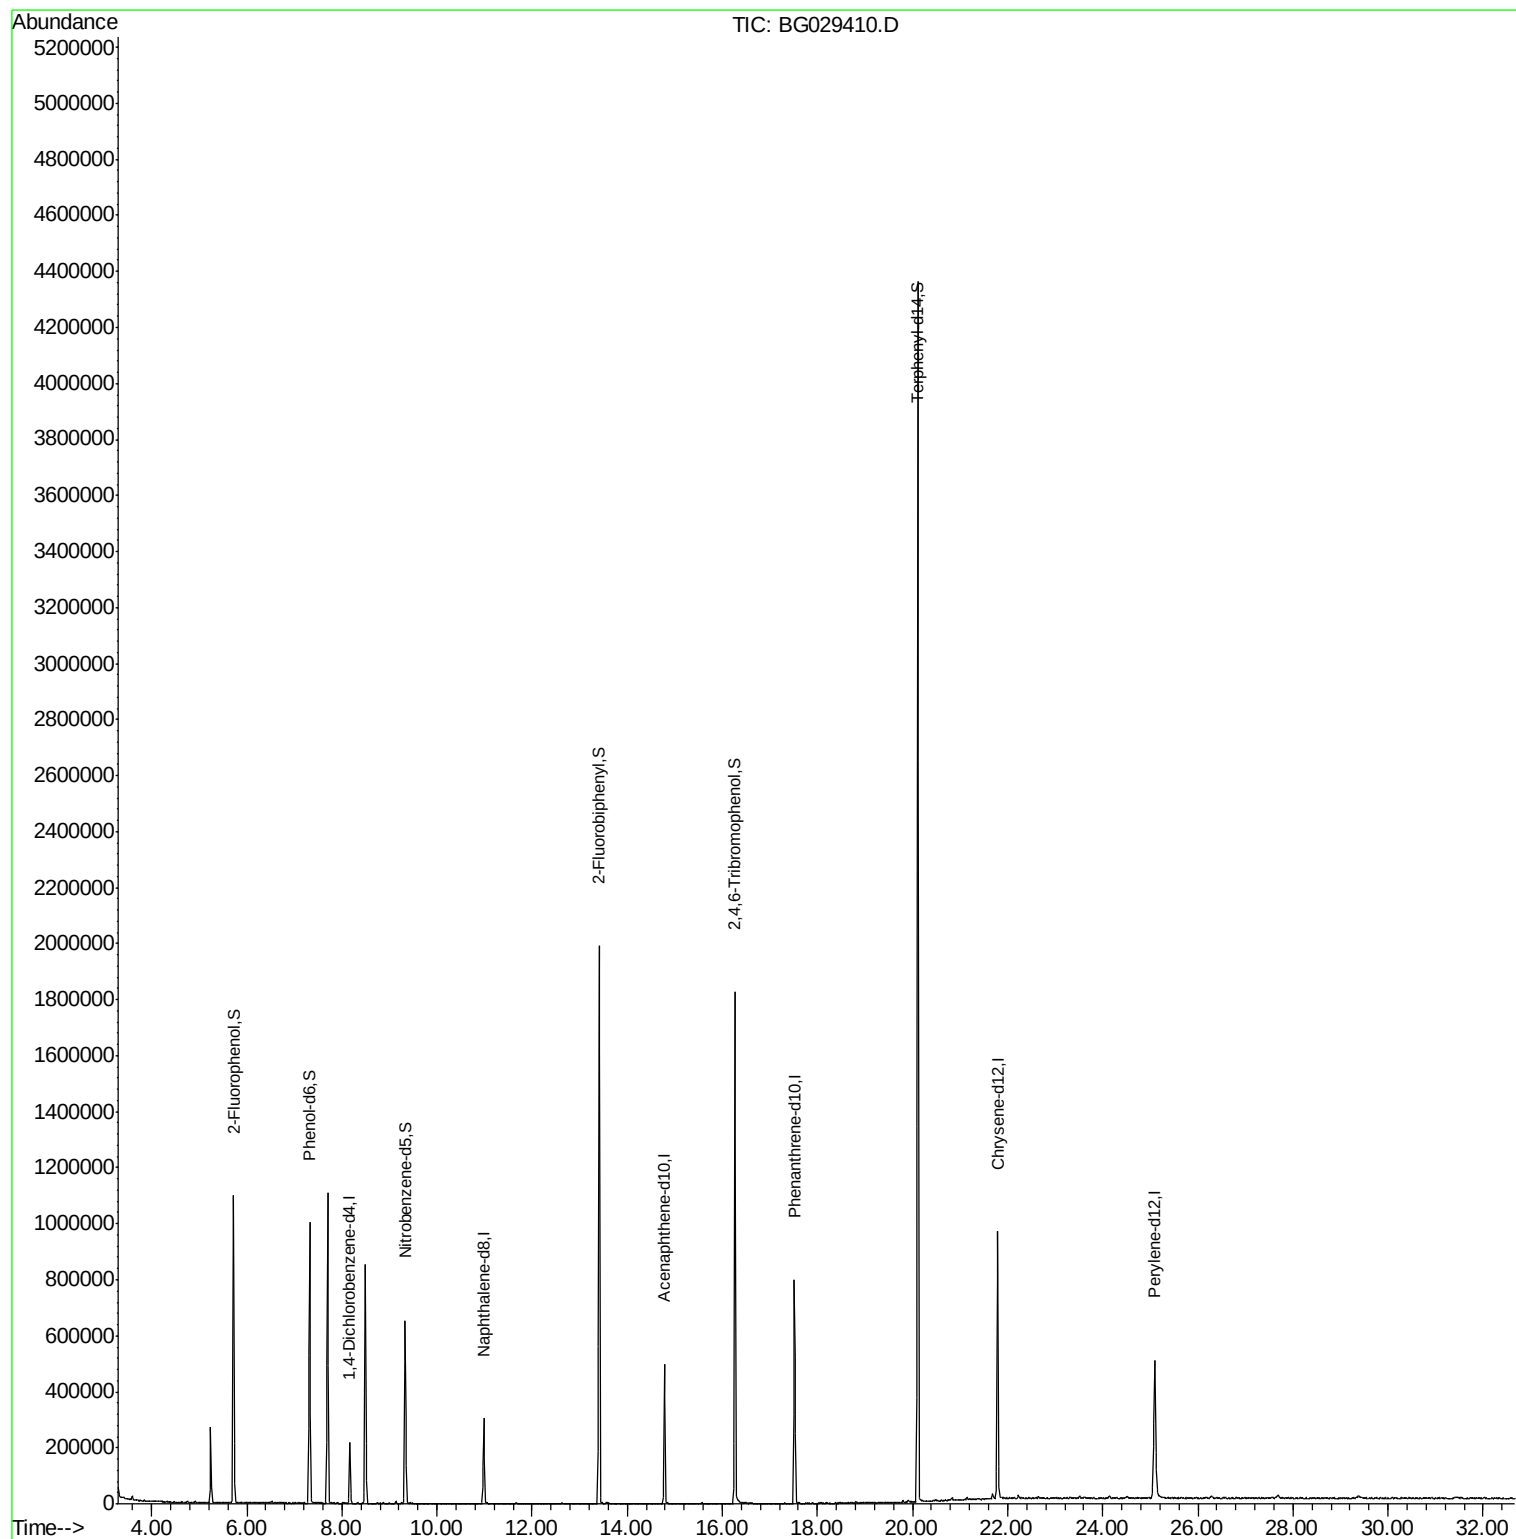

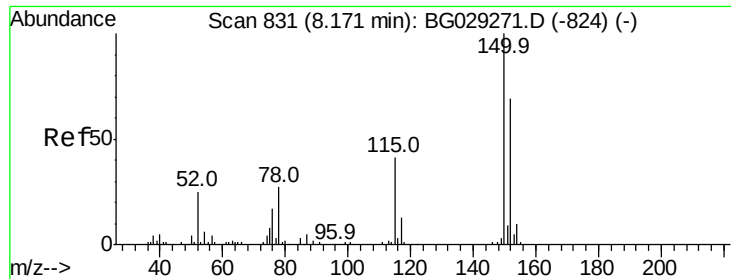


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.16 min Scan# 830
Delta R.T. -0.01 min
Lab File: BG029410.D
Acq: 23 Oct 2017 22:11

Instrument :
BNA_G
ClientSampleId :
15-40-RT4651

Tot Ion:152 Resp: 62493
Ion Ratio Lower Upper
152 100
150 157.9 126.6 189.8
115 61.4 53.0 79.4

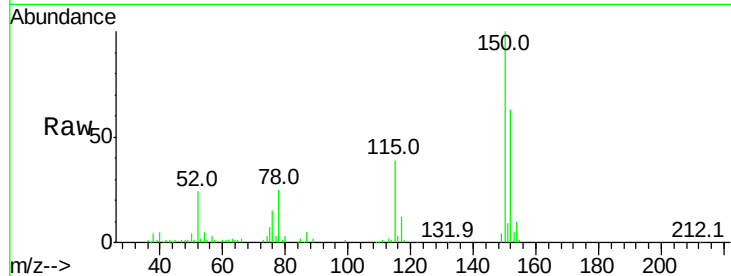


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

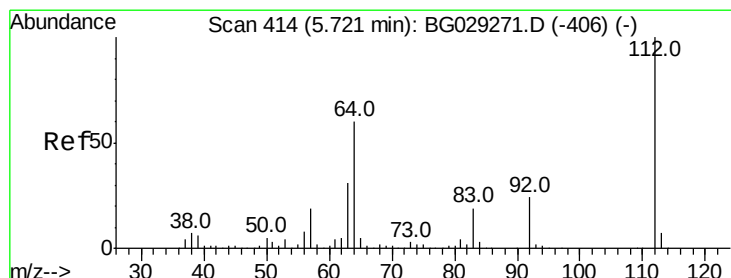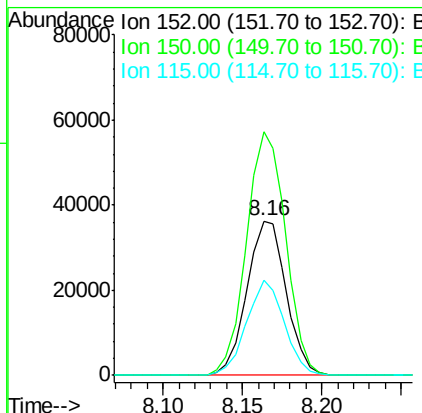



#5


2-Fluorophenol
Concen: 129.701 ng
RT: 5.72 min Scan# 414
Delta R.T. -0.00 min
Lab File: BG029410.D
Acq: 23 Oct 2017 22:11

Tgt Ion:112 Resp: 485193
Ion Ratio Lower Upper
112 100
64 61.3 56.3 84.5
63 31.4 30.1 45.1

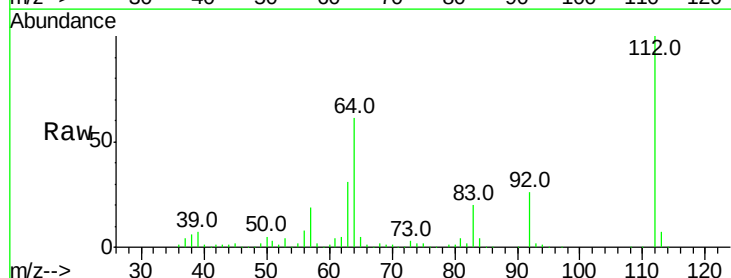

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

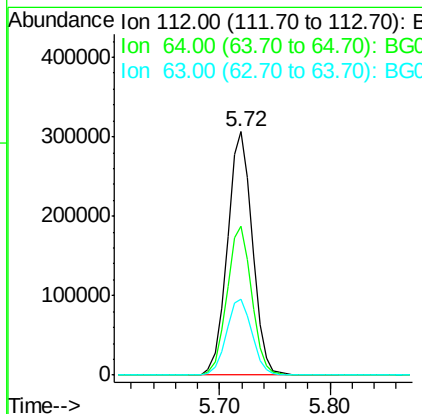

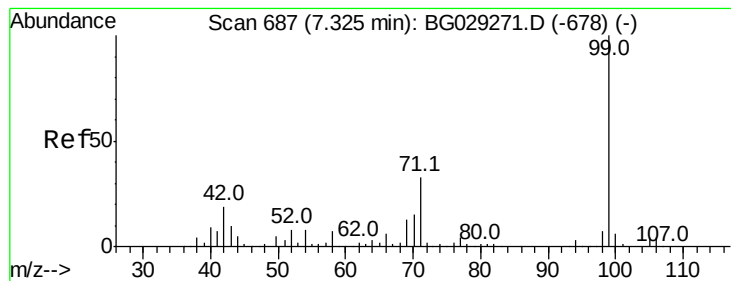

#7

Phenol-d6

Concen: 112.068 ng

RT: 7.32 min Scan# 686

Delta R.T. -0.01 min

Lab File: BG029410.D

Acq: 23 Oct 2017 22:11

Instrument :

BNA_G

ClientSampleId :

15-40-RT4651


Tot Ion: 99 Resp: 588455

Ion Ratio Lower Upper




99 100

42 19.3 14.1 21.1

71 34.3 26.1 39.1

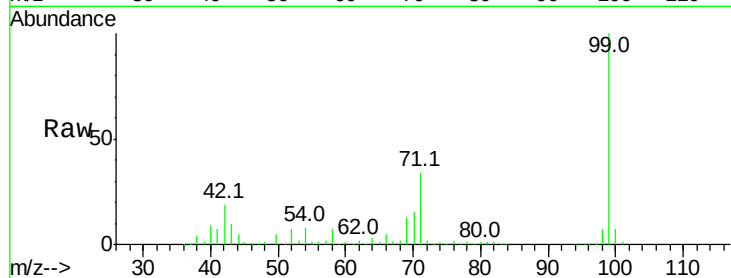

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

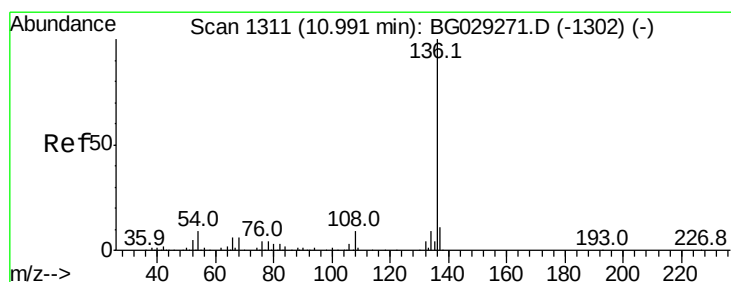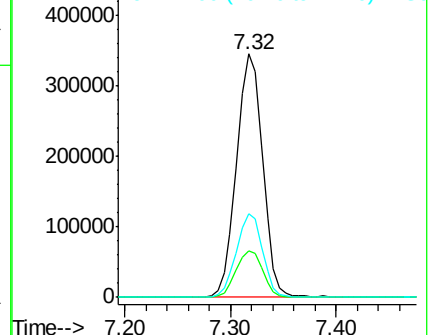

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.98 min Scan# 1310

Delta R.T. -0.01 min

Lab File: BG029410.D

Acq: 23 Oct 2017 22:11

Tgt Ion: 136 Resp: 273334


Ion Ratio Lower Upper

136 100



137 11.0 9.2 13.8


54 8.4 10.3 15.5#

68 5.8 4.5 6.7

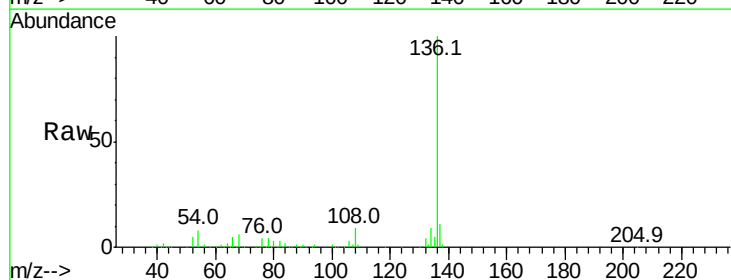

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



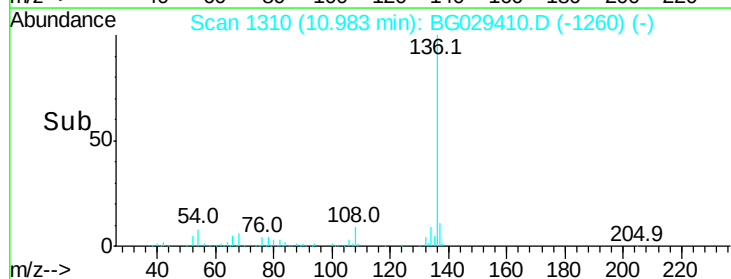
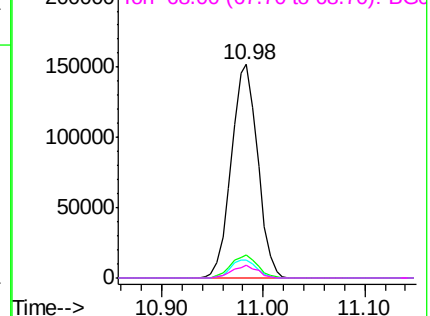


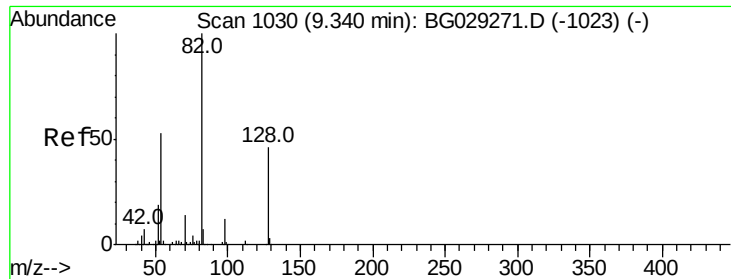

#23
 Nitrobenzene-d5
 Concen: 93.450 ng
 RT: 9.33 min Scan# 1029
 Delta R.T. -0.01 min
 Lab File: BG029410.D
 Acq: 23 Oct 2017 22:11




Instrument :
 BNA_G
 ClientSampleId :
 15-40-RT4651


Tot Ion	Ratio	Lower	Upper
82	100		
128	45.5	29.7	44.5#
54	52.1	43.1	64.7

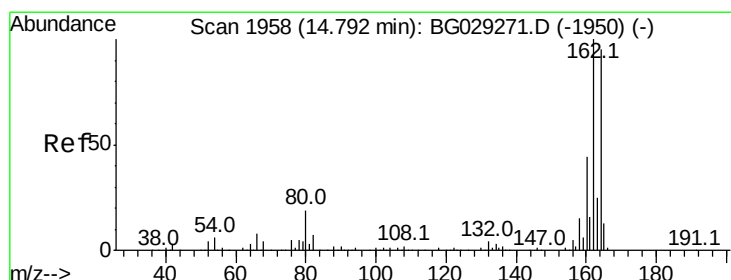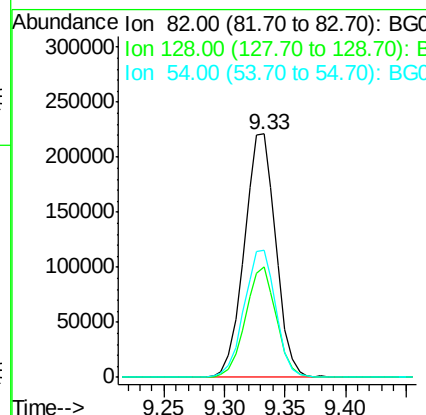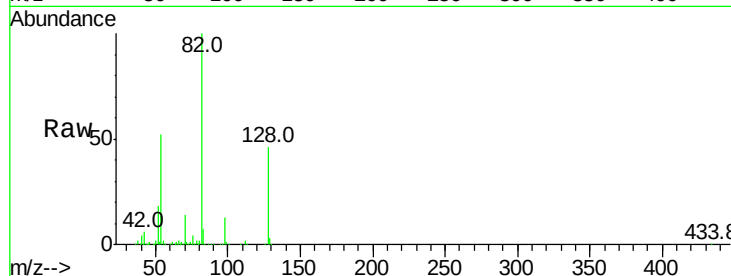

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.78 min Scan# 1956
 Delta R.T. -0.01 min
 Lab File: BG029410.D
 Acq: 23 Oct 2017 22:11

Tgt Ion	Ratio	Lower	Upper
164	100		
162	98.3	78.8	118.2
160	44.0	35.4	53.0

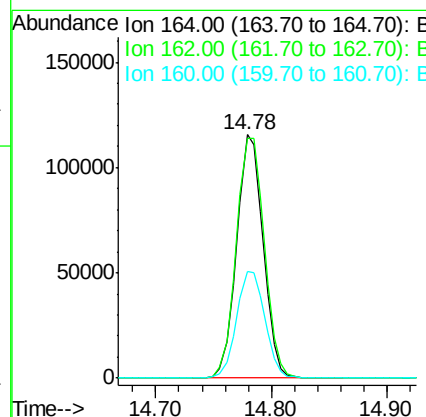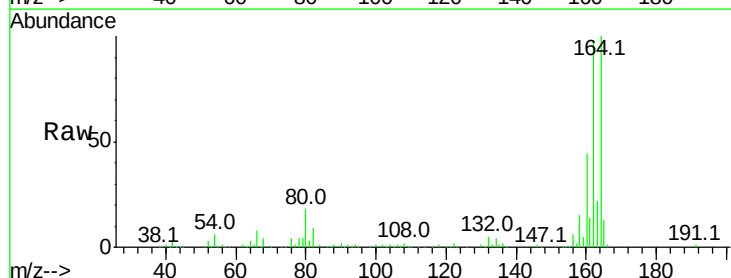







#41
 2,4,6-Tribromophenol
 Concen: 157.624 ng
 RT: 16.27 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: BG029410.D
 Acq: 23 Oct 2017 22:11

Instrument :
 BNA_G
 ClientSampleId :
 15-40-RT4651

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.0	115.6
141	34.1	25.2	37.8

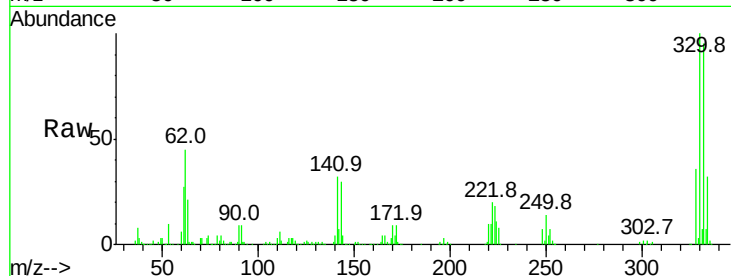


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

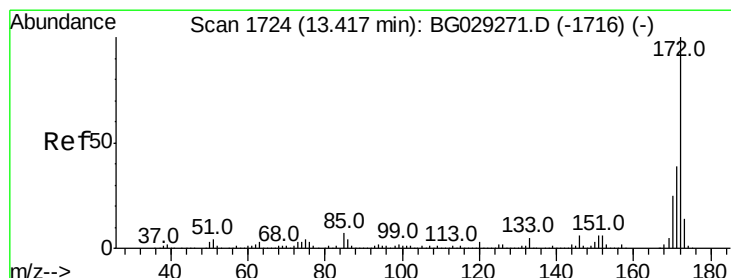
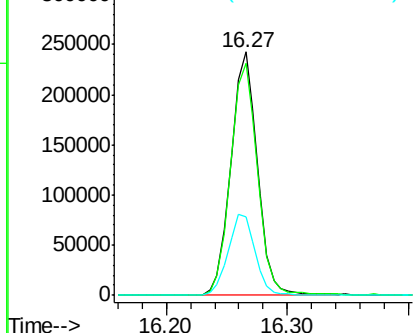



#44
 2-Fluorobiphenyl
 Concen: 85.681 ng
 RT: 13.41 min Scan# 1723
 Delta R.T. -0.01 min
 Lab File: BG029410.D
 Acq: 23 Oct 2017 22:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.3	30.0	45.0
170	24.6	19.5	29.3

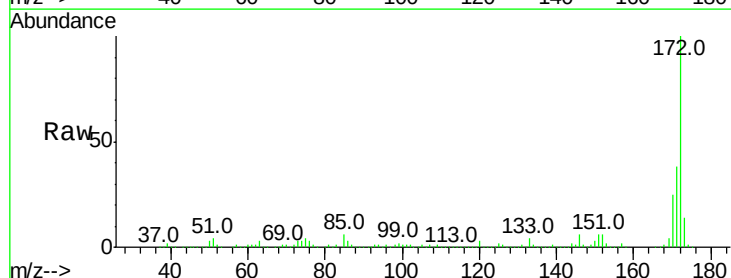

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E




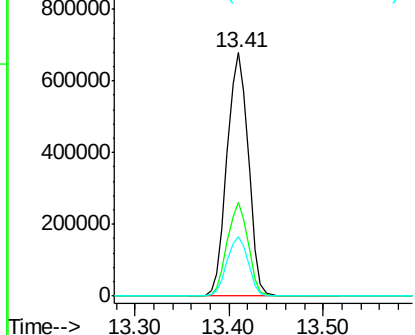


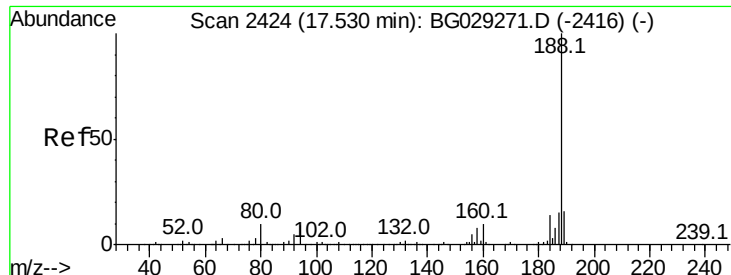

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.52 min Scan# 2422
Delta R.T. -0.01 min
Lab File: BG029410.D
Acq: 23 Oct 2017 22:11




Instrument :
BNA_G
ClientSampleId :
15-40-RT4651


Tot Ion:188 Resp: 504096
Ion Ratio Lower Upper
188 100
94 8.1 6.9 10.3
80 8.8 7.7 11.5

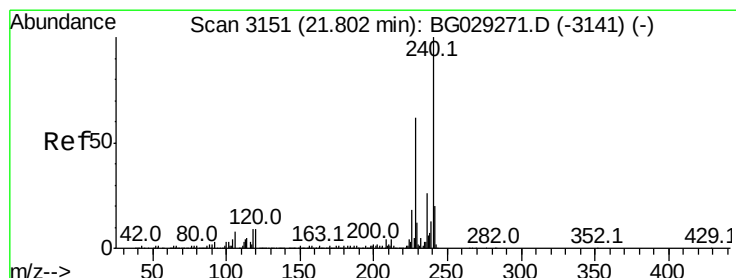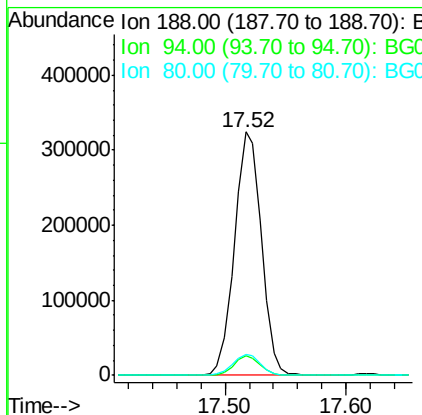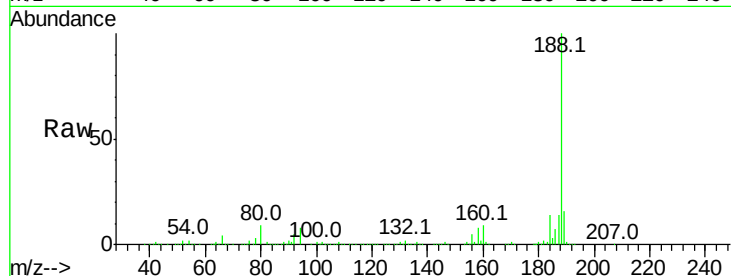

#75
Chrysene-d12
Concen: 20.000 ng
RT: 21.79 min Scan# 3149
Delta R.T. -0.01 min
Lab File: BG029410.D
Acq: 23 Oct 2017 22:11

Tgt Ion:240 Resp: 586059
Ion Ratio Lower Upper
240 100
120 8.5 6.8 10.2
236 26.0 20.9 31.3

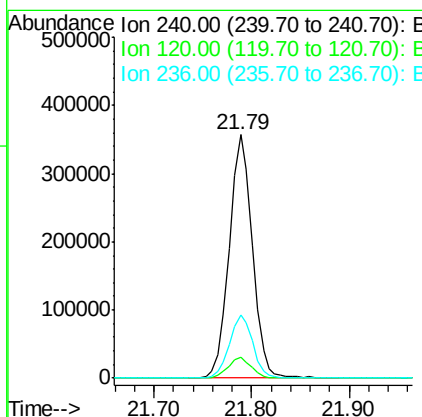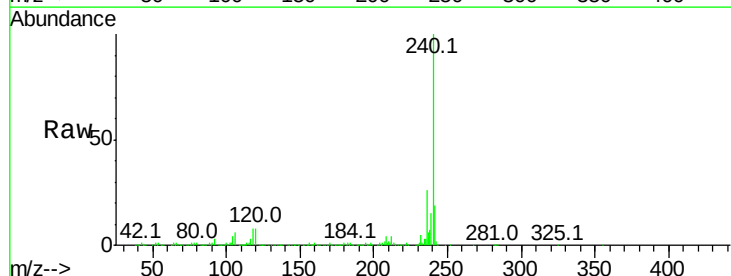

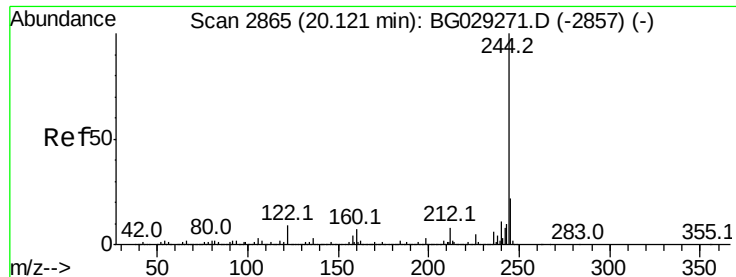

#78

Terphenyl-d14

Concen: 79.012 ng

RT: 20.11 min Scan# 2863

Delta R.T. -0.01 min

Lab File: BG029410.D

Acq: 23 Oct 2017 22:11

Instrument :

BNA_G

ClientSampleId :

15-40-RT4651


Tot Ion:244 Resp: 2035489

Ion Ratio Lower Upper

244 100

212 8.6 5.8 8.8




122 10.2 7.0 10.4

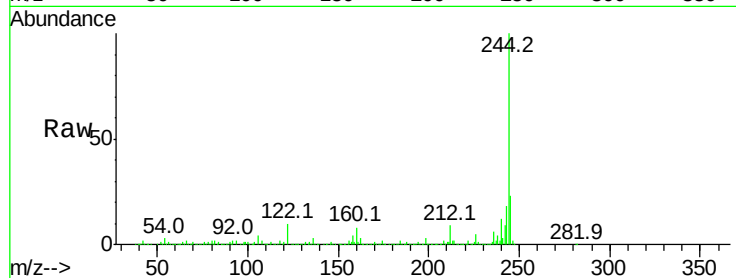

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

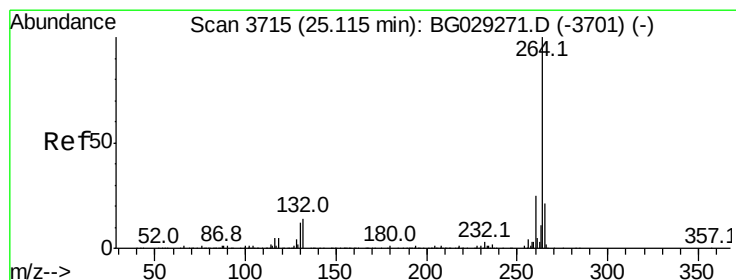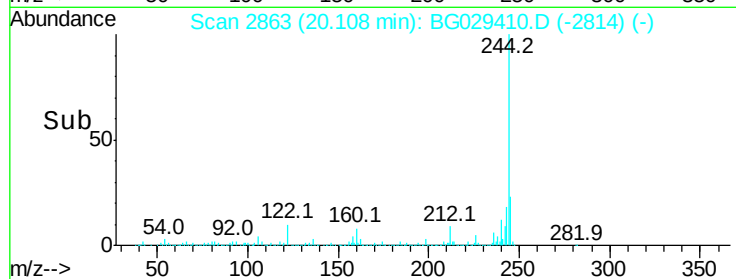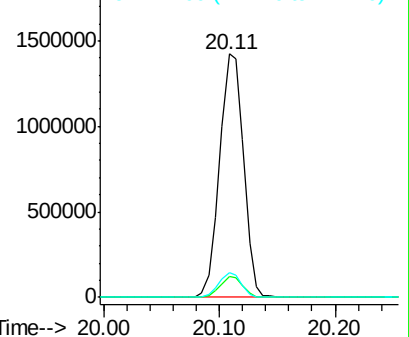

#86

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712

Delta R.T. -0.02 min

Lab File: BG029410.D

Acq: 23 Oct 2017 22:11


Tgt Ion:264 Resp: 574765

Ion Ratio Lower Upper

264 100

260 24.9 17.4 26.0

265 22.3 17.7 26.5

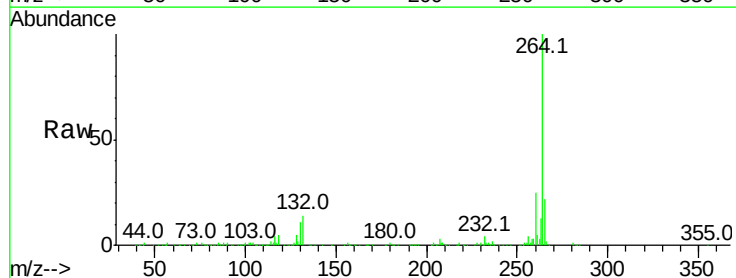

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

