

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102417\
 Data File : BG029423.D
 Acq On : 24 Oct 2017 14:02
 Operator : SJ/JU
 Sample : I5925-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB3L2

Manual Integrations
 APPROVED

Sohil
 10/25/2017 6:27:04 PM

Quant Time: Oct 24 19:25:28 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 17 07:42:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	62764	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.98	136	302197	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	208228	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.52	188	518976	20.00	ng/ul	-0.01
75) Chrysene-d12	21.79	240	573865	20.00	ng/ul	-0.01
83) Perylene-d12	25.10	264	568956	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	7294	4.72	ng/uL	0.00
5) Phenol-d5	7.31	99	146225	24.27	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.48	67	84687	22.47	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.69	132	114464	26.94	ng/ul	-0.01
13) 4-Methylphenol-d8	8.86	113	126366	25.97	ng/ul	-0.01
19) Nitrobenzene-d5	9.33	128	58530	26.98	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.06	143	68239	30.70	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	131392	25.94	ng/ul	-0.01
29) 4-Chloroaniline-d4	11.11	131	166377	28.27	ng/ul	-0.01
43) Dimethylphthalate-d6	14.18	166	447128	25.12	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	550012	25.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	60038	18.27	ng/ul	0.00
57) Fluorene-d10	15.77	176	408487	28.02	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.88	200	47952	18.93	ng/ul	-0.01
70) Anthracene-d10	17.62	188	640071	26.08	ng/ul	-0.01
76) Pyrene-d10	19.89	212	738605	24.86	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	721134	26.76	ng/ul	-0.02

Target Compounds

					Ovalue
56) Diethylphthalate	15.58	149	21621	1.208 ng/ul	98
69) Phenanthrene	17.56	178	95211	3.394 ng/ul	96
74) Fluoranthene	19.56	202	159992	5.103 ng/ul	99
77) Pyrene	19.92	202	140827	3.662 ng/ul	97
80) Benzo(a)anthracene	21.77	228	69468	1.932 ng/ul	98
82) Chrysene	21.84	228	69342	2.122 ng/ul	99
85) Benzo(b)fluoranthene	24.05	252	80671	2.362 ng/ul	97
88) Benzo(a)pyrene	24.94	252	45936	1.382 ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102417\
Data File : BG029423.D
Acq On : 24 Oct 2017 14:02
Operator : SJ/JU
Sample : I5925-05
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
CB3L2

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:04 PM

Quant Time: Oct 24 19:25:28 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 17 07:42:23 2017
Response via : Initial Calibration

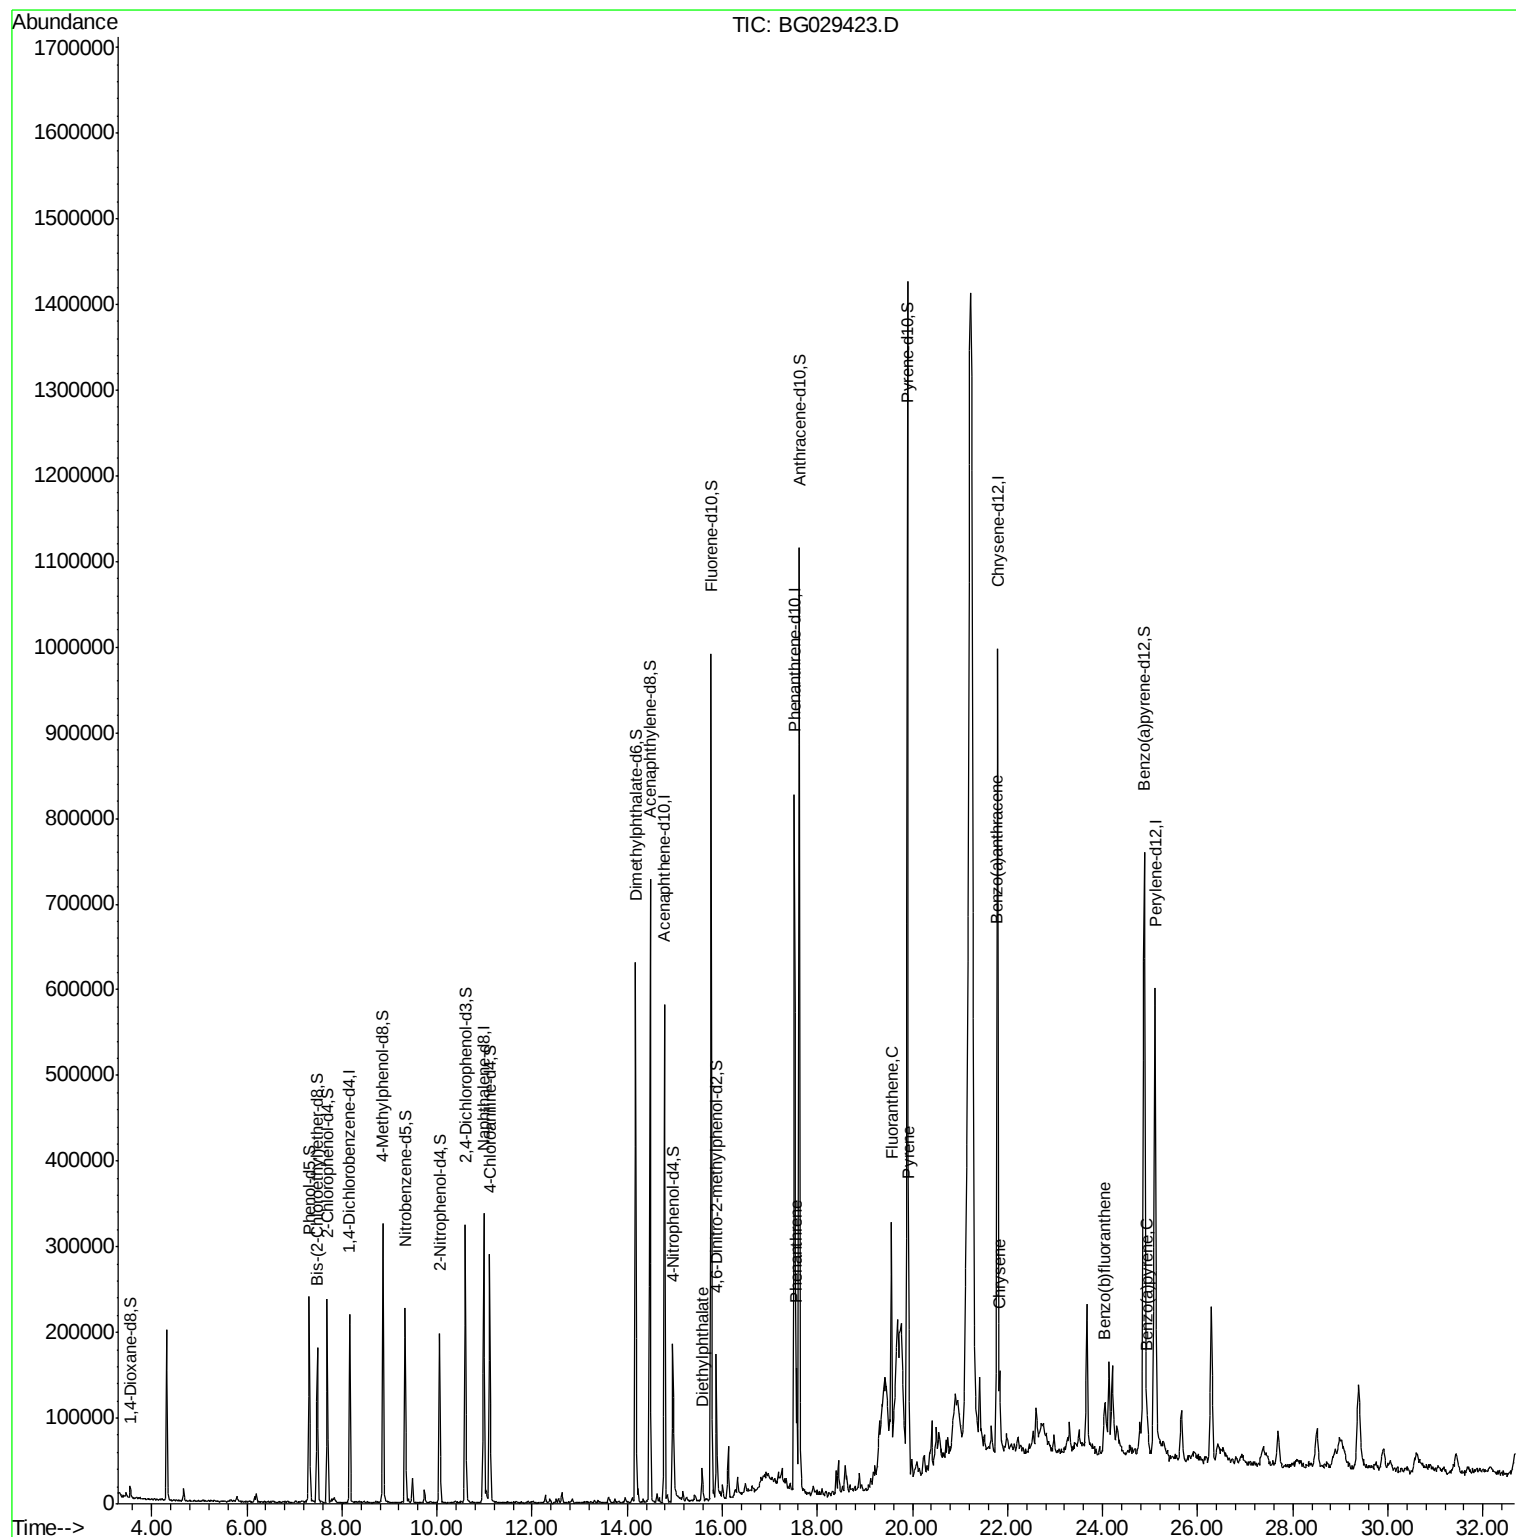

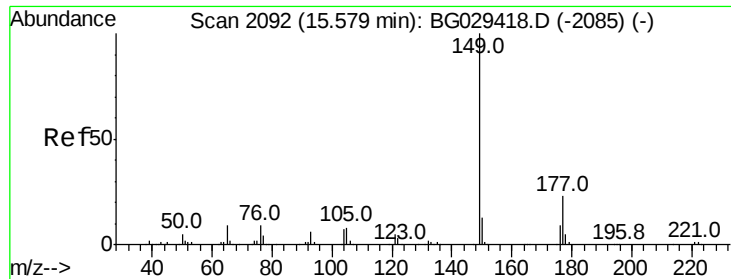

#56

Diethylphthalate

Concen: 1.208 ng/ul

RT: 15.58 min Scan# 2092

Delta R.T. -0.01 min

Lab File: BG029423.D

Acq: 24 Oct 2017 14:02

Instrument :

BNA_G





ClientSampleId :

CB3L2

Tot Ion:	149	Resp:	21621
Ion Ratio	Lower	Upper	
149	100		
177	21.1	17.8	26.6
150	12.8	9.8	14.8

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:04 PM

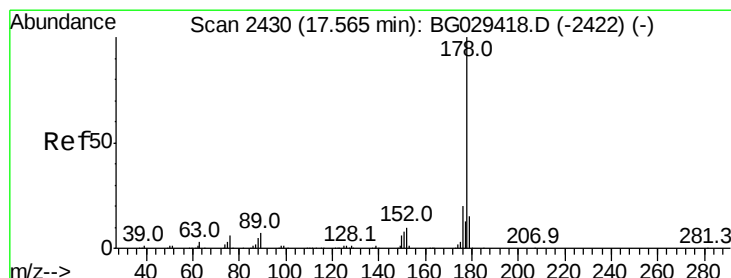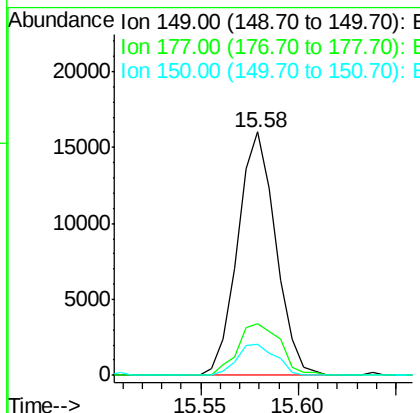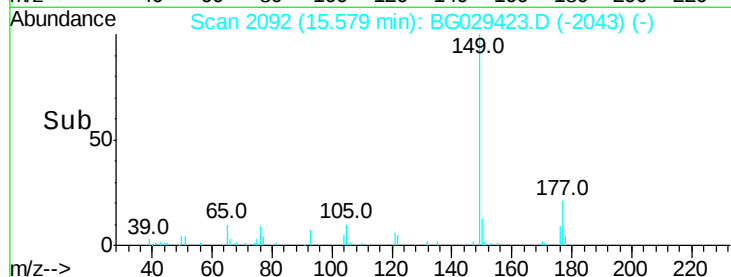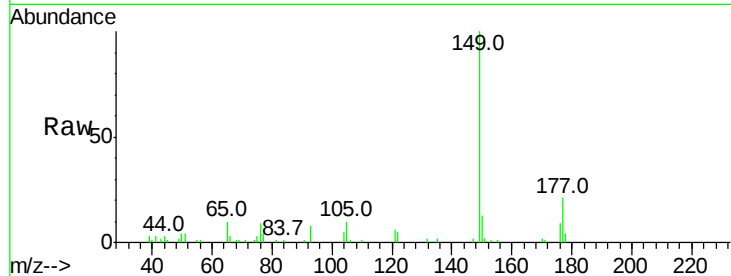

#69

Phenanthrene

Concen: 3.394 ng/ul




RT: 17.56 min Scan# 2429


Delta R.T. -0.01 min

Lab File: BG029423.D

Acq: 24 Oct 2017 14:02

Tgt Ion:	178	Resp:	95211
Ion Ratio	Lower	Upper	
178	100		
179	15.2	13.0	19.6
176	21.3	15.3	22.9

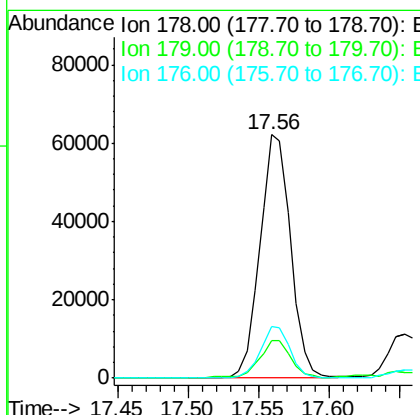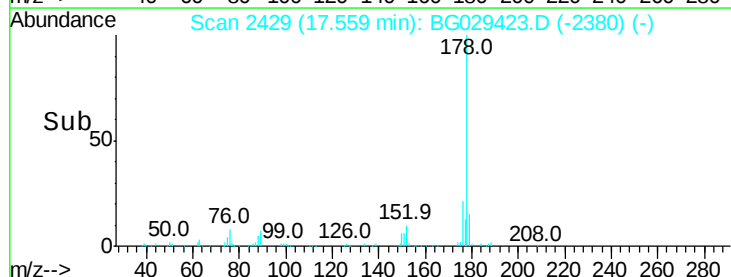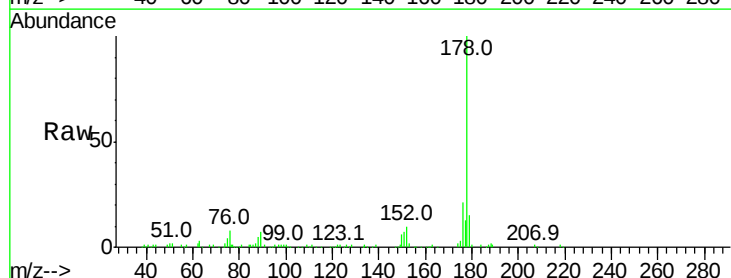

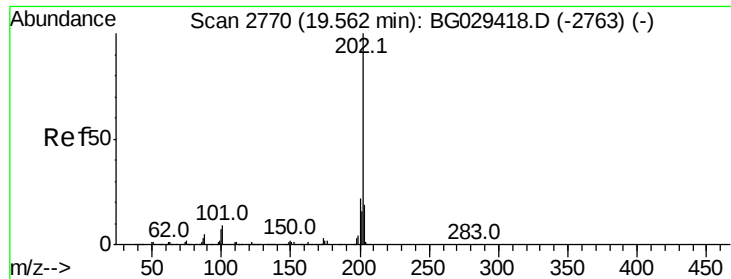





#74
 Fluoranthene
 Concen: 5.103 ng/ul
 RT: 19.56 min Scan# 2769
 Delta R.T. -0.01 min
 Lab File: BG029423.D
 Acq: 24 Oct 2017 14:02

Instrument :
 BNA_G
 ClientSampleId :
 CB3L2

Tot Ion:	202	Resp:	159992
Ion Ratio	Lower	Upper	
202	100		
101	9.3	7.4	11.2
100	7.4	5.6	8.4




Manual Integrations
 APPROVED


Sohil
 10/25/2017 6:27:04 PM

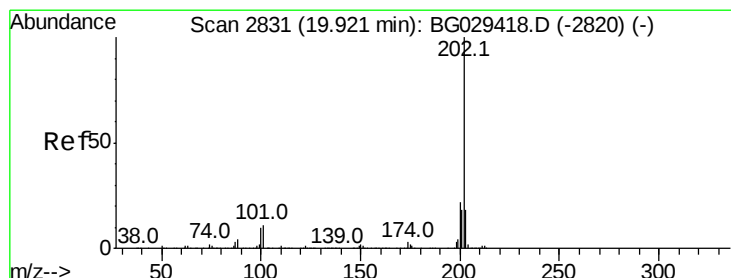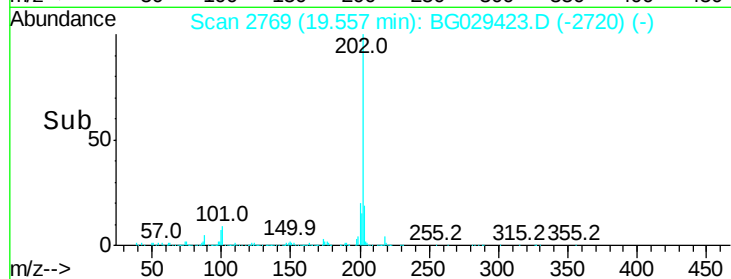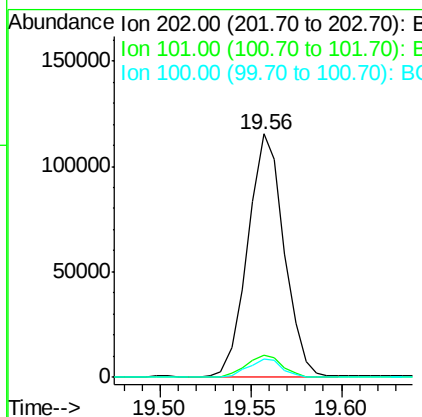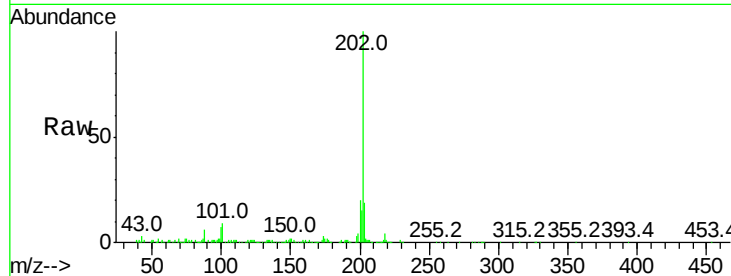

#77
 Pyrene
 Concen: 3.662 ng/ul
 RT: 19.92 min Scan# 2831
 Delta R.T. -0.01 min
 Lab File: BG029423.D
 Acq: 24 Oct 2017 14:02

Tgt Ion:	202	Resp:	140827
Ion Ratio	Lower	Upper	
202	100		
101	9.3	8.4	12.6
100	8.1	7.0	10.6

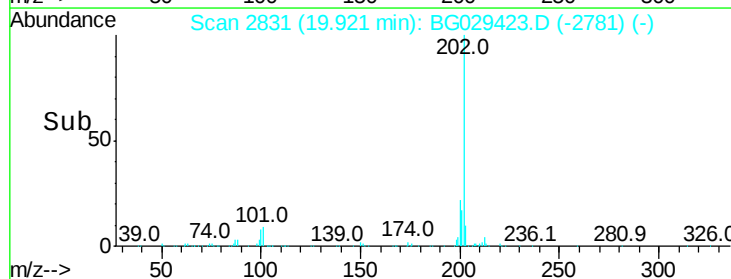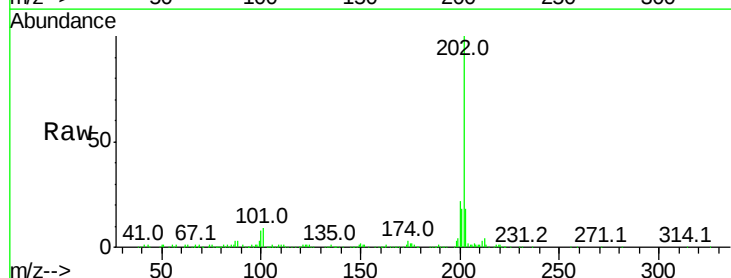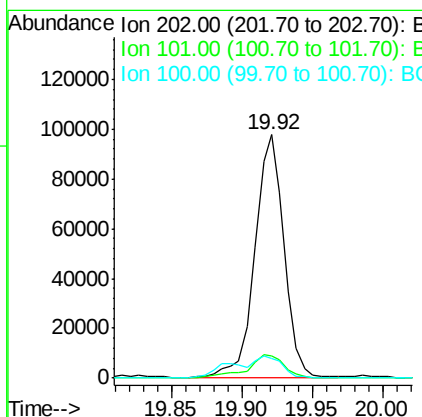

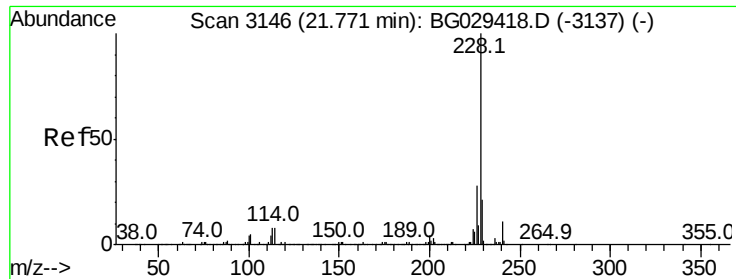





#80
Benzo(a)anthracene
Concen: 1.932 ng/ul
RT: 21.77 min Scan# 3146
Delta R.T. -0.01 min
Lab File: BG029423.D
Acq: 24 Oct 2017 14:02

Instrument :
BNA_G
ClientSampled :
CB3L2

Tot Ion	Ratio	Lower	Upper
228	100		
229	19.1	16.2	24.4
226	28.2	22.2	33.2




Manual Integrations
APPROVED


Sohil
10/25/2017 6:27:04 PM

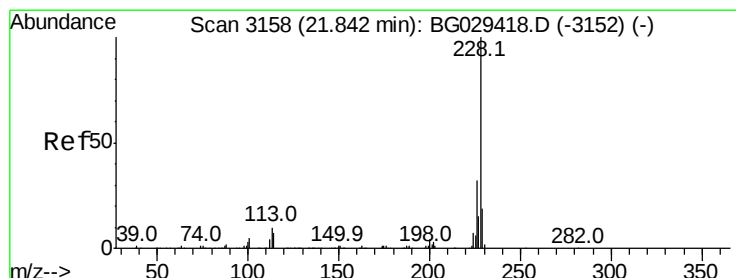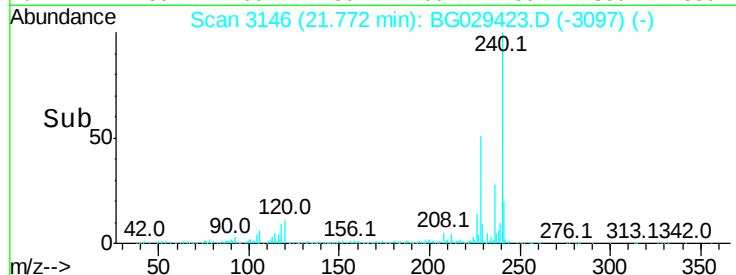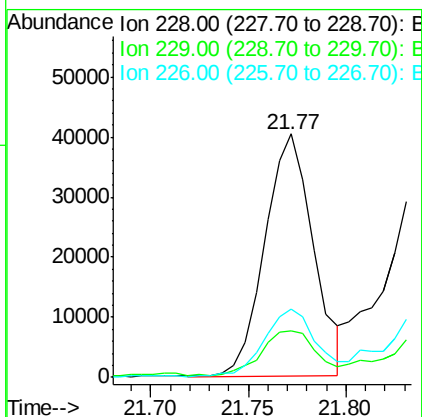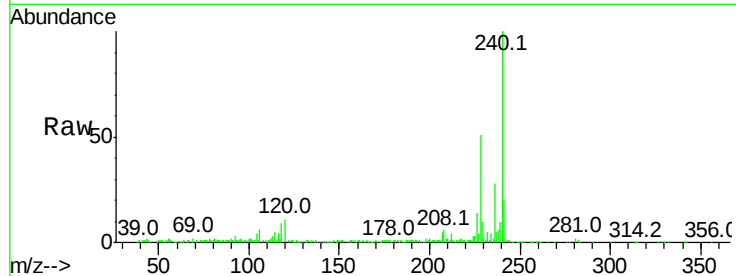

#82
Chrysene
Concen: 2.122 ng/ul
RT: 21.84 min Scan# 3157
Delta R.T. -0.01 min
Lab File: BG029423.D
Acq: 24 Oct 2017 14:02

Tgt Ion	Ratio	Lower	Upper
228	100		
226	31.0	24.2	36.2
229	19.2	15.2	22.8

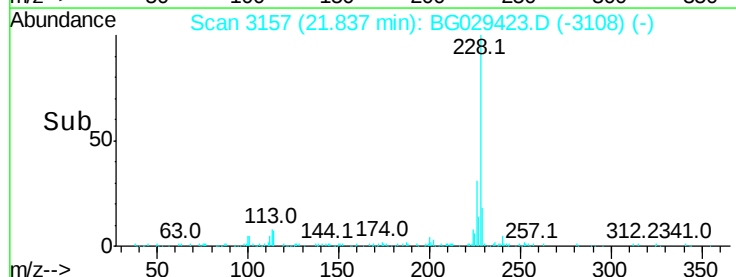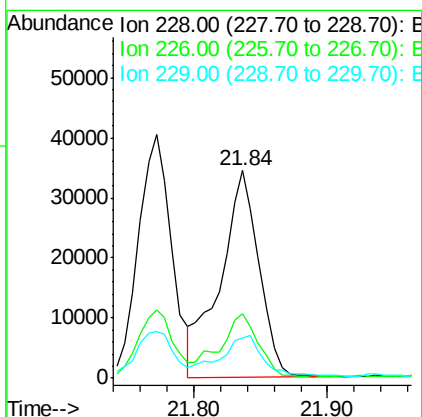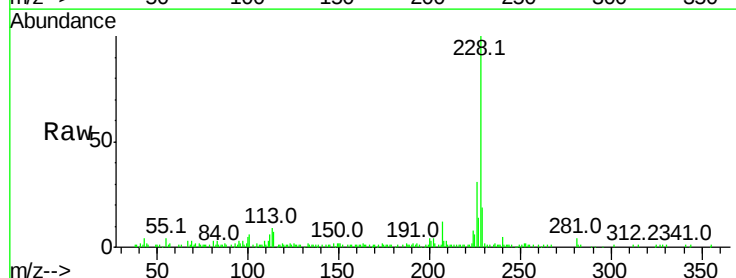

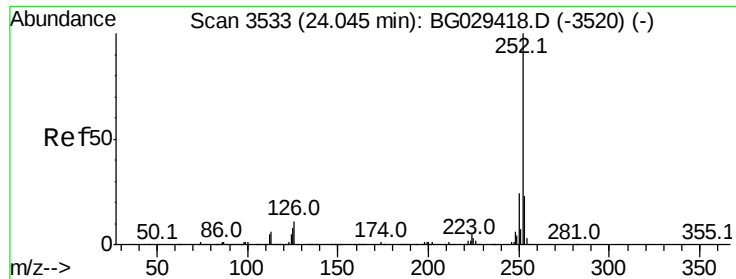

#85

Benzo(b)fluoranthene

Concen: 2.362 ng/ul

RT: 24.05 min Scan# 3533

Delta R.T. -0.02 min

Lab File: BG029423.D

Acq: 24 Oct 2017 14:02

Instrument :

BNA_G





ClientSampleId :

CB3L2

Tot Ion:	252	Resp:	80671
Ion Ratio	Lower	Upper	
252	100		
253	22.5	17.0	25.4
125	10.2	7.5	11.3

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:04 PM

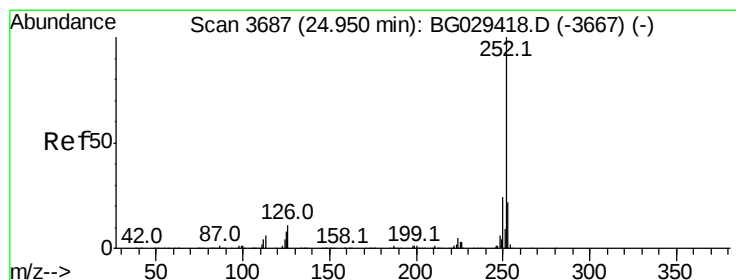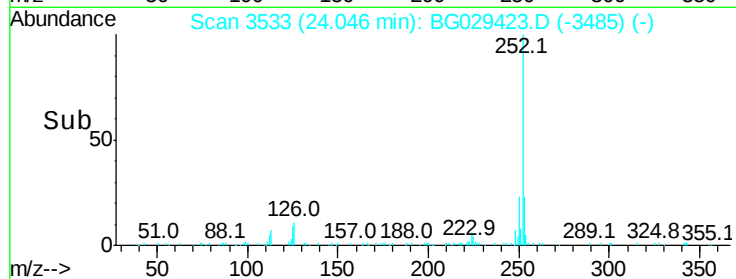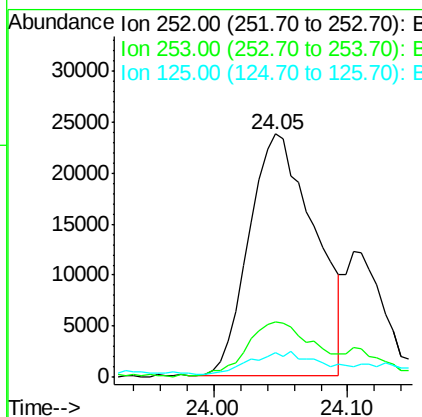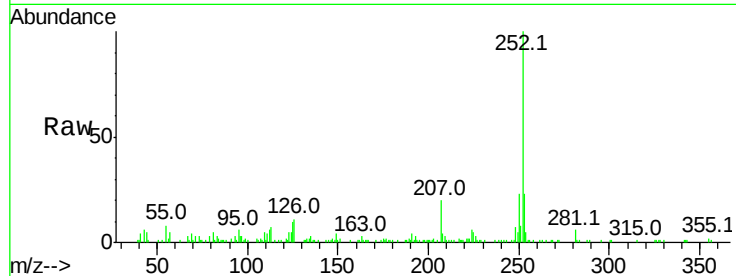

#88

Benzo(a)pyrene

Concen: 1.382 ng/ul

RT: 24.94 min Scan# 3685

Delta R.T. -0.02 min

Lab File: BG029423.D

Acq: 24 Oct 2017 14:02

Tgt Ion:	252	Resp:	45936
Ion Ratio	Lower	Upper	
252	100		
253	22.4	17.1	25.7
125	12.7	7.8	11.8#

