

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102417\
 Data File : BG029428.D
 Acq On : 24 Oct 2017 17:21
 Operator : SJ/JU
 Sample : I5925-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB3L7

Manual Integrations
 APPROVED

Sohil
 10/25/2017 6:27:12 PM

Quant Time: Oct 24 19:42:17 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 17 07:42:23 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	63780	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.98	136	305826	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.78	164	207552	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.52	188	491141	20.00	ng/ul	-0.01
75) Chrysene-d12	21.79	240	531250	20.00	ng/ul	-0.01
83) Perylene-d12	25.10	264	531907	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	8534	5.44	ng/uL	0.00
5) Phenol-d5	7.32	99	170458	27.85	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.48	67	98267	25.65	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.70	132	134848	31.23	ng/ul	-0.01
13) 4-Methylphenol-d8	8.87	113	153919	31.13	ng/ul	-0.01
19) Nitrobenzene-d5	9.33	128	68765	31.32	ng/ul	-0.01
22) 2-Nitrophenol-d4	10.06	143	81606	36.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	158736	30.97	ng/ul	-0.01
29) 4-Chloroaniline-d4	11.11	131	194515	32.66	ng/ul	-0.01
43) Dimethylphthalate-d6	14.18	166	523199	29.49	ng/ul	-0.01
46) Acenaphthylene-d8	14.48	160	647287	30.00	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.97	143	69717	21.28	ng/ul	-0.01
57) Fluorene-d10	15.77	176	479121	32.97	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.88	200	67590	28.19	ng/ul	-0.01
70) Anthracene-d10	17.62	188	717362	30.88	ng/ul	-0.01
76) Pyrene-d10	19.89	212	828429	30.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.88	264	802286	31.85	ng/ul	-0.02

Target Compounds

					Ovalue	
44) Dimethylphthalate	14.22	163	37972	2.194	ng/ul#	97
69) Phenanthrene	17.56	178	203334	7.658	ng/ul	98
71) Anthracene	17.66	178	34735	1.268	ng/ul	96
74) Fluoranthene	19.56	202	348776	11.754	ng/ul	99
77) Pyrene	19.92	202	310090	8.709	ng/ul	98
80) Benzo(a)anthracene	21.77	228	174586	5.244	ng/ul	99
82) Chrysene	21.84	228	177906	5.881	ng/ul	98
85) Benzo(b)fluoranthene	24.05	252	230980	7.233	ng/ul	99
86) Benzo(k)fluoranthene	24.11	252	87035m	2.819	ng/ul	
88) Benzo(a)pyrene	24.94	252	155985	5.018	ng/ul	99
89) Indeno(1,2,3-cd)pyrene	28.87	276	119234	3.391	ng/ul	98
90) Dibenzo(a,h)anthracene	28.93	278	34330	1.175	ng/ul#	93
91) Benzo(g,h,i)perylene	30.06	276	111195	3.815	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102417\
Data File : BG029428.D
Acq On : 24 Oct 2017 17:21
Operator : SJ/JU
Sample : I5925-12
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampled :
CB3L7

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:12 PM

Quant Time: Oct 24 19:42:17 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 17 07:42:23 2017
Response via : Initial Calibration

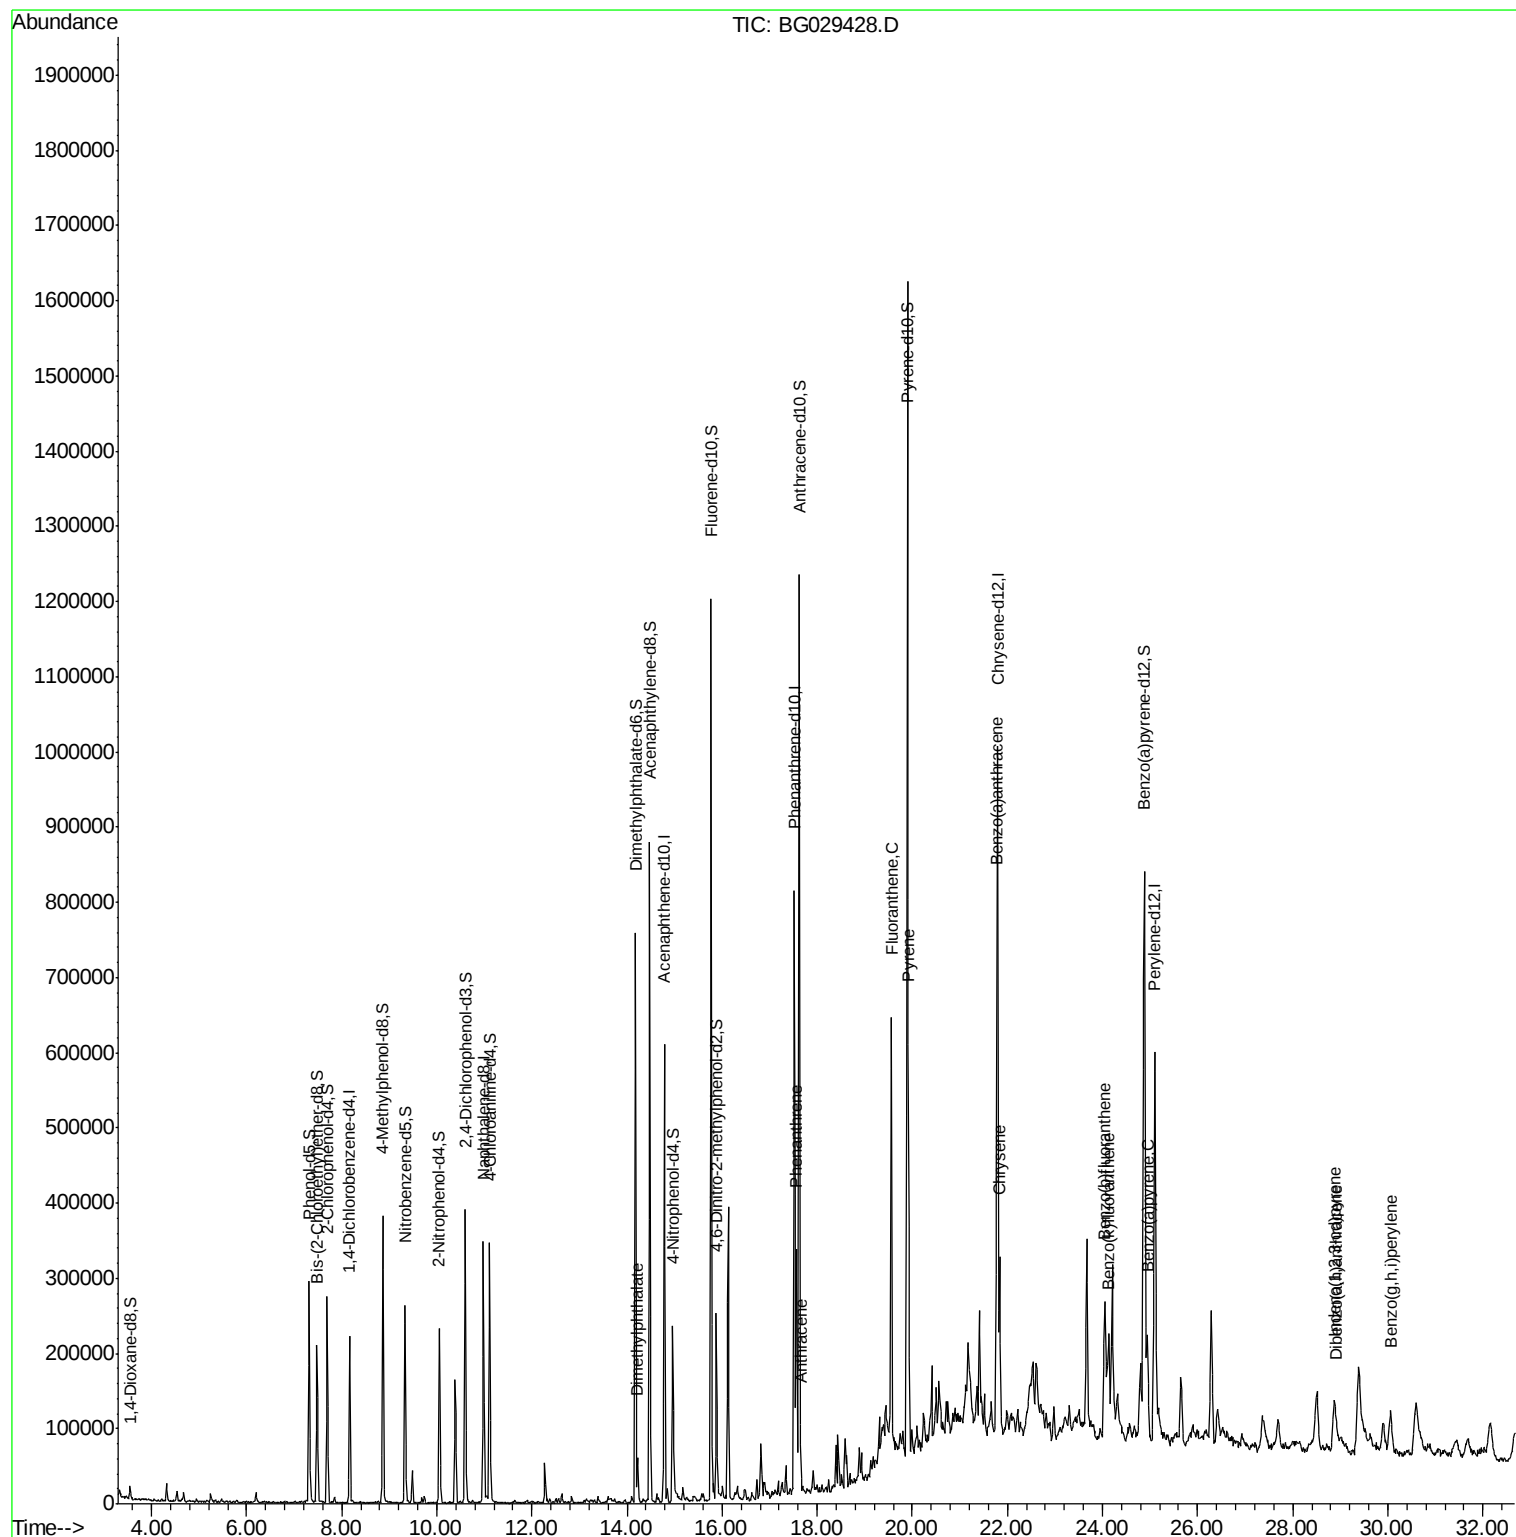

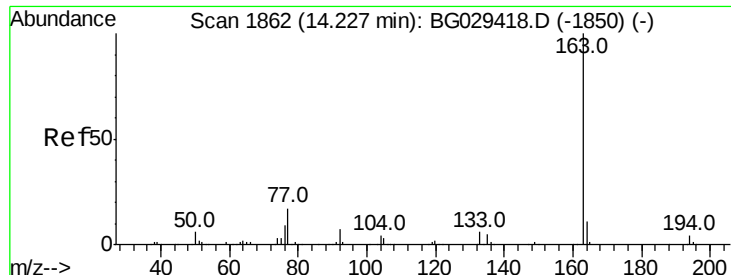


#44
Dimethylphthalate
Concen: 2.194 ng/ul
RT: 14.22 min Scan# 1861
Delta R.T. -0.01 min
Lab File: BG029428.D
Acq: 24 Oct 2017 17:21

Instrument :
BNA_G
ClientSampleId :
CB3L7




Tot Ion	Ratio	Lower	Upper
163	100		
194	5.9	3.5	5.3#
164	10.6	7.6	11.4

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:12 PM

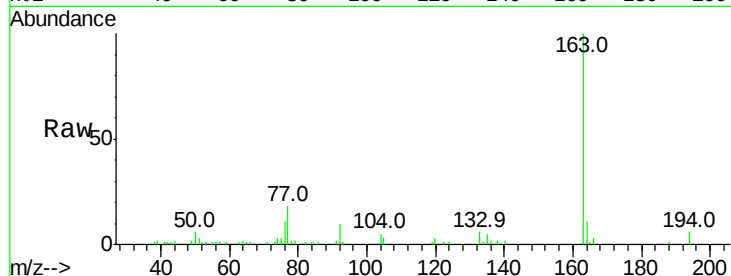


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

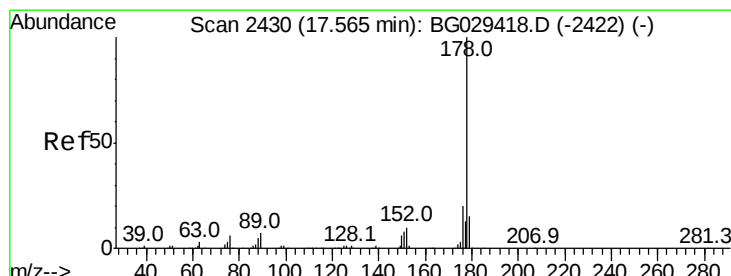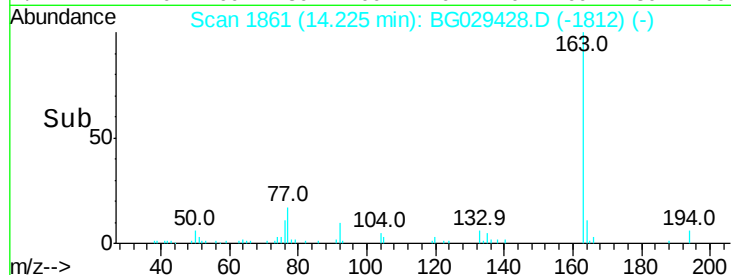
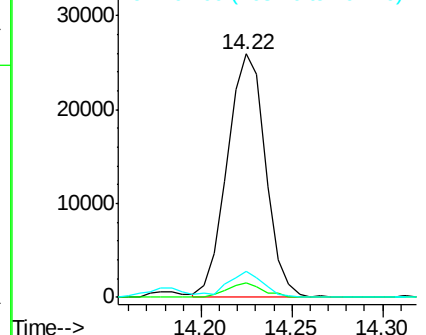



#69
Phenanthrene
Concen: 7.658 ng/ul
RT: 17.56 min Scan# 2429
Delta R.T. -0.01 min
Lab File: BG029428.D
Acq: 24 Oct 2017 17:21

Tgt Ion	Ratio	Lower	Upper
178	100		
179	15.2	13.0	19.6
176	19.5	15.3	22.9

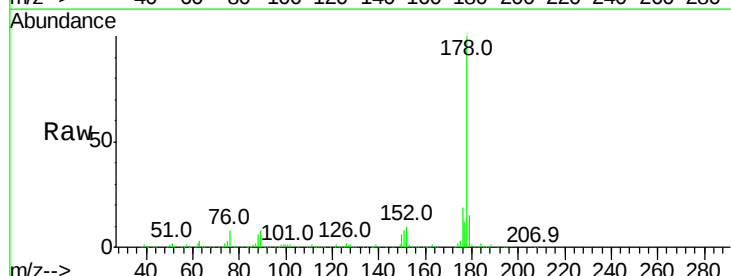

Abundance Ion 178.00 (177.70 to 178.70): E
Ion 179.00 (178.70 to 179.70): E
Ion 176.00 (175.70 to 176.70): E

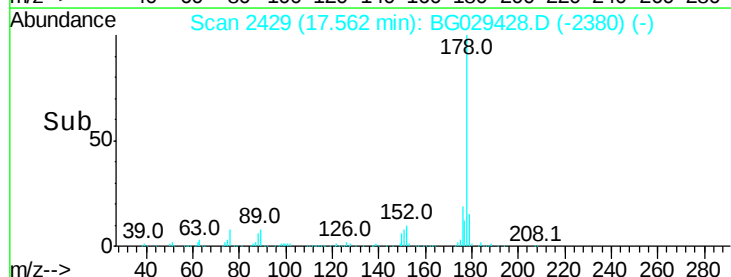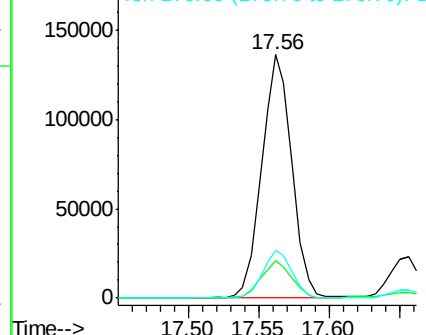

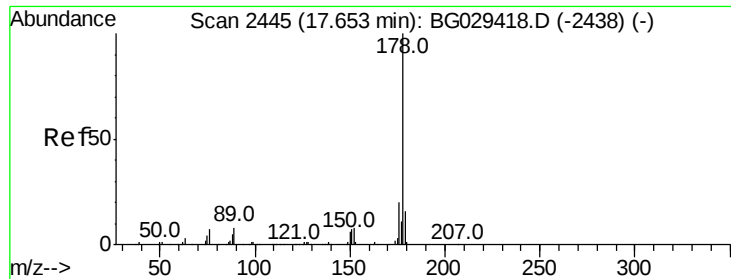





#71
 Anthracene
 Concen: 1.268 ng/ul
 RT: 17.66 min Scan# 2445
 Delta R.T. -0.01 min
 Lab File: BG029428.D
 Acq: 24 Oct 2017 17:21

Instrument :
 BNA_G
 ClientSampleId :
 CB3L7

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.7	13.2	19.8
176	18.4	16.0	24.0




Manual Integrations
 APPROVED


Sohil
 10/25/2017 6:27:12 PM

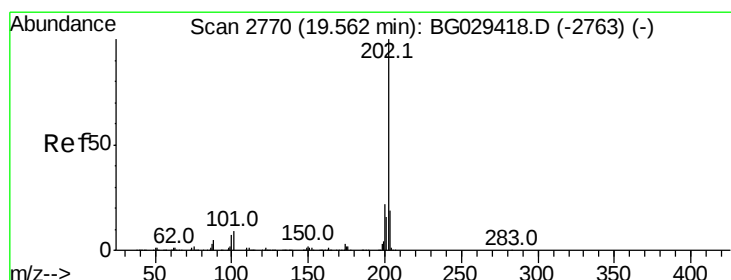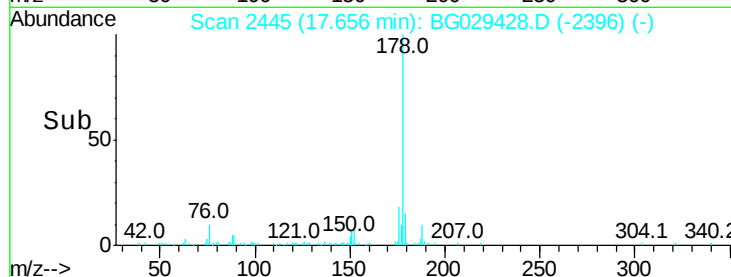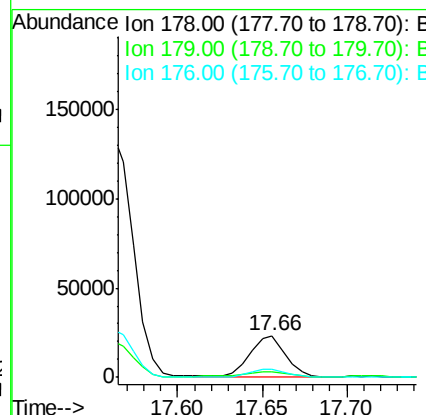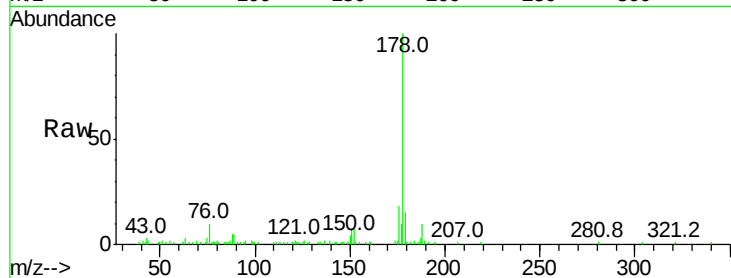

#74
 Fluoranthene
 Concen: 11.754 ng/ul
 RT: 19.56 min Scan# 2769
 Delta R.T. -0.01 min
 Lab File: BG029428.D
 Acq: 24 Oct 2017 17:21

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.4	7.4	11.2
100	7.6	5.6	8.4

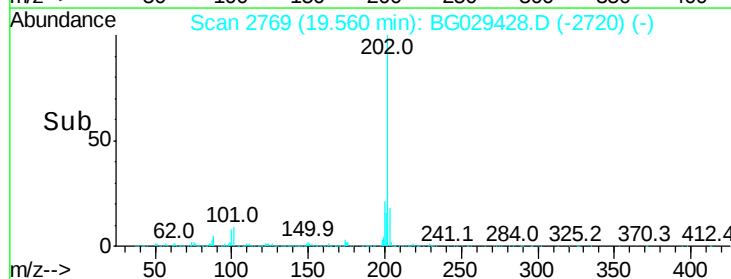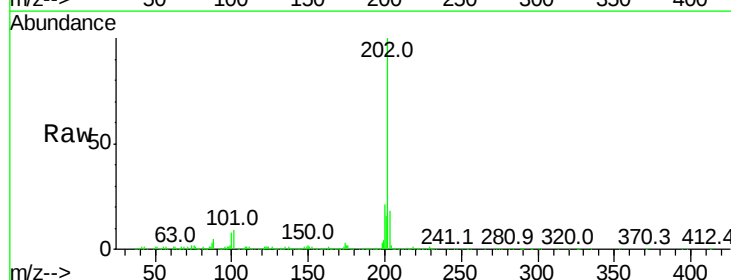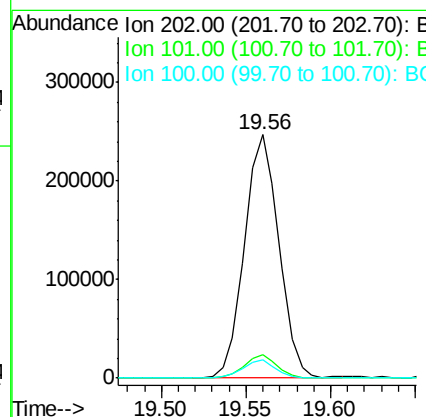

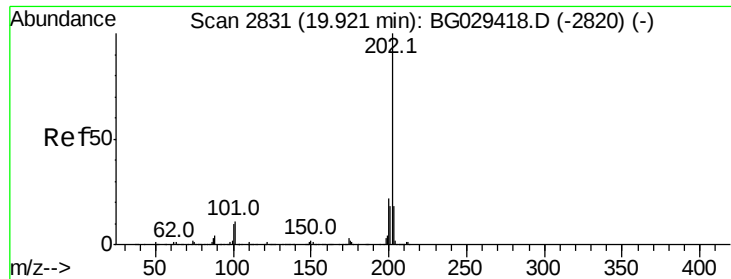

#77

Pvrene

Concen: 8.709 ng/ul

RT: 19.92 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Instrument :

BNA_G





ClientSampled :

CB3L7

Tot Ion:	202	Resp:	310090
Ion Ratio	Lower	Upper	
202	100		
101	11.5	8.4	12.6
100	9.5	7.0	10.6

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:12 PM

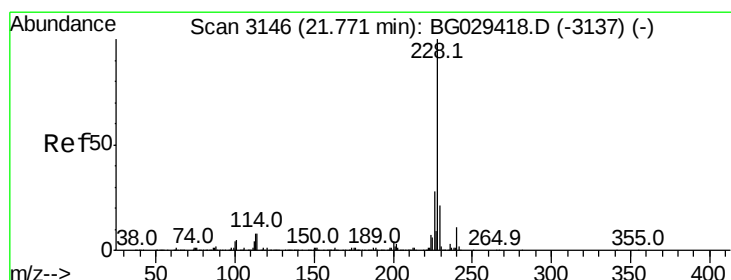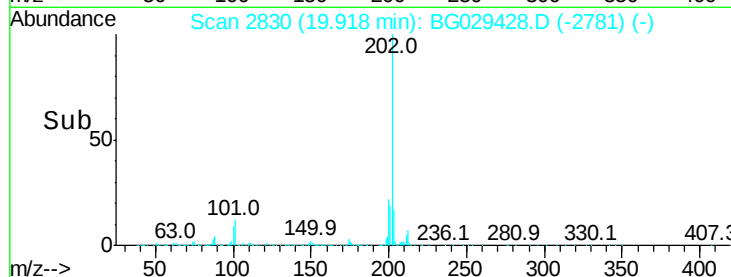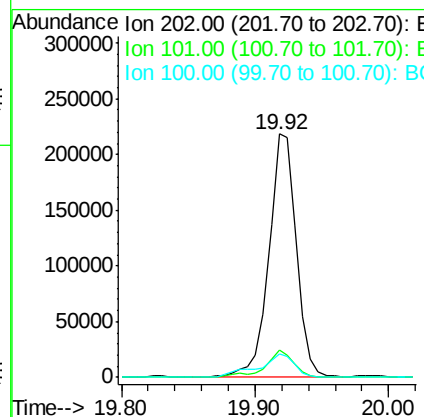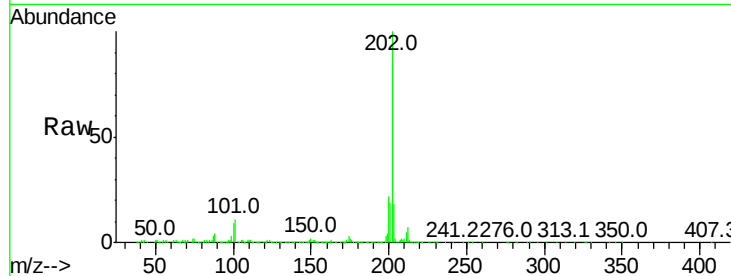

#80

Benzo(a)anthracene

Concen: 5.244 ng/ul




RT: 21.77 min Scan# 3146


Delta R.T. -0.01 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Tgt Ion:	228	Resp:	174586
Ion Ratio	Lower	Upper	
228	100		
229	20.6	16.2	24.4
226	27.4	22.2	33.2

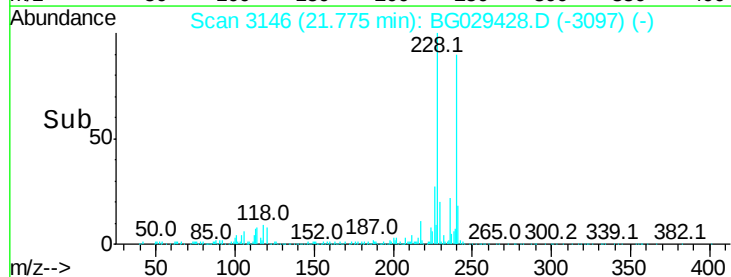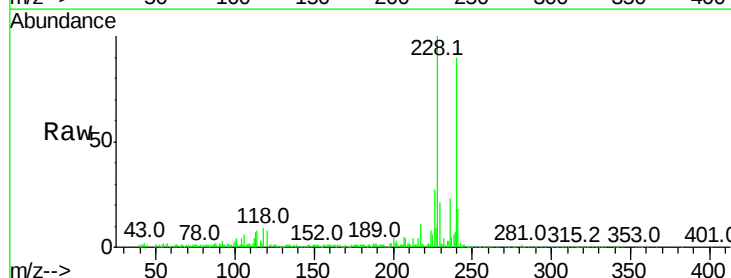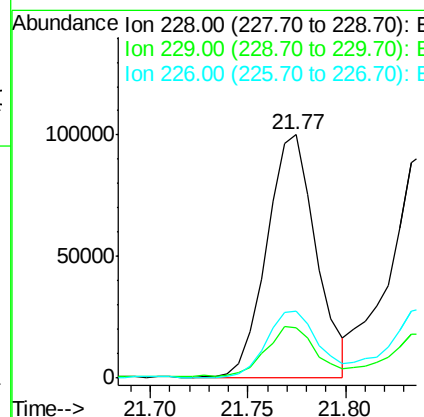

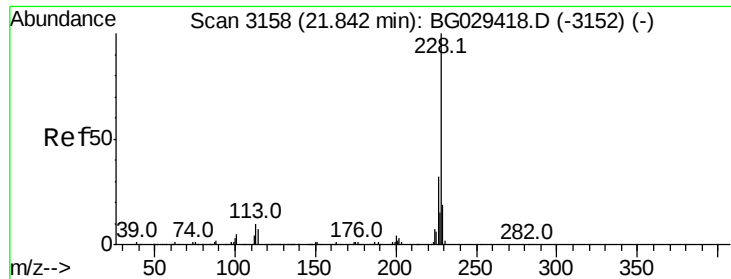

#82

Chrysene

Concen: 5.881 ng/ul

RT: 21.84 min Scan# 3157

Delta R.T. -0.01 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Instrument :

BNA_G


ClientSampleId :

CB3L7

Tot Ion:	228	Resp:	177906
Ion Ratio	Lower	Upper	
228	100		
226	31.3	24.2	36.2
229	19.8	15.2	22.8

Manual Integrations
APPROVED




Sohil
10/25/2017 6:27:12 PM

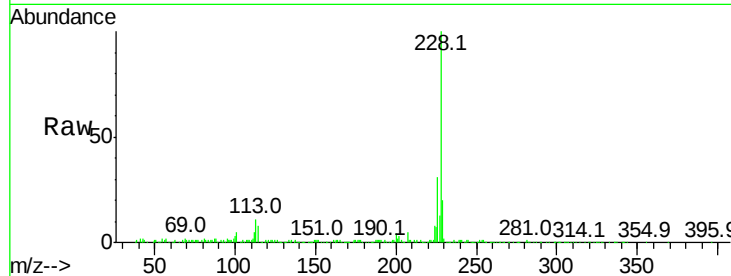

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

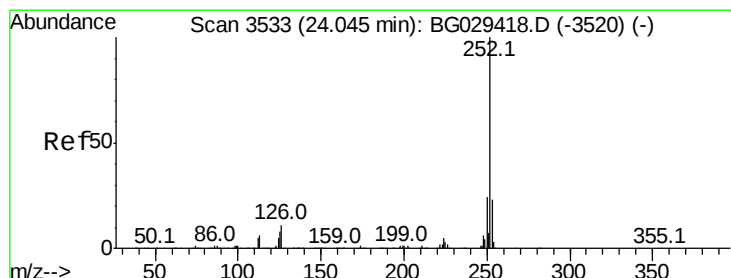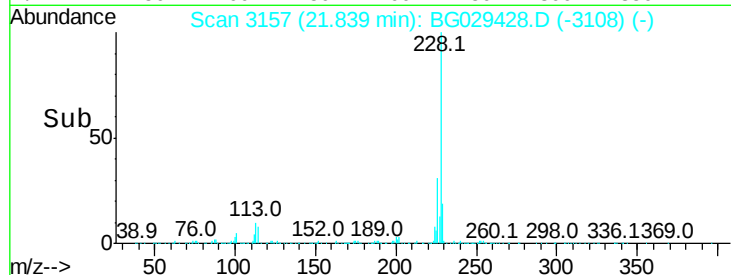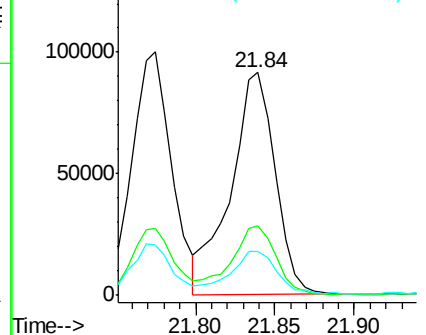

#85

Benzo(b)fluoranthene

Concen: 7.233 ng/ul

RT: 24.05 min Scan# 3533

Delta R.T. -0.02 min

Lab File: BG029428.D




Acq: 24 Oct 2017 17:21


Tgt Ion:	252	Resp:	230980
Ion Ratio	Lower	Upper	
252	100		
253	21.5	17.0	25.4
125	10.1	7.5	11.3

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

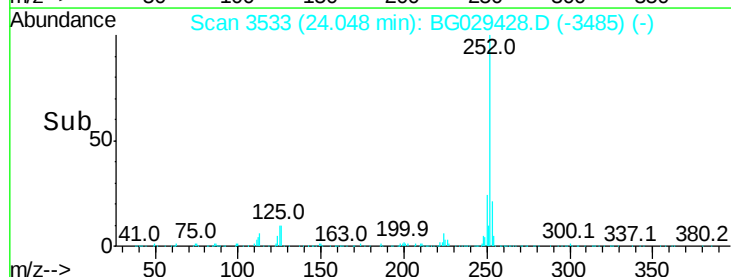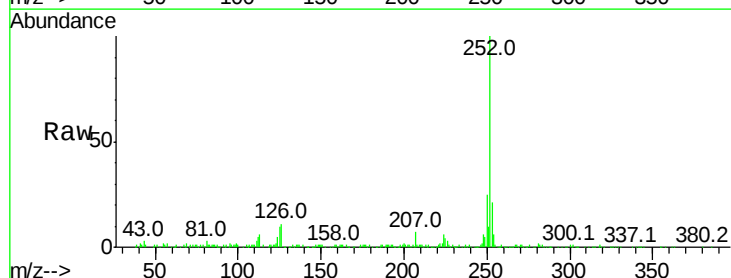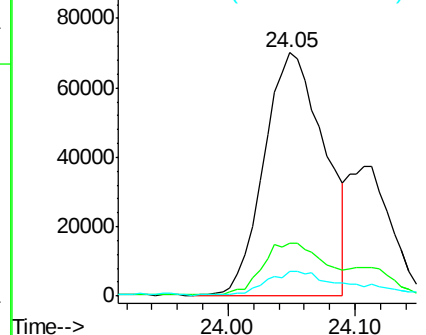

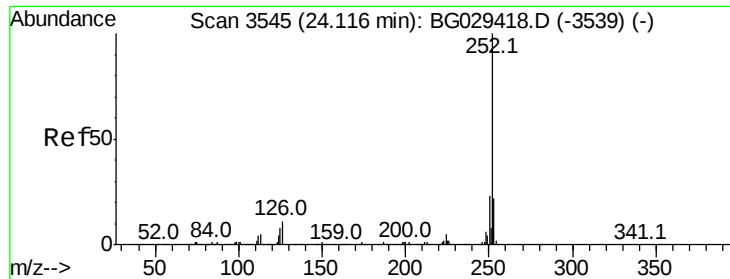





#86
Benzo(k)fluoranthene
Concen: 2.819 ng/ul
RT: 24.11 min Scan# 3544
Delta R.T. -0.02 min
Lab File: BG029428.D
Acq: 24 Oct 2017 17:21

Instrument :
BNA_G
ClientSampleId :
CB3L7

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.8	17.2	25.8
125	9.5	7.8	11.8




Manual Integrations
APPROVED


Sohil
10/25/2017 6:27:12 PM

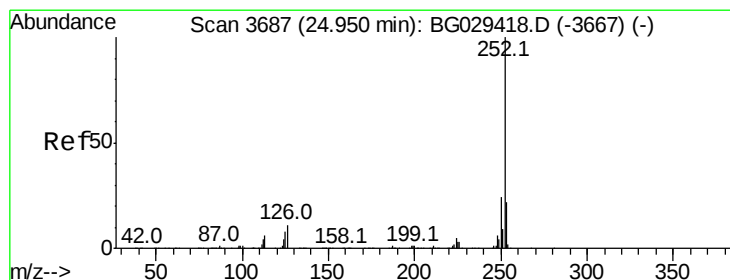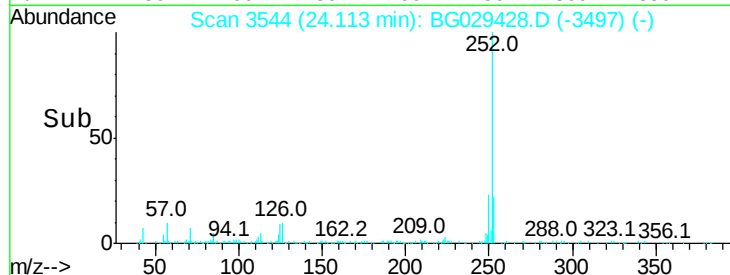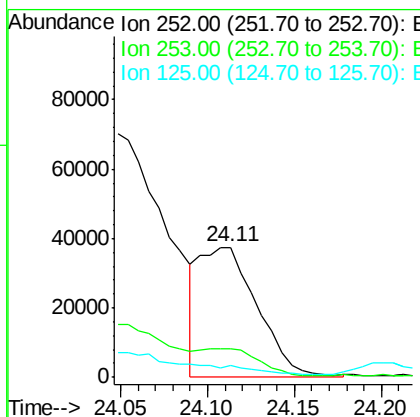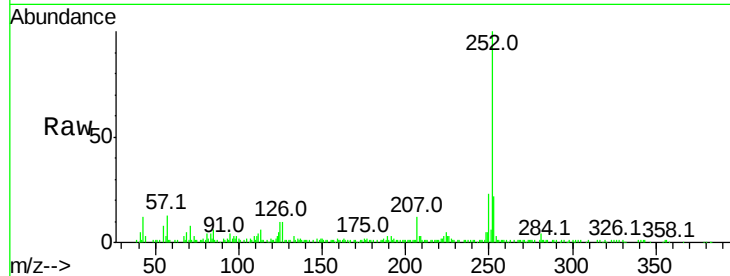

#88
Benzo(a)pyrene
Concen: 5.018 ng/ul
RT: 24.94 min Scan# 3685
Delta R.T. -0.02 min
Lab File: BG029428.D
Acq: 24 Oct 2017 17:21

Tgt Ion	Ratio	Lower	Upper
252	100		
253	21.5	17.1	25.7
125	8.7	7.8	11.8

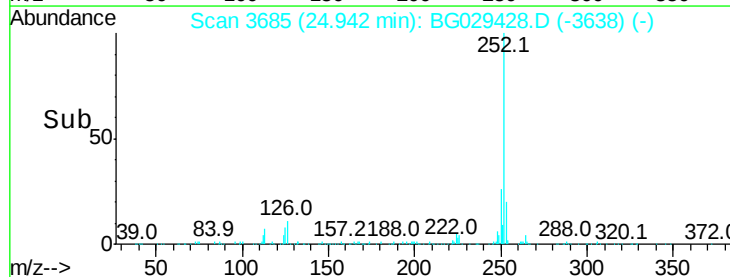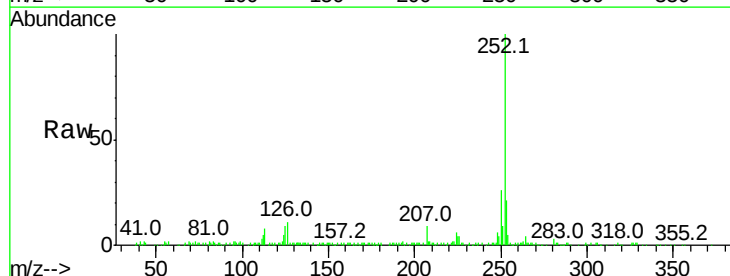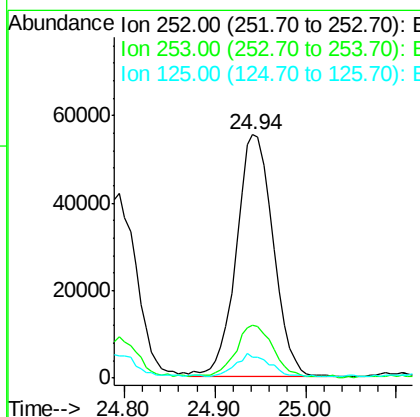

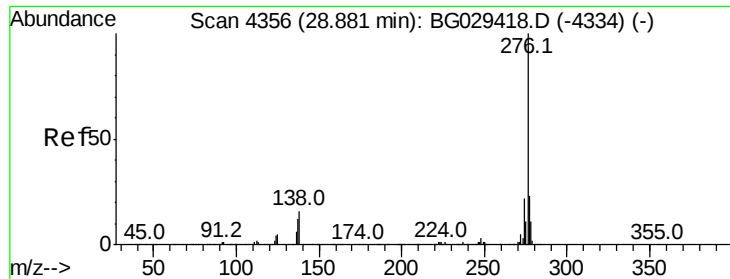

#89

Indeno(1,2,3-cd)pyrene

Concen: 3.391 ng/ul

RT: 28.87 min Scan# 4354

Delta R.T. -0.04 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Instrument :

BNA_G





ClientSampleId :

CB3L7

Tot Ion:	276	Resp:	119234
Ion Ratio	Lower	Upper	
276	100		
138	17.8	13.4	20.0
277	22.9	18.6	28.0

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:12 PM

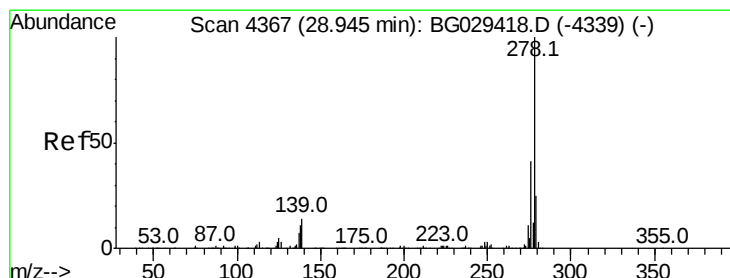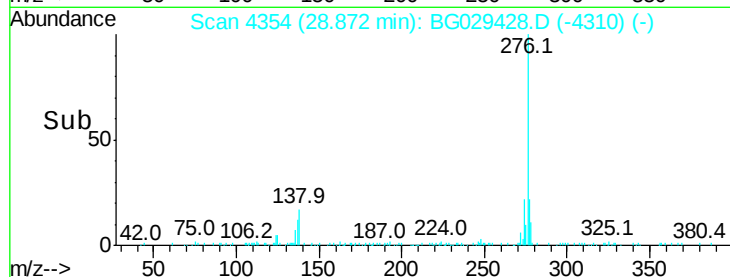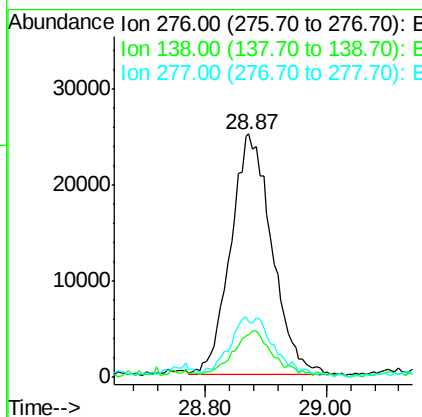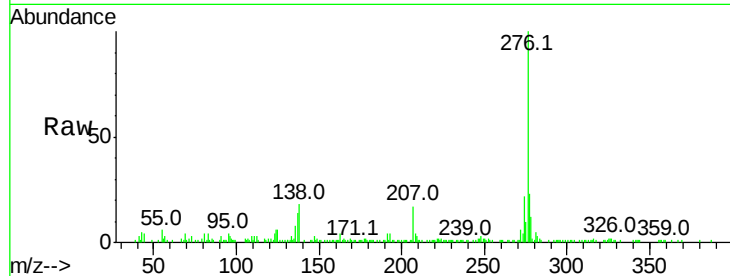

#90

Dibenzo(a,h)anthracene

Concen: 1.175 ng/ul




RT: 28.93 min Scan# 4363


Delta R.T. -0.06 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Tgt Ion:	278	Resp:	34330
Ion Ratio	Lower	Upper	
278	100		
139	16.3	9.4	14.2#
279	20.6	18.4	27.6

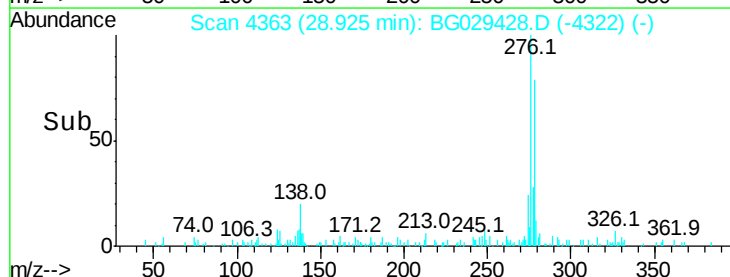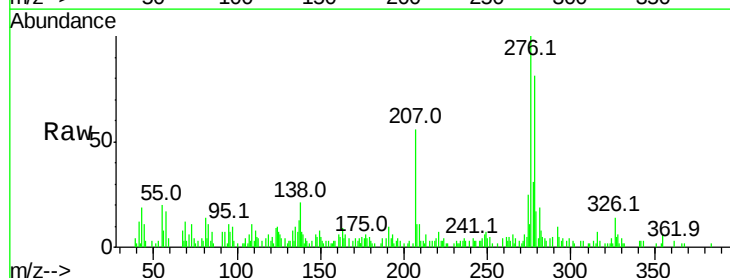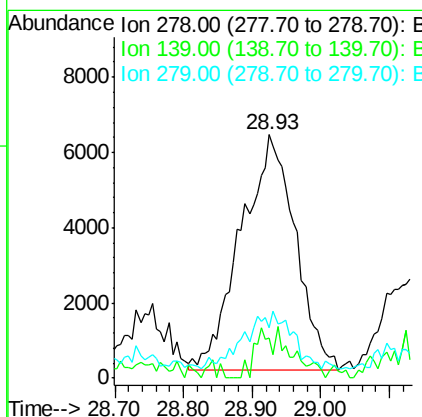

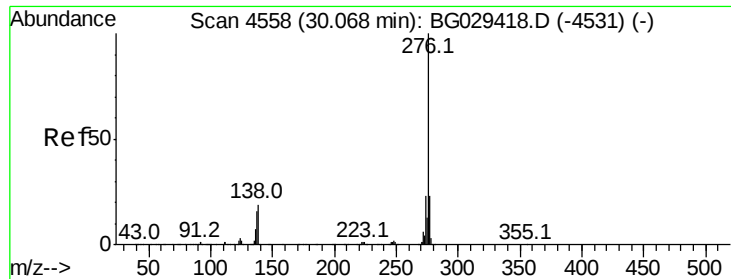

#91

Benzo(a,h,i)perylene

Concen: 3.815 ng/ul

RT: 30.06 min Scan# 4556

Delta R.T. -0.04 min

Lab File: BG029428.D

Acq: 24 Oct 2017 17:21

Instrument :

BNA_G

ClientSampleId :

CB3L7

Tot Ion:	276	Resp:	111195
Ion Ratio	Lower	Upper	
276	100		
138	16.3	12.1	18.1
277	24.4	17.7	26.5

Manual Integrations
APPROVED

Sohil
10/25/2017 6:27:12 PM

