

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102418\
 Data File : BG037513.D
 Acq On : 24 Oct 2018 16:09
 Operator : JU/SJ
 Sample : PB1141123BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 25 07:59:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	52092	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	232383	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	165101	20.00	ng	0.00
64) Phenanthrene-d10	17.49	188	403960	20.00	ng	0.00
76) Chrysene-d12	21.77	240	370607	20.00	ng	0.00
87) Perylene-d12	25.10	264	358856	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	390328	125.27	ng	0.00
7) Phenol-d6	7.25	99	580899	123.29	ng	0.00
23) Nitrobenzene-d5	9.28	82	328839	79.27	ng	0.00
42) 2,4,6-Tribromophenol	16.23	330	212967	118.27	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	819444	74.84	ng	0.00
79) Terphenyl-d14	20.08	244	1281276	73.87	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.28	70	41835	12.894	ng	# 71
51) 2,6-Dinitrotoluene	14.74	165	21725	7.689	ng	# 25
57) 2,4-Dinitrotoluene	14.74	165	21725	5.857	ng	# 25
65) 4,6-Dinitro-2-methylphenol	16.22	198	591	8.737	ng	88
67) 4-Bromophenyl-phenylether	16.22	248	15377	3.466	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102418\
Data File : BG037513.D
Acq On : 24 Oct 2018 16:09
Operator : JU/SJ
Sample : PB1141123BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 25 07:59:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

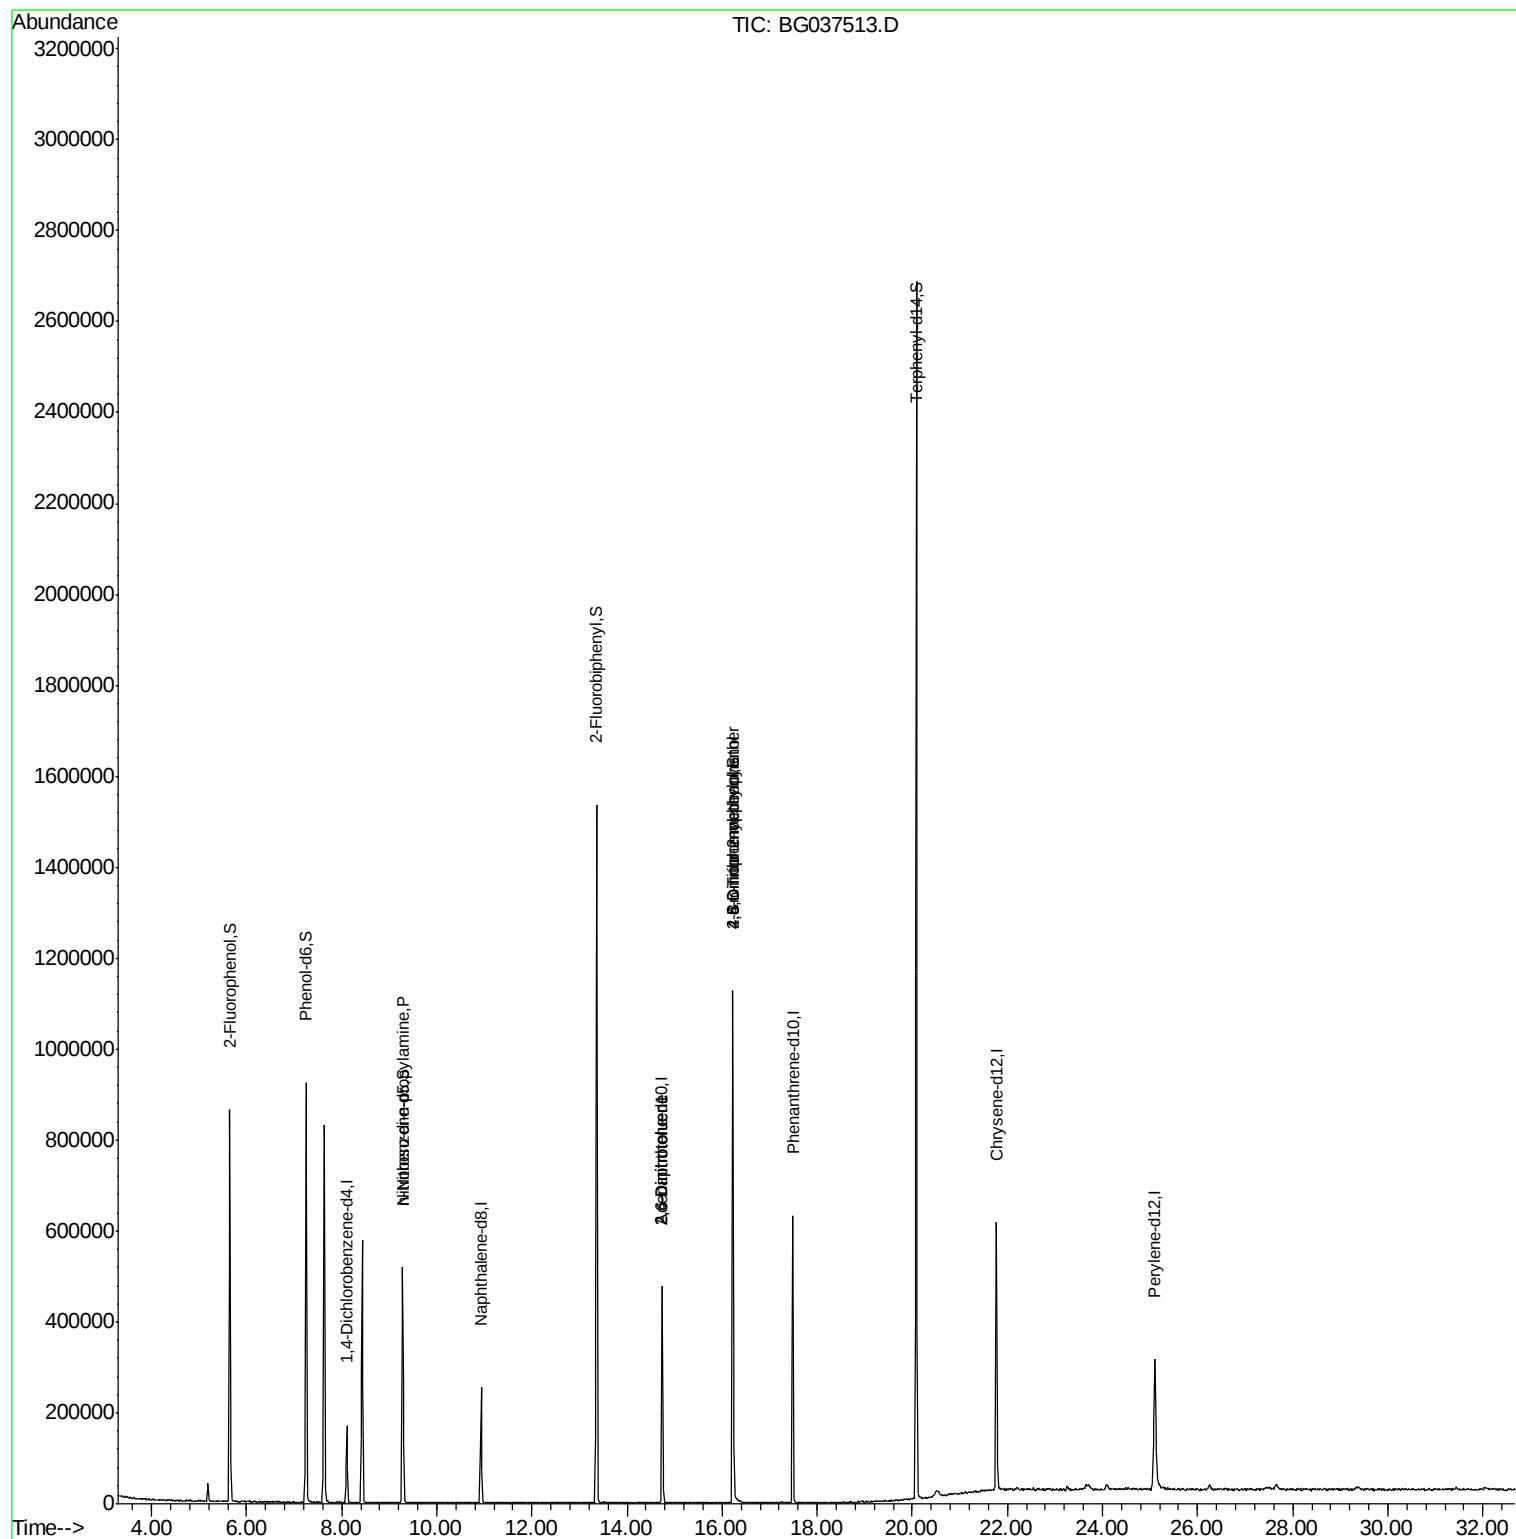




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 52092
Ion Ratio Lower Upper
152 100
150 162.9 126.0 189.0
115 54.1 45.5 68.3

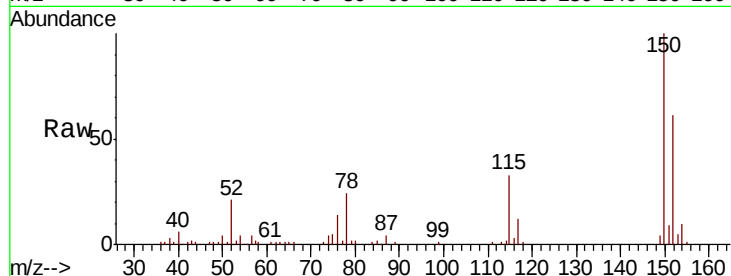


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

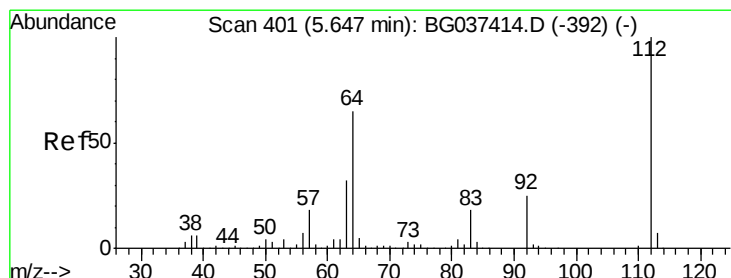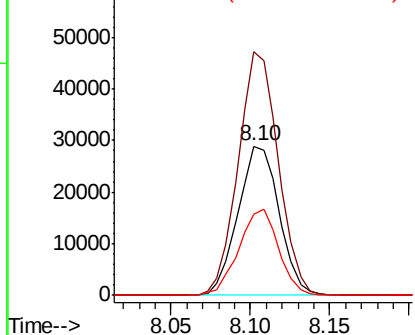



#5


2-Fluorophenol
Concen: 125.273 ng
RT: 5.65 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Tgt Ion:112 Resp: 390328
Ion Ratio Lower Upper
112 100
64 66.5 53.1 79.7
63 32.8 27.3 40.9

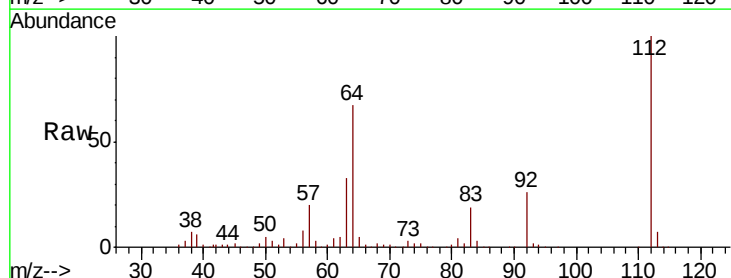

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

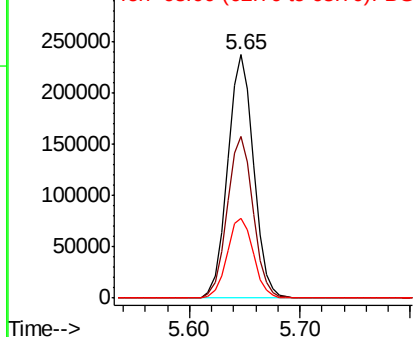

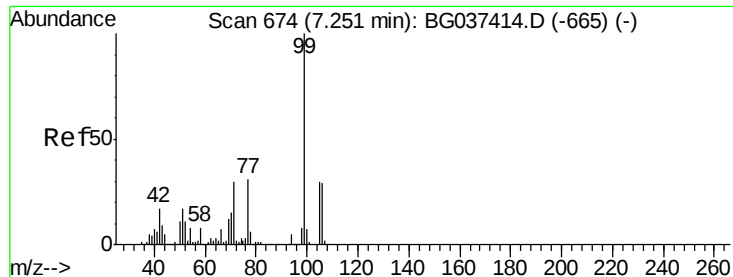

#7

Phenol-d6

Concen: 123.293 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.00 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampled :


Tot Ion: 99 Resp: 580899

Ion Ratio Lower Upper




99 100

42 18.2 15.0 22.4

71 30.1 25.5 38.3

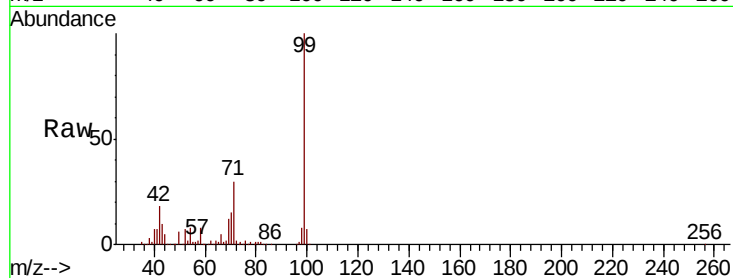

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

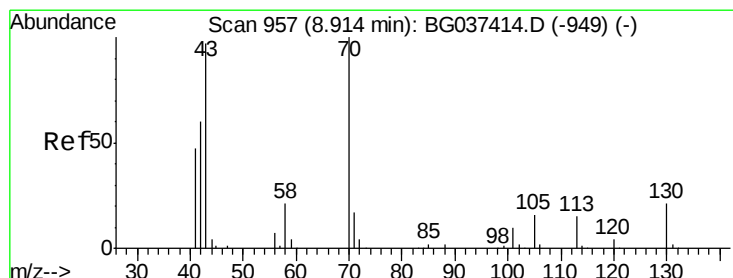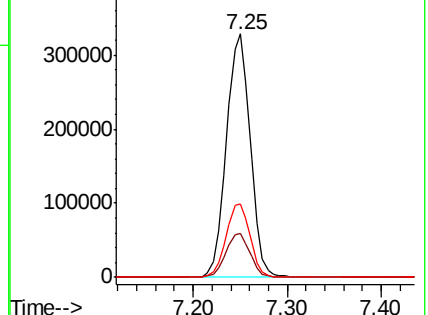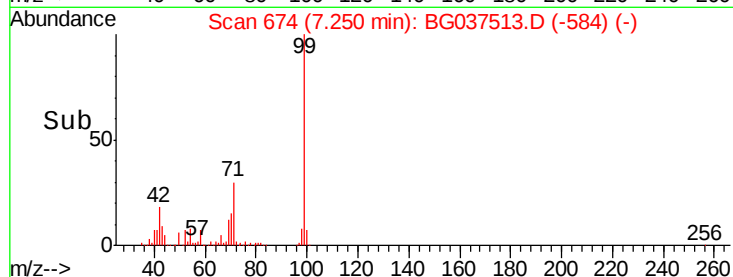

#19

n-Nitroso-di-n-propylamine

Concen: 12.894 ng

RT: 9.28 min Scan# 1020

Delta R.T. 0.37 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Tgt Ion: 70 Resp: 41835


Ion Ratio Lower Upper

70 100



42 47.9 53.9 80.9#

101 0.0 8.2 12.2#

130 2.1 18.2 27.4#

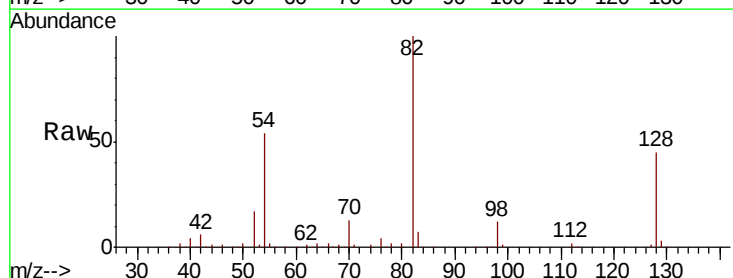

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

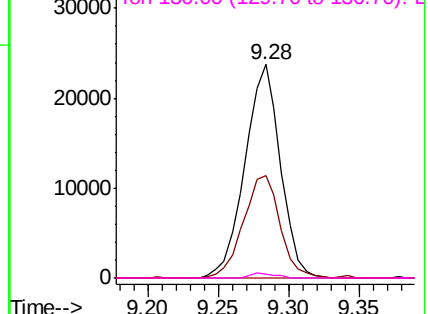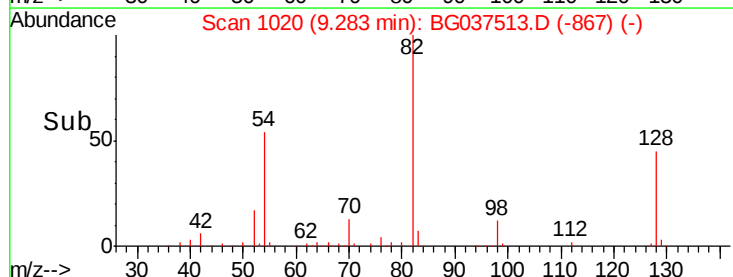






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. -0.00 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	136	Resp:	232383
Ion	Ratio	Lower	Upper
136	100		
137	11.8	9.6	14.4
54	9.9	7.9	11.9
68	6.1	4.8	7.2

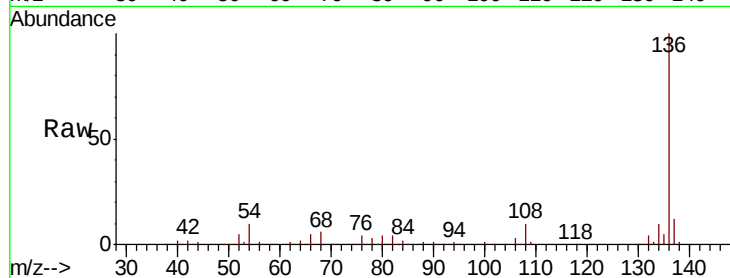


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

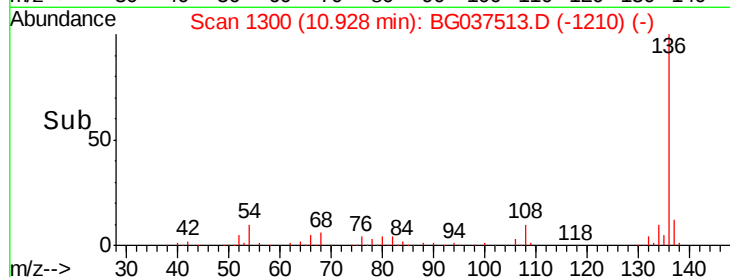
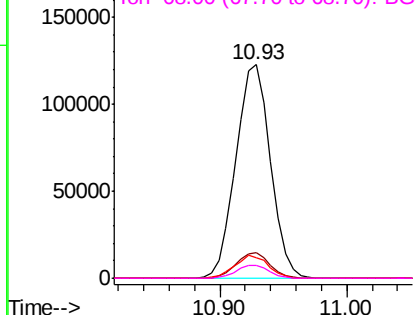



#23
Nitrobenzene-d5
Concen: 79.271 ng
RT: 9.28 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Tgt Ion:	82	Resp:	328839
Ion	Ratio	Lower	Upper
82	100		
128	45.1	34.6	51.8
54	54.4	45.3	67.9

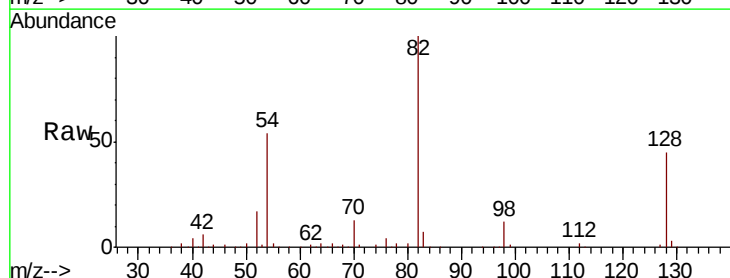

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

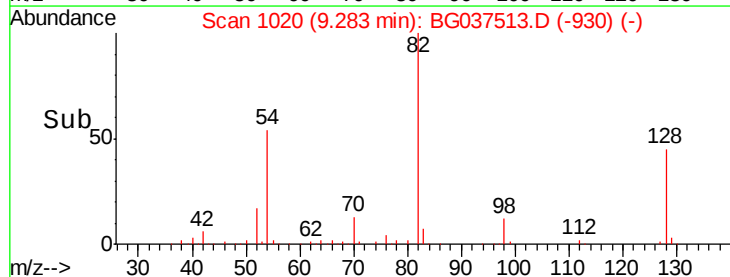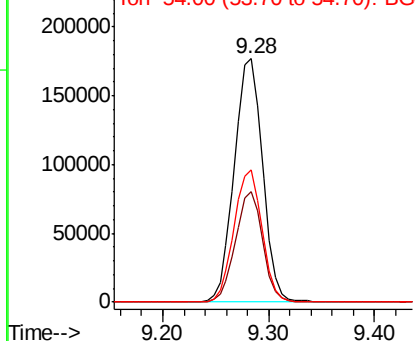



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.74 min Scan# 1948

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 165101

Ion Ratio Lower Upper

164 100

162 104.3 81.3 121.9




160 44.9 36.3 54.5

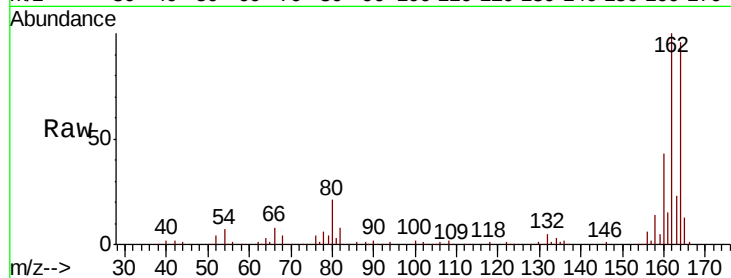

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

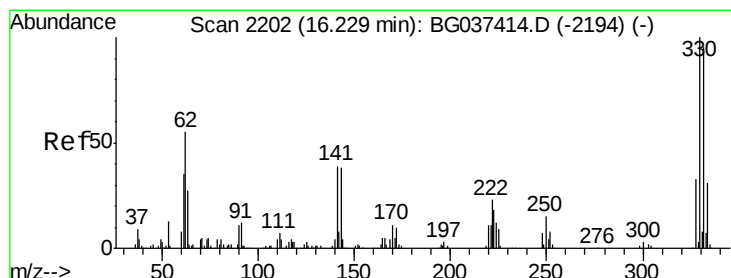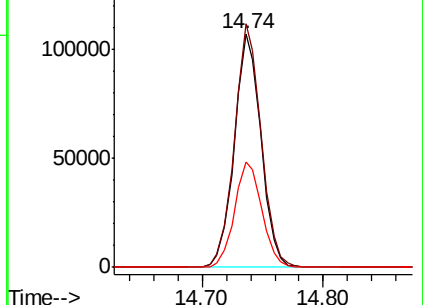

#42

2,4,6-Tribromophenol

Concen: 118.266 ng

RT: 16.23 min Scan# 2202

Delta R.T. -0.00 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09


Tgt Ion:330 Resp: 212967

Ion Ratio Lower Upper

330 100

332 96.8 78.4 117.6



141 40.3 32.2 48.2

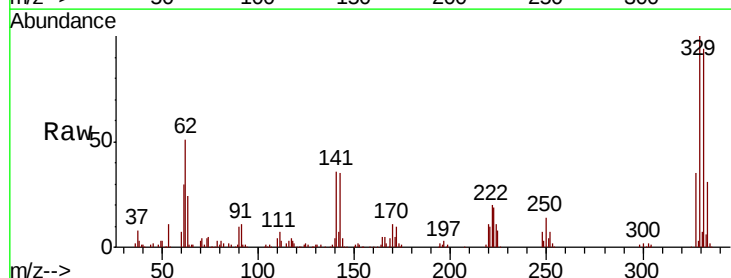

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E


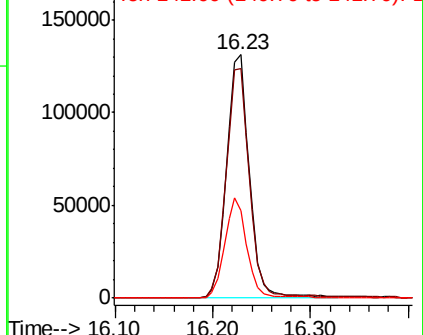





#45
2-Fluorobiphenyl
Concen: 74.844 ng
RT: 13.36 min Scan# 1714
Delta R.T. -0.01 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09




Instrument :
BNA_G
ClientSampleId :

Tot Ion:172 Resp: 819444
Ion Ratio Lower Upper
172 100
171 39.0 31.0 46.4
170 25.8 20.2 30.2

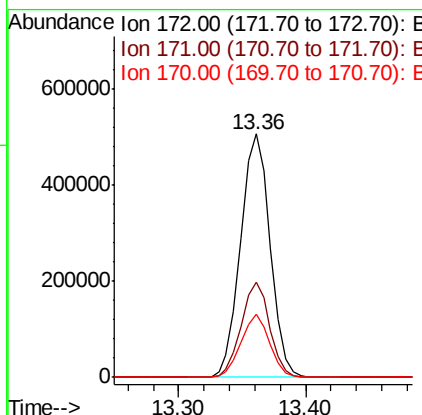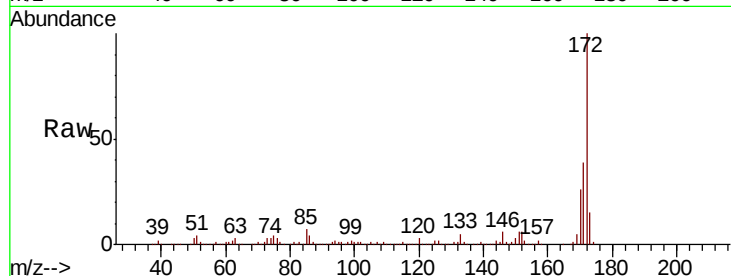

#51
2,6-Dinitrotoluene
Concen: 7.689 ng
RT: 14.74 min Scan# 1948
Delta R.T. 0.42 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Tgt Ion:165 Resp: 21725
Ion Ratio Lower Upper
165 100
63 1.3 43.4 65.2#
89 1.6 45.8 68.6#

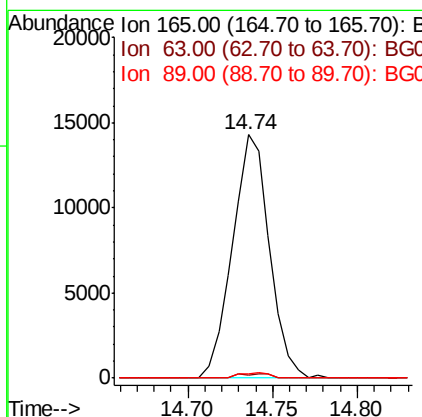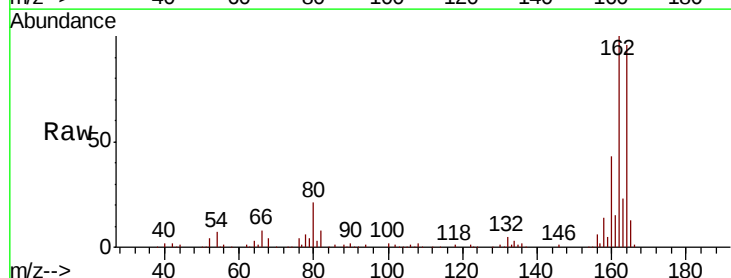




#57
2,4-Dinitrotoluene
Concen: 5.857 ng
RT: 14.74 min Scan# 1948
Delta R.T. -0.36 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.3	33.4	50.0#
89	1.6	57.2	85.8#
182	0.0	2.6	4.0#



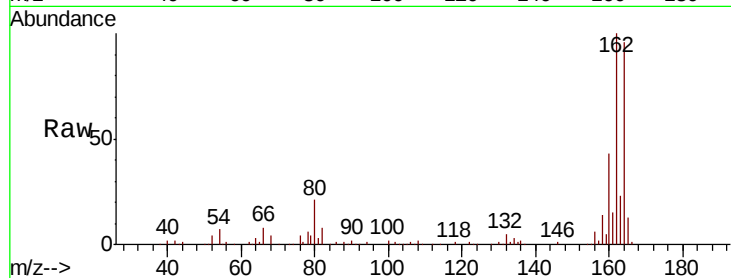


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC


Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

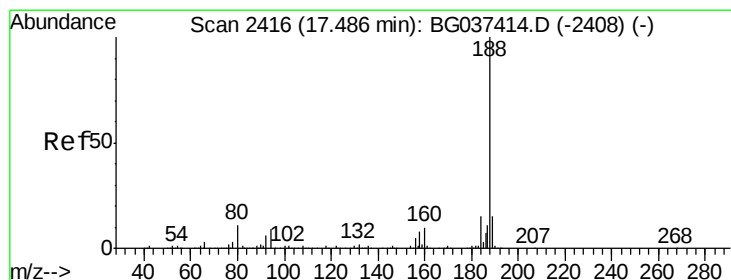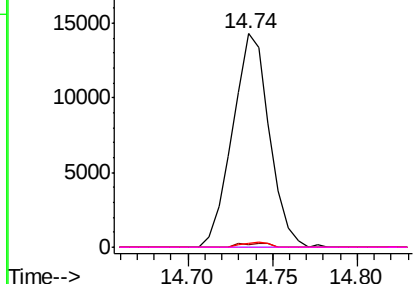

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.49 min Scan# 2416
Delta R.T. -0.00 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09



Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.7	7.2	10.8
80	9.9	7.7	11.5

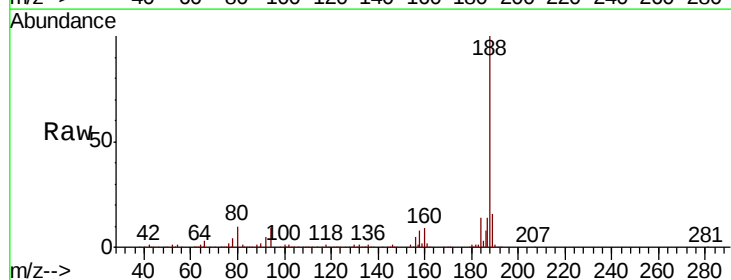

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

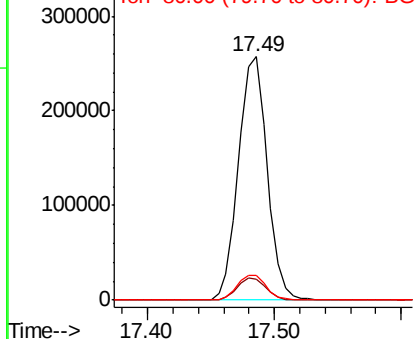






#65
 4,6-Dinitro-2-methylphenol
 Concen: 8.737 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. 0.36 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:198 Resp: 591
 Ion Ratio Lower Upper
 198 100
 51 38.8 22.7 62.7
 105 28.5 19.7 59.7

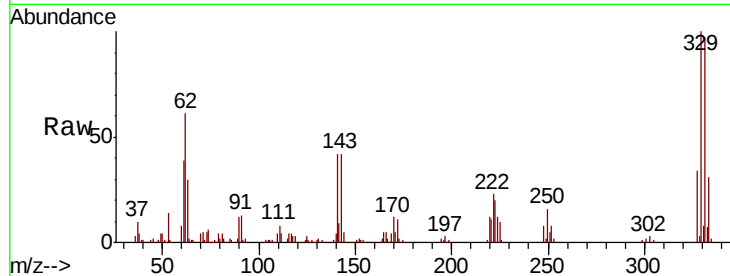


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BG
 Ion 105.00 (104.70 to 105.70): E

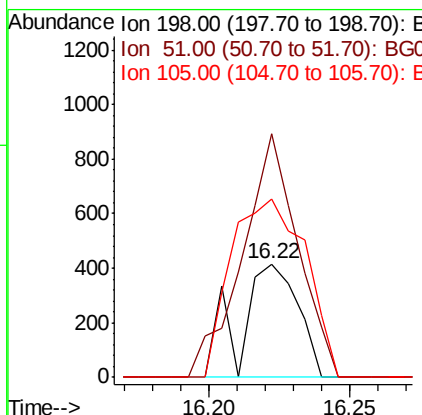
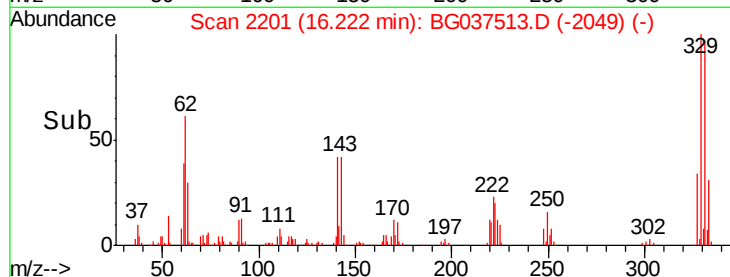



#67
 4-Bromophenyl-phenylether
 Concen: 3.466 ng
 RT: 16.22 min Scan# 2201
 Delta R.T. -0.45 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09

Tgt Ion:248 Resp: 15377
 Ion Ratio Lower Upper
 248 100
 250 208.1 77.0 115.6#
 141 426.5 55.5 83.3#

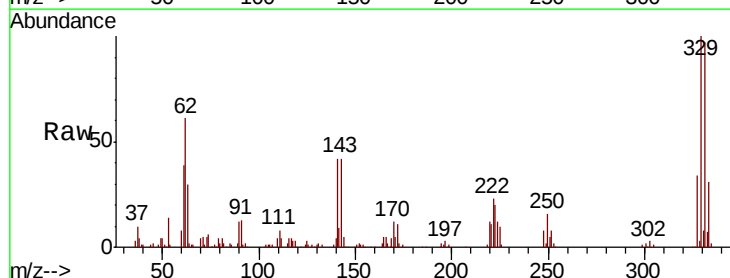

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

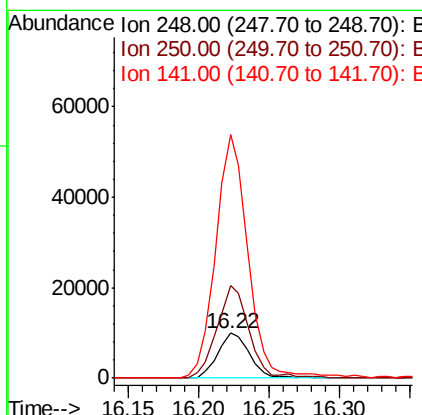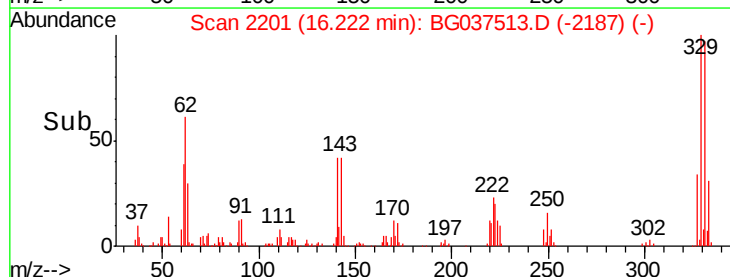

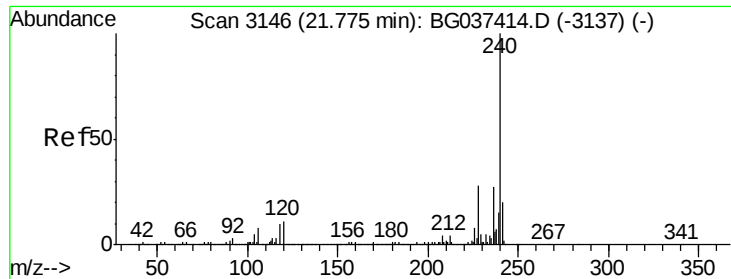

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 370607

Ion Ratio Lower Upper

240 100

120 10.2 8.1 12.1




236 25.8 21.4 32.0

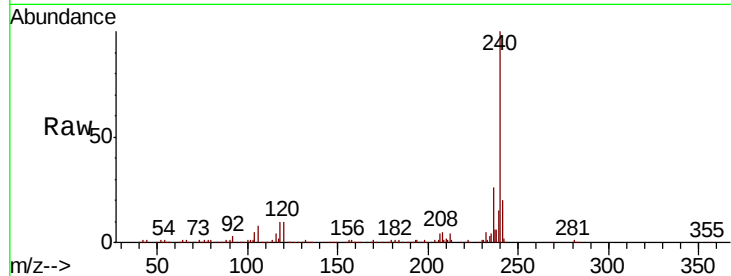

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

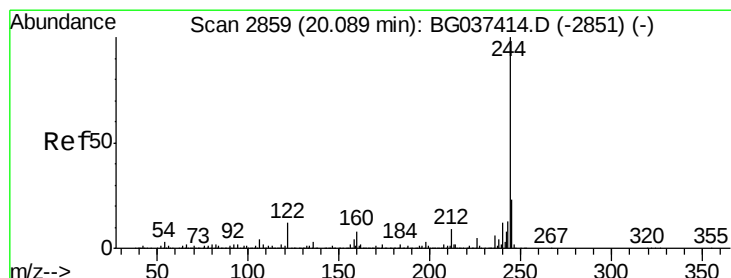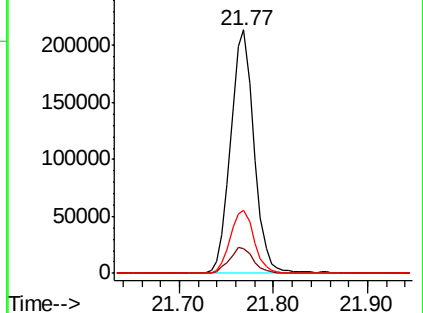

#79

Terphenyl-d14

Concen: 73.873 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09


Tgt Ion:244 Resp: 1281276

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7



122 11.7 9.0 13.4

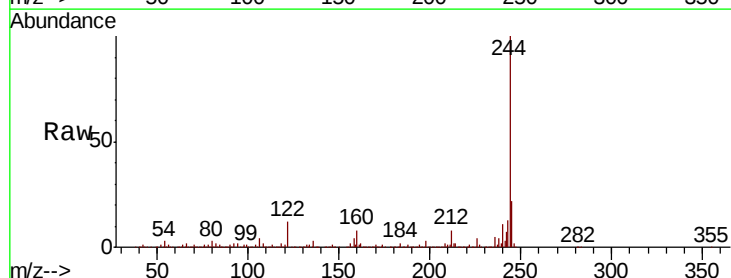


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

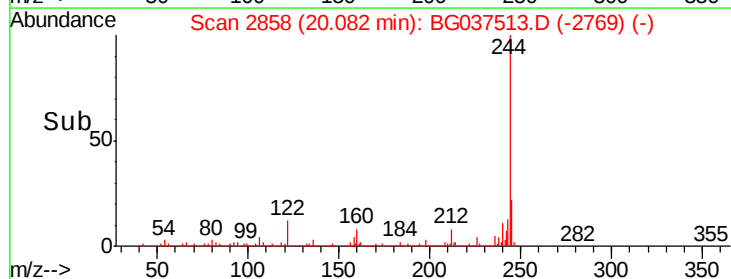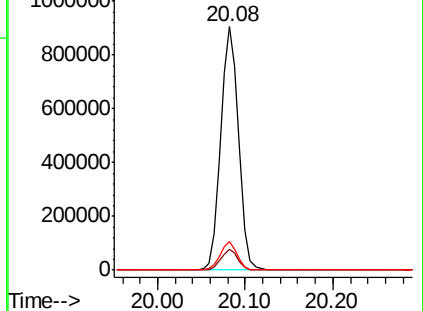

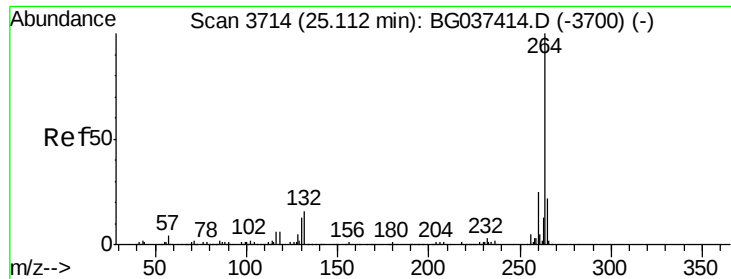

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.10 min Scan# 3712
Delta R.T. -0.01 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.5	18.2	27.4
265	22.0	17.9	26.9

