

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102418\
 Data File : BG037521.D
 Acq On : 24 Oct 2018 21:25
 Operator : JU/SJ
 Sample : J5198-26
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 25 08:01:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	56693	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	242750	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	167522	20.00	ng	0.00
64) Phenanthrene-d10	17.48	188	390566	20.00	ng	0.00
76) Chrysene-d12	21.77	240	363317	20.00	ng	0.00
87) Perylene-d12	25.10	264	337873	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.64	112	407953	120.30	ng	0.00
7) Phenol-d6	7.25	99	537609	104.84	ng	0.00
23) Nitrobenzene-d5	9.28	82	381318	88.00	ng	0.00
42) 2,4,6-Tribromophenol	16.23	330	200626	109.80	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	896063	80.66	ng	0.00
79) Terphenyl-d14	20.08	244	1388493	81.66	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.28	70	47835	13.547	ng	# 72
51) 2,6-Dinitrotoluene	14.73	165	20854	7.274	ng	# 26
57) 2,4-Dinitrotoluene	14.73	165	20854	5.541	ng	# 26
65) 4,6-Dinitro-2-methylphenol	16.22	198	736	8.803	ng	88
67) 4-Bromophenyl-phenylether	16.22	248	14941	3.484	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102418\
Data File : BG037521.D
Acq On : 24 Oct 2018 21:25
Operator : JU/SJ
Sample : J5198-26
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 25 08:01:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

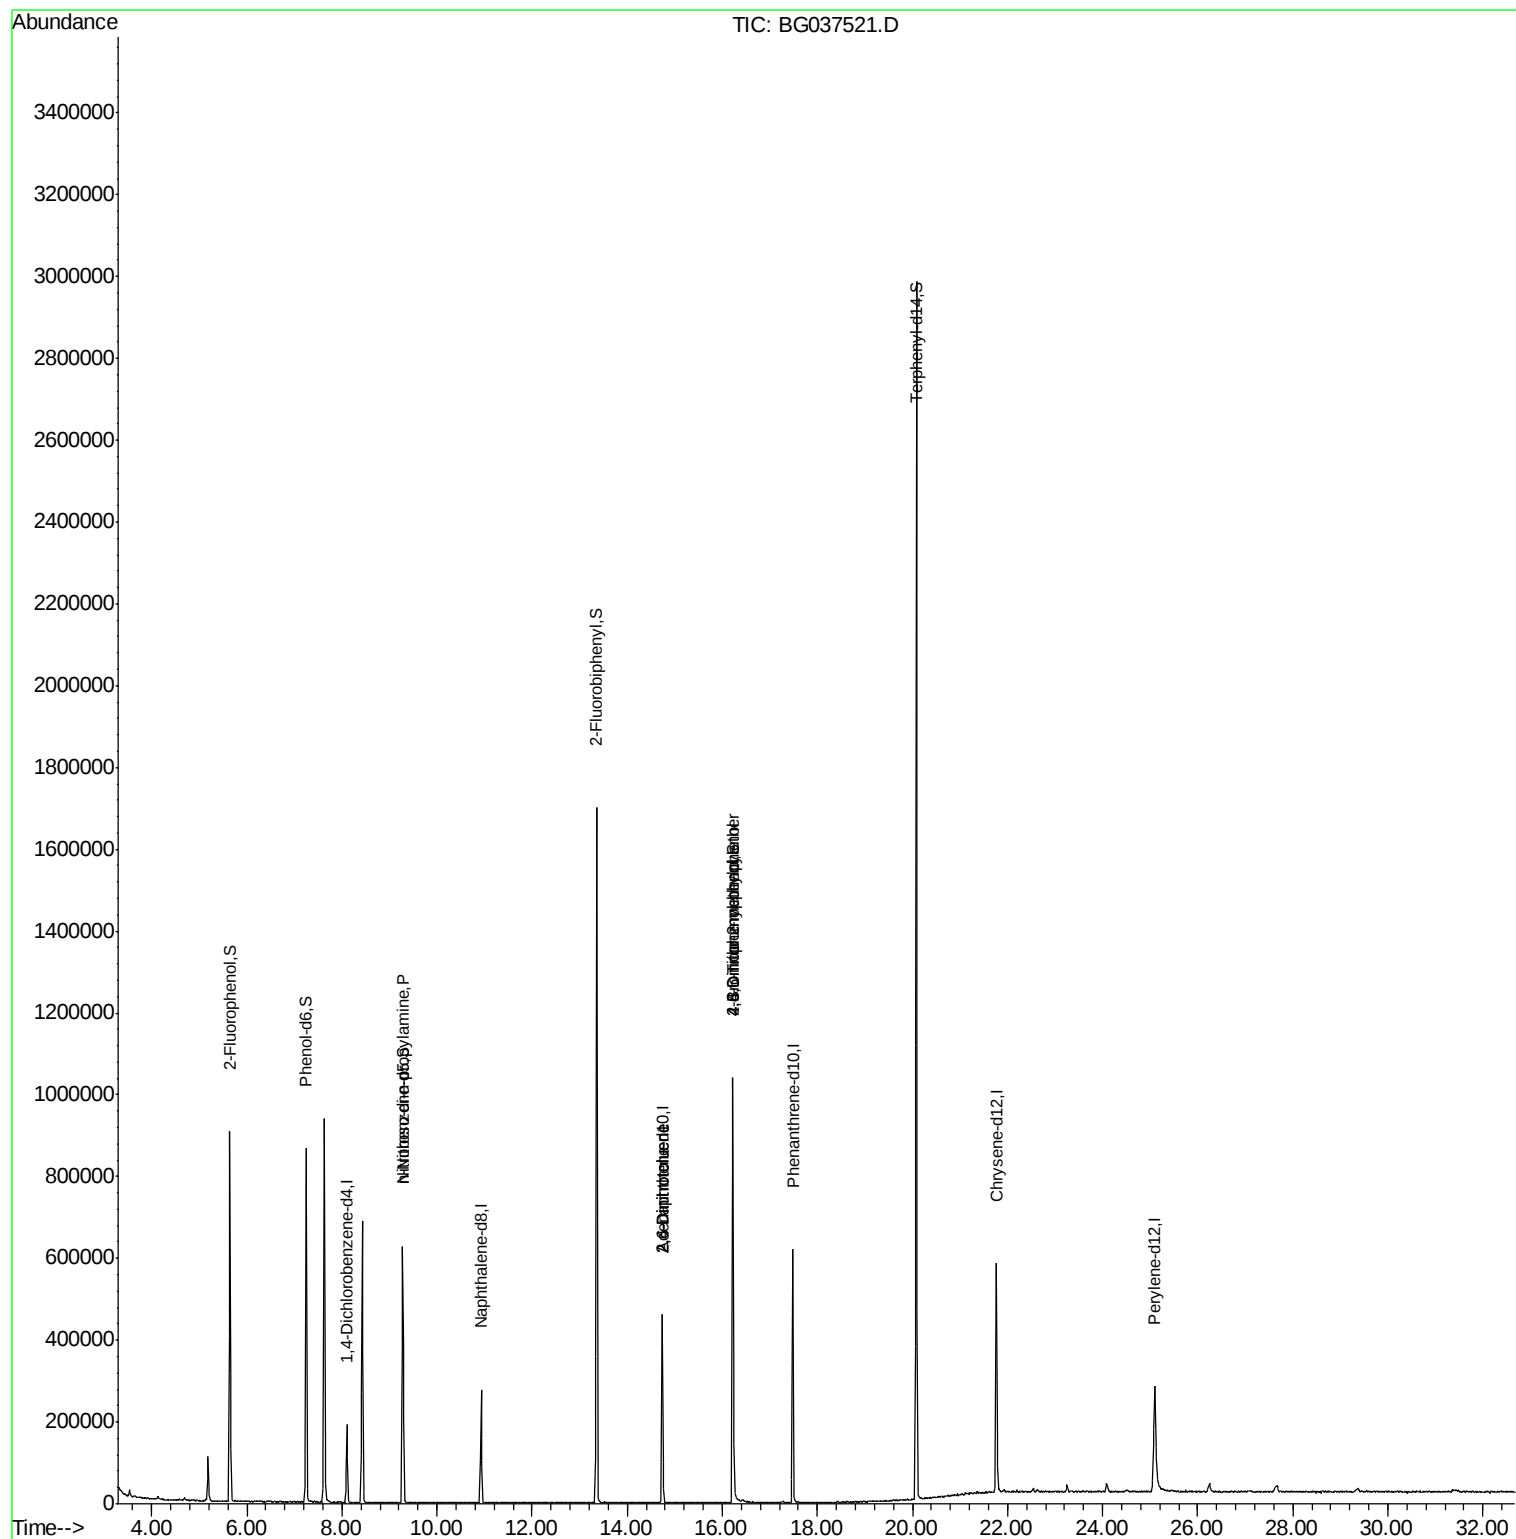


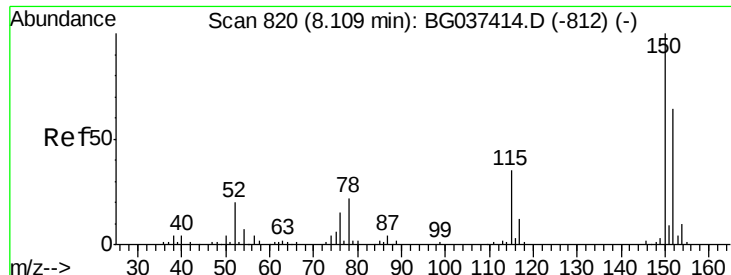




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.11 min Scan# 820
 Delta R.T. -0.00 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:152 Resp: 56693
 Ion Ratio Lower Upper
 152 100
 150 158.1 126.0 189.0
 115 53.2 45.5 68.3

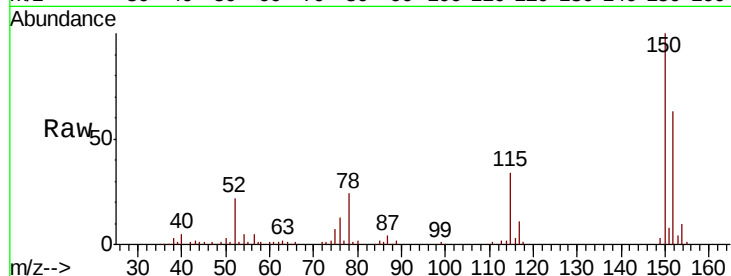


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

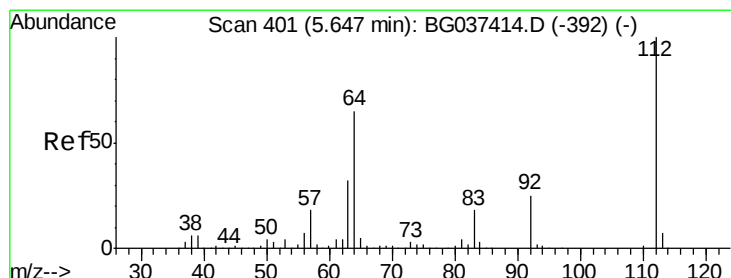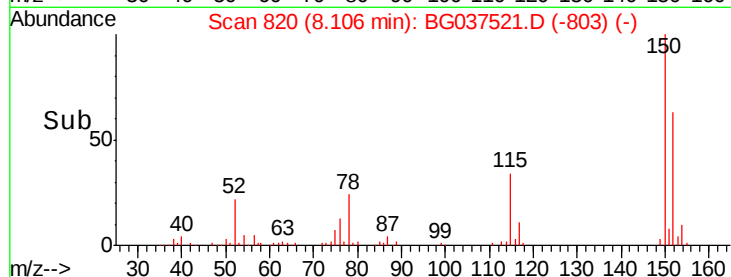
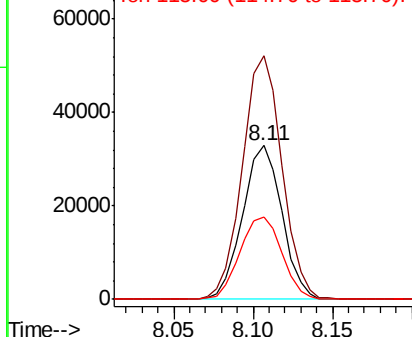


#5
 2-Fluorophenol
 Concen: 120.304 ng
 RT: 5.64 min Scan# 401
 Delta R.T. -0.00 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Tgt Ion:112 Resp: 407953
 Ion Ratio Lower Upper
 112 100
 64 68.3 53.1 79.7
 63 34.6 27.3 40.9

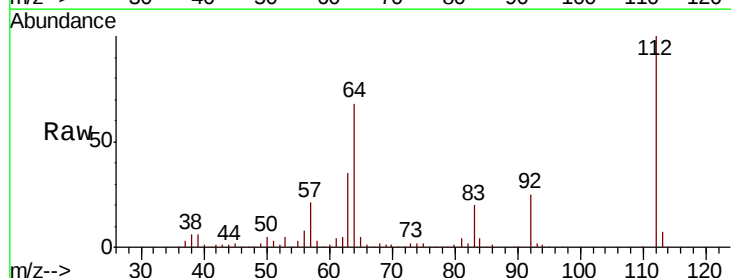

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BGC
 Ion 63.00 (62.70 to 63.70): BGC

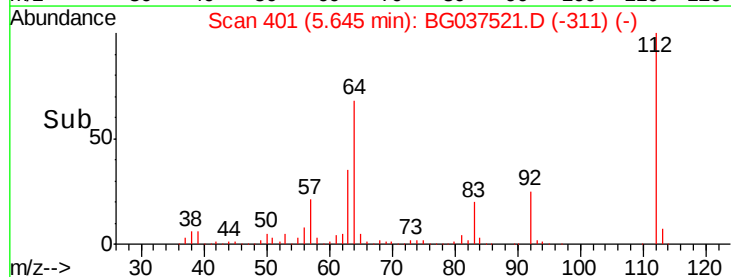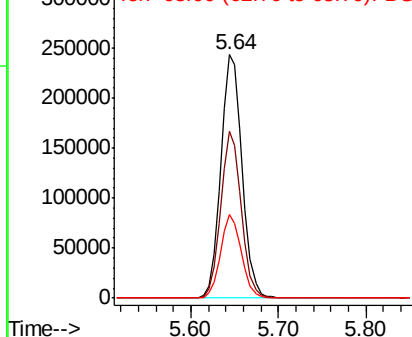



#7

Phenol-d6

Concen: 104.845 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.00 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 537609

Ion Ratio Lower Upper




99 100

42 18.4 15.0 22.4

71 31.2 25.5 38.3

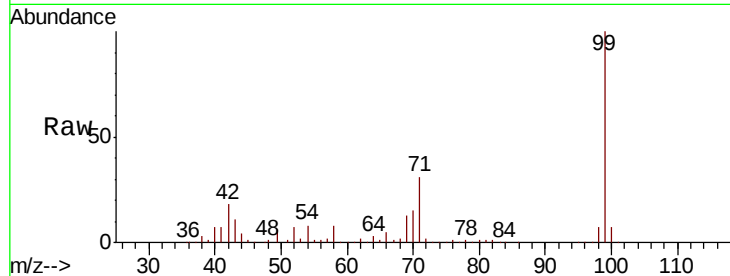

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

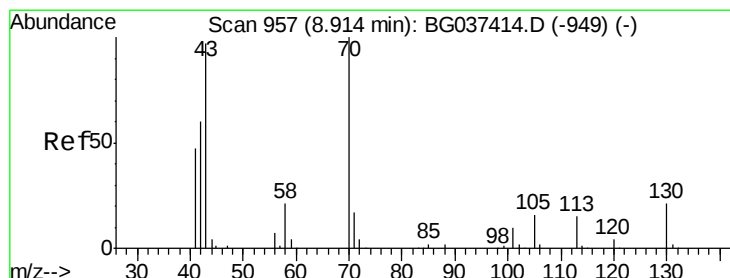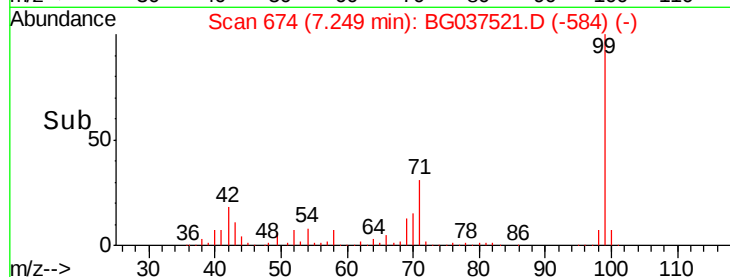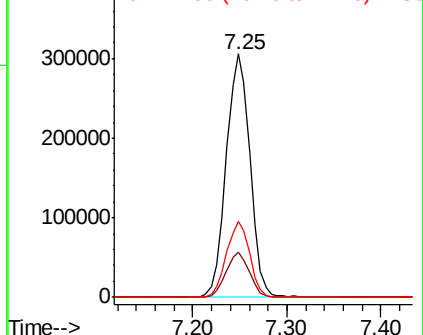

#19

n-Nitroso-di-n-propylamine

Concen: 13.547 ng

RT: 9.28 min Scan# 1020

Delta R.T. 0.37 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25

Tgt Ion: 70 Resp: 47835


Ion Ratio Lower Upper

70 100



42 48.8 53.9 80.9#

101 0.0 8.2 12.2#

130 2.4 18.2 27.4#

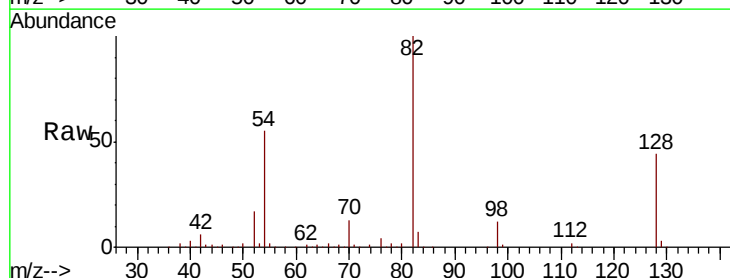

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC



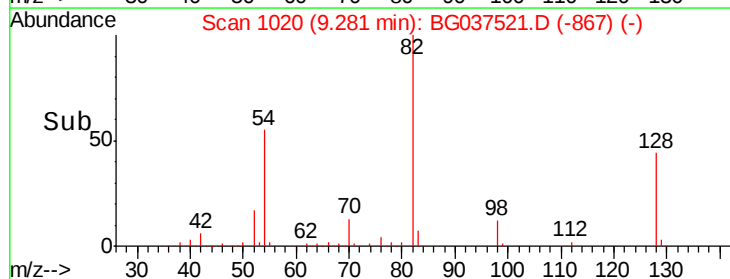
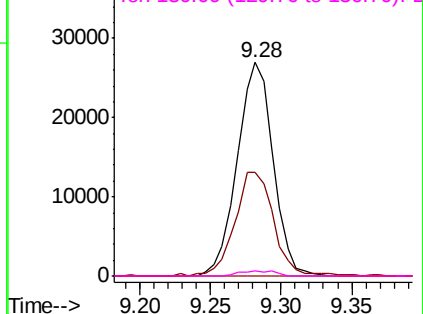




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.93 min Scan# 1300
Delta R.T. -0.00 min
Lab File: BG037521.D
Acq: 24 Oct 2018 21:25




Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	242750
Ion Ratio	Lower	Upper
136 100		
137 11.9	9.6	14.4
54 9.8	7.9	11.9
68 6.5	4.8	7.2

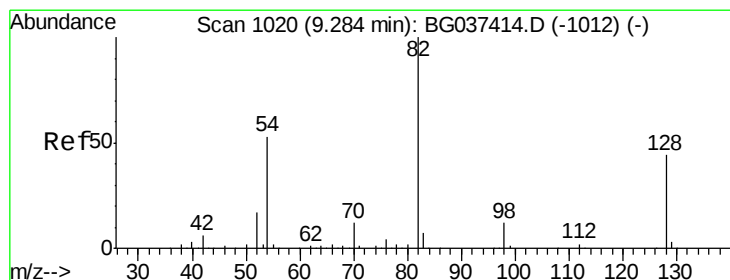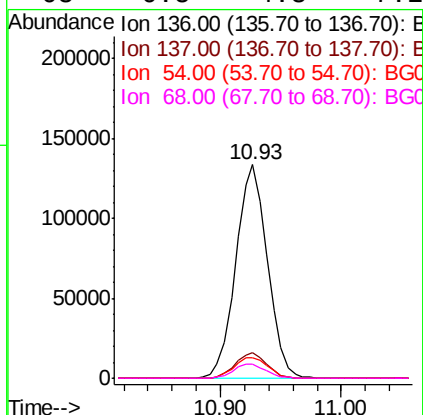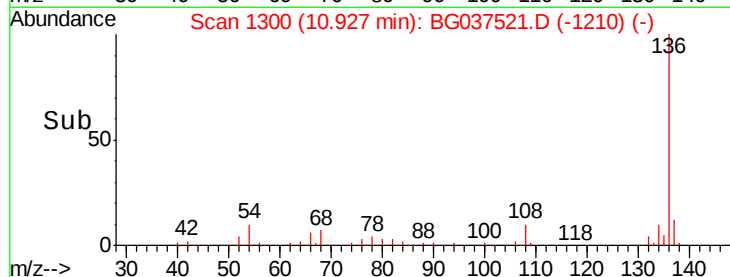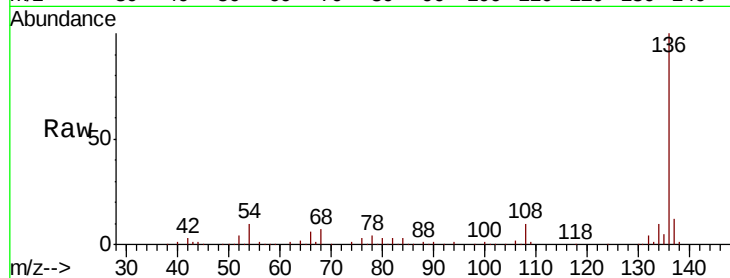

#23
Nitrobenzene-d5
Concen: 87.996 ng
RT: 9.28 min Scan# 1020
Delta R.T. -0.00 min
Lab File: BG037521.D
Acq: 24 Oct 2018 21:25

Tgt Ion: 82	Resp: 381318
Ion Ratio	Lower Upper
82 100	
128 44.3	34.6 51.8
54 54.8	45.3 67.9

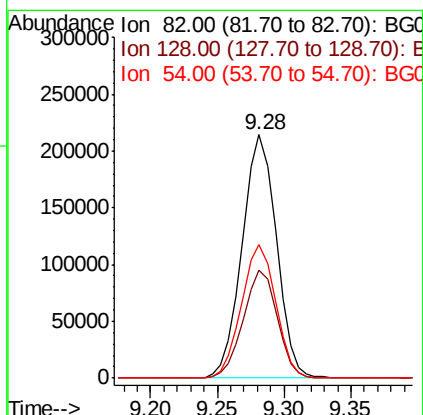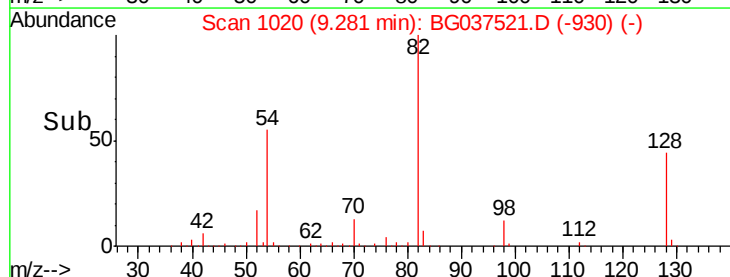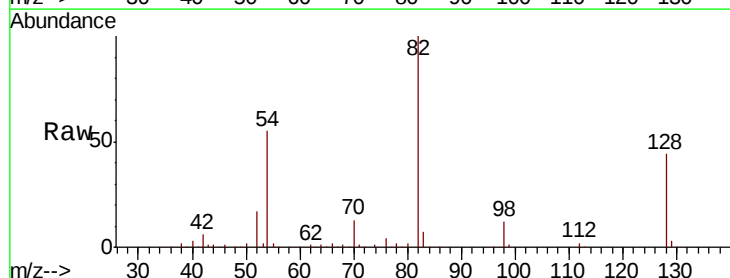



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.74 min Scan# 1949

Delta R.T. -0.00 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 167522

Ion Ratio Lower Upper

164 100

162 101.6 81.3 121.9



160 47.5 36.3 54.5

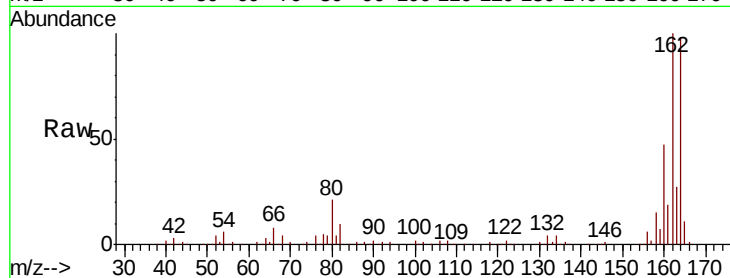

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

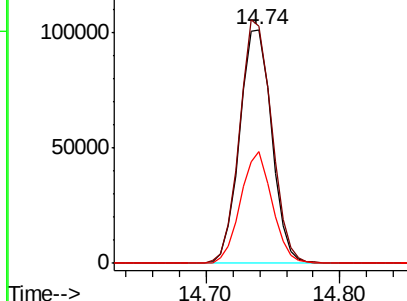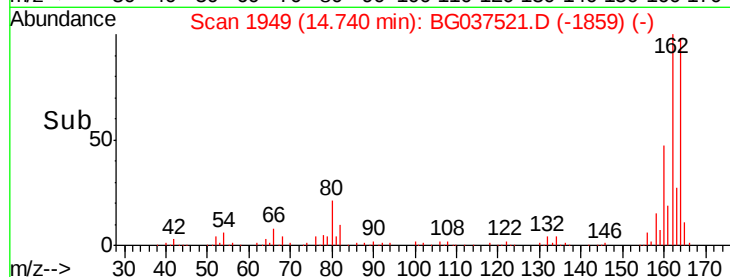

#42

2,4,6-Tribromophenol

Concen: 109.803 ng

RT: 16.23 min Scan# 2202

Delta R.T. -0.00 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25


Tgt Ion:330 Resp: 200626

Ion Ratio Lower Upper

330 100

332 94.9 78.4 117.6



141 39.2 32.2 48.2

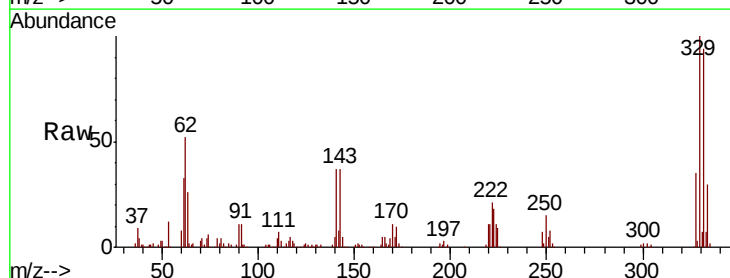

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

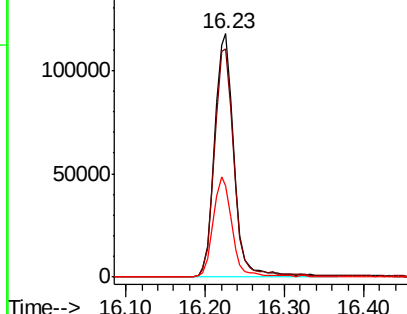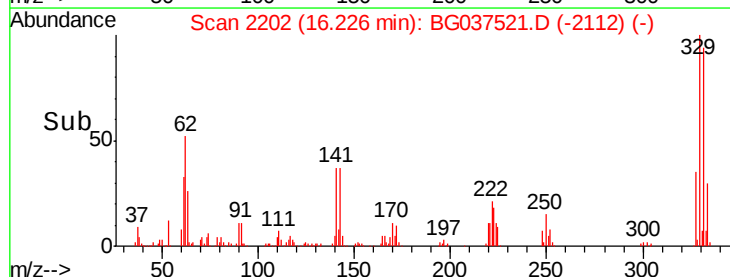







#45
 2-Fluorobiphenyl
 Concen: 80.659 ng
 RT: 13.36 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
172	100		
171	39.0	31.0	46.4
170	25.5	20.2	30.2

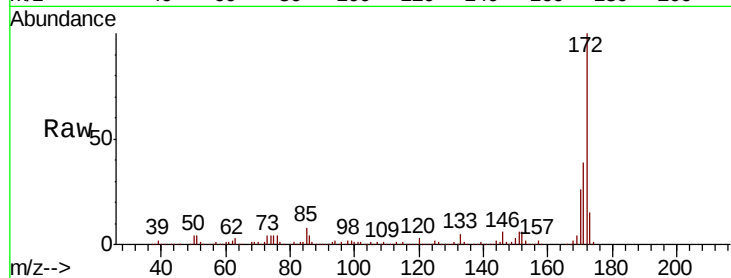


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

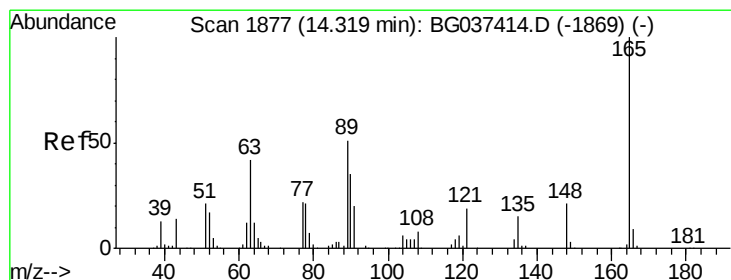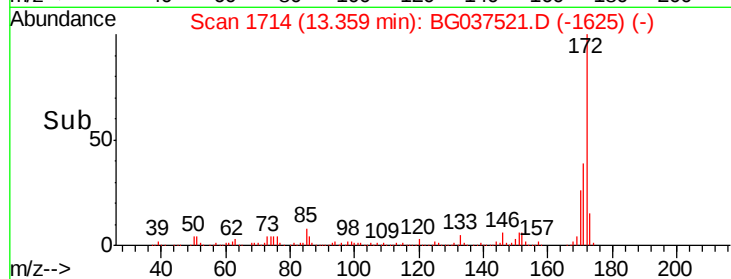
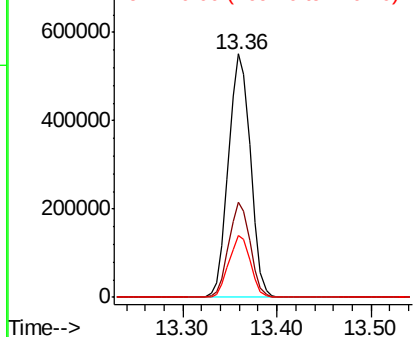


#51
 2,6-Dinitrotoluene
 Concen: 7.274 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. 0.41 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	43.4	65.2#
89	3.3	45.8	68.6#

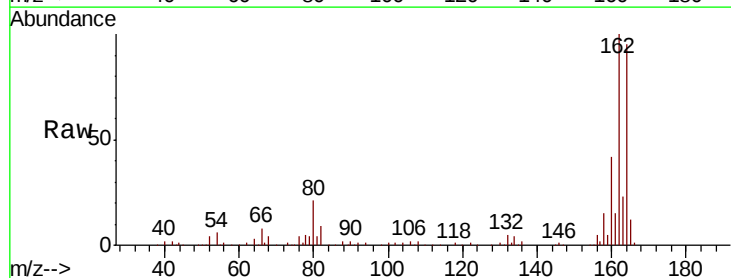

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG
 Ion 89.00 (88.70 to 89.70): BG

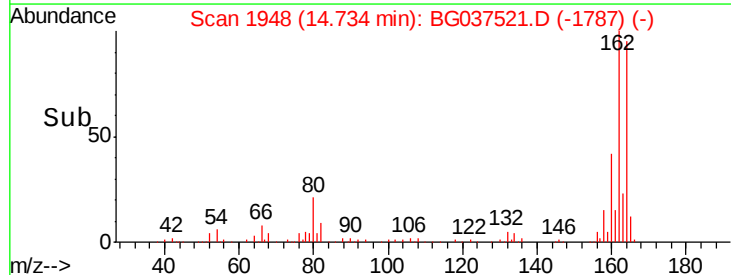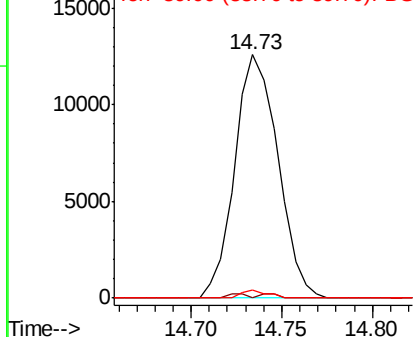







#57
 2,4-Dinitrotoluene
 Concen: 5.541 ng
 RT: 14.73 min Scan# 1948
 Delta R.T. -0.37 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:165	Resp:	20854
Ion Ratio	Lower	Upper
165	100	
63	0.0	33.4 50.0#
89	3.3	57.2 85.8#
182	0.0	2.6 4.0#

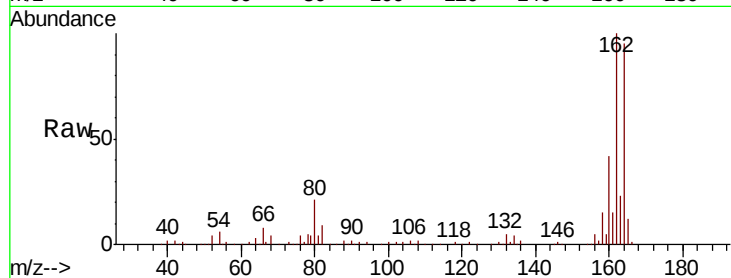


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

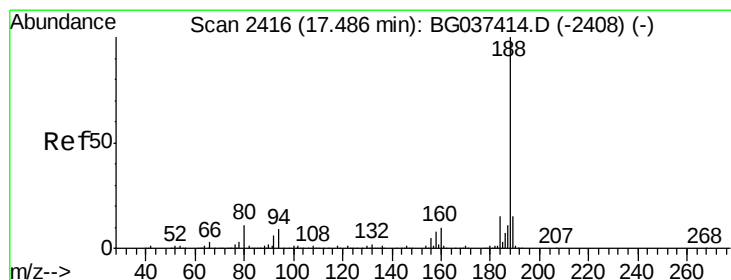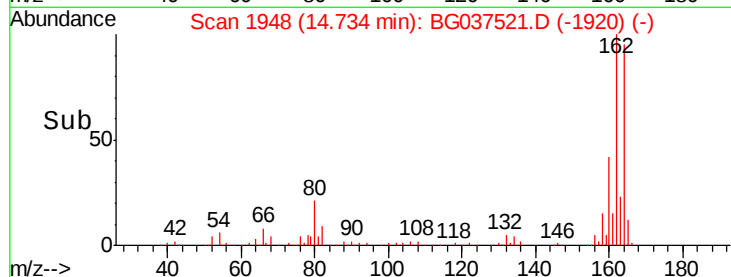
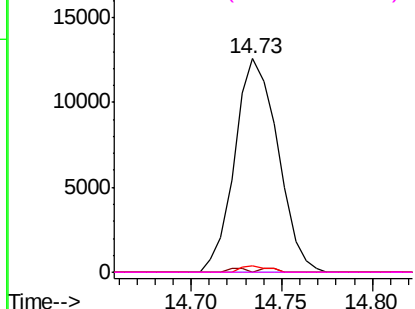



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.48 min Scan# 2416
 Delta R.T. -0.00 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Tgt Ion:188	Resp:	390566
Ion Ratio	Lower	Upper
188	100	
94	9.0	7.2 10.8
80	10.8	7.7 11.5

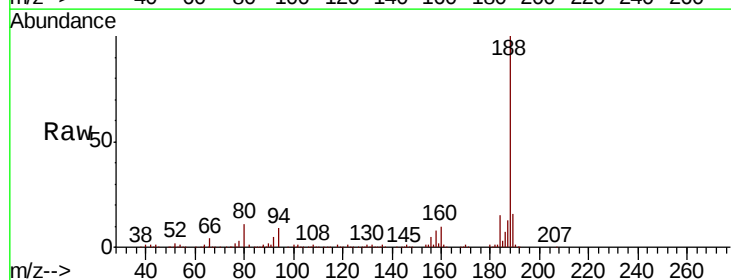

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

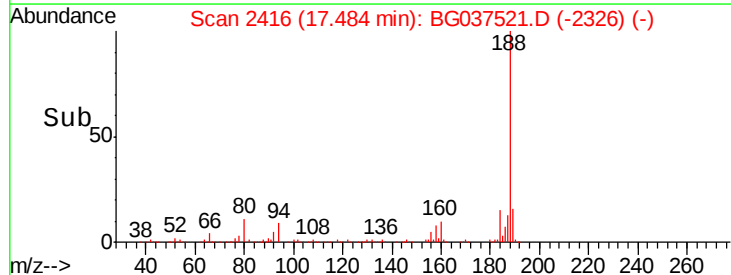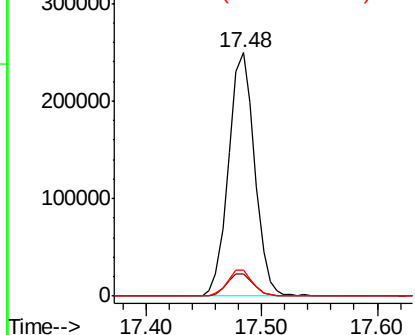

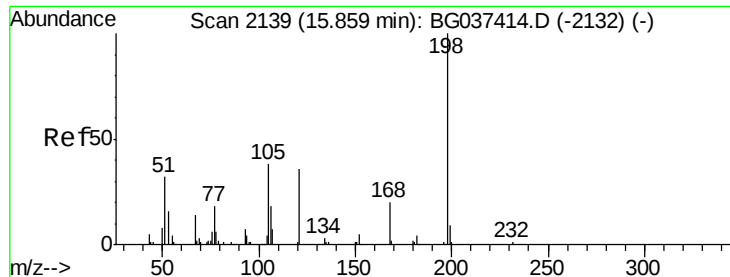

#65

4,6-Dinitro-2-methylphenol

Concen: 8.803 ng

RT: 16.22 min Scan# 2201

Delta R.T. 0.36 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25

Instrument :

BNA_G

ClientSampled :


Tot Ion:198 Resp: 736

Ion Ratio Lower Upper

198 100

51 37.1 22.7 62.7




105 30.1 19.7 59.7

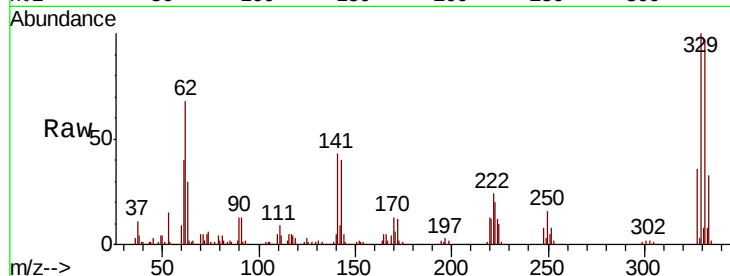

Abundance Ion 198.00 (197.70 to 198.70): E

Ion 51.00 (50.70 to 51.70): BG

Ion 105.00 (104.70 to 105.70): E

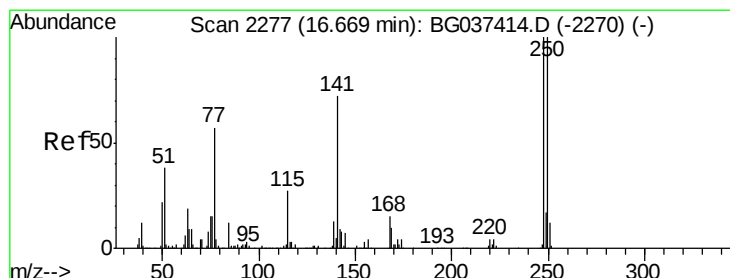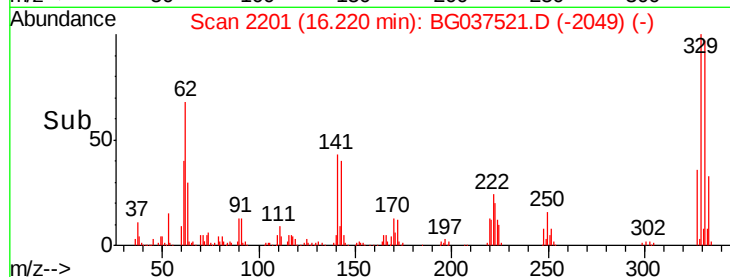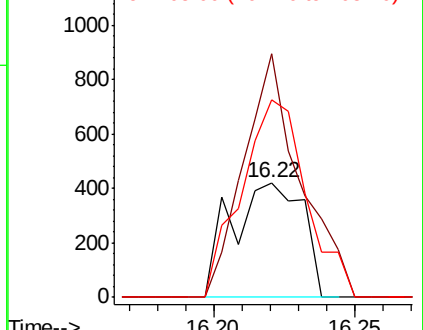

#67

4-Bromophenyl-phenylether

Concen: 3.484 ng

RT: 16.22 min Scan# 2201

Delta R.T. -0.45 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25


Tgt Ion:248 Resp: 14941

Ion Ratio Lower Upper

248 100

250 188.6 77.0 115.6#



141 397.4 55.5 83.3#

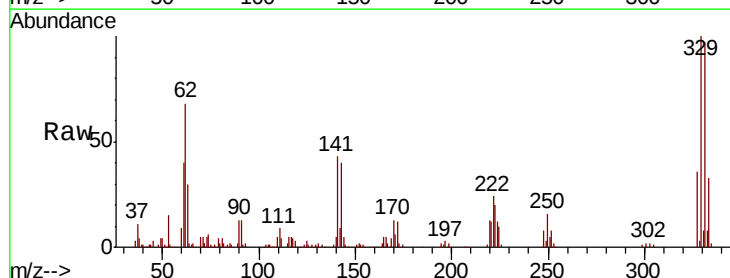


Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

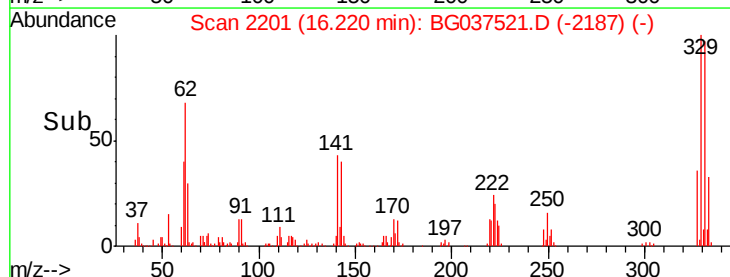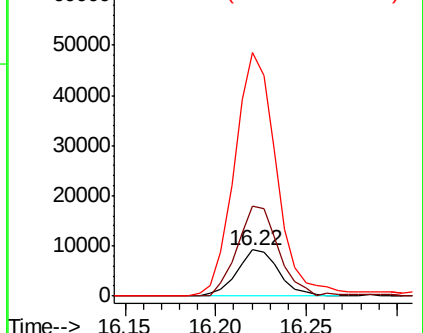

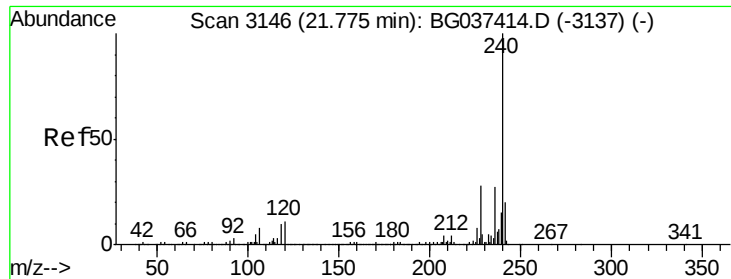

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25

Instrument :

BNA_G

ClientSampled :


Tot Ion:240 Resp: 363317

Ion Ratio Lower Upper

240 100

120 10.7 8.1 12.1




236 26.1 21.4 32.0

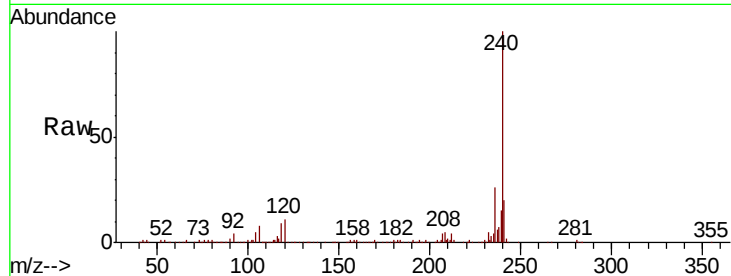

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

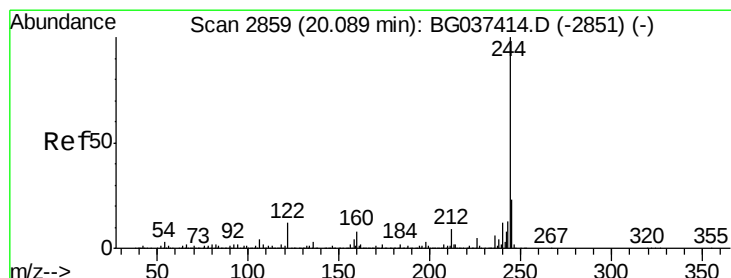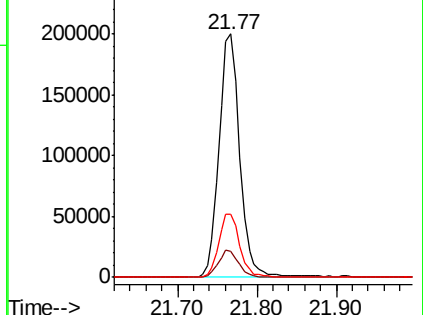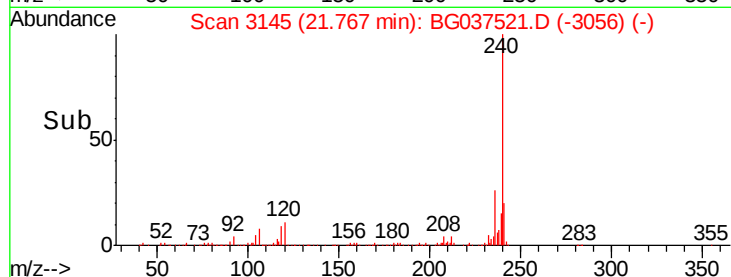

#79

Terphenyl-d14

Concen: 81.661 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037521.D

Acq: 24 Oct 2018 21:25


Tgt Ion:244 Resp: 1388493

Ion Ratio Lower Upper

244 100

212 8.6 6.5 9.7



122 11.6 9.0 13.4

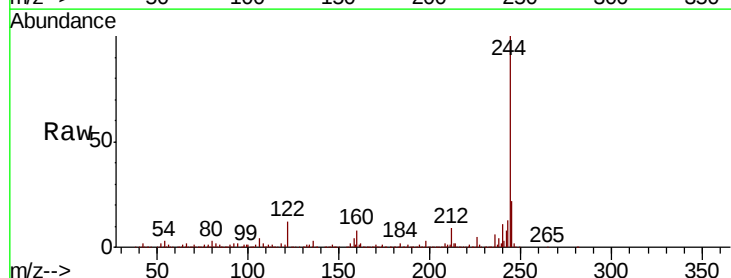

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

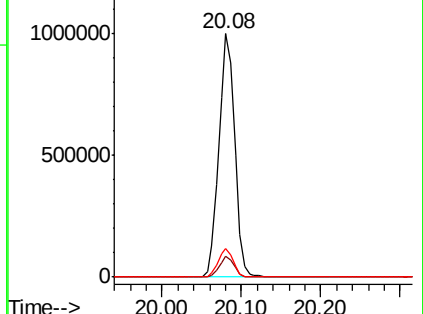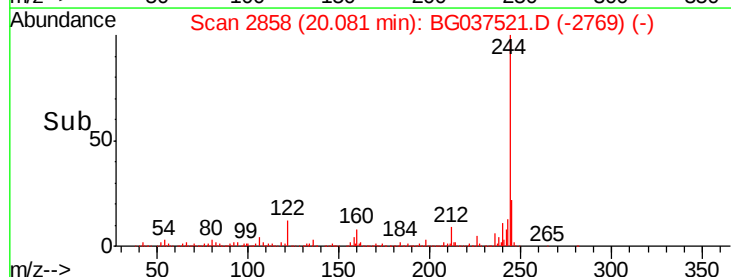



#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.10 min Scan# 3712
 Delta R.T. -0.01 min
 Lab File: BG037521.D
 Acq: 24 Oct 2018 21:25

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.2	27.4
265	19.7	17.9	26.9

