

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102418\
 Data File : BG037513.D
 Acq On : 24 Oct 2018 16:09
 Operator : JU/SJ
 Sample : PB114123BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB114123BL

Quant Time: Oct 25 08:07:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 18 14:06:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.10	152	52092	20.00	ng	0.00
21) Naphthalene-d8	10.93	136	232383	20.00	ng	0.00
39) Acenaphthene-d10	14.74	164	165101	20.00	ng	0.00
64) Phenanthrene-d10	17.49	188	403960	20.00	ng	0.00
76) Chrysene-d12	21.77	240	370607	20.00	ng	0.00
87) Perylene-d12	25.10	264	358856	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	390328	125.27	ng	0.00
7) Phenol-d6	7.25	99	580899	123.29	ng	0.00
23) Nitrobenzene-d5	9.28	82	328839	79.27	ng	0.00
42) 2,4,6-Tribromophenol	16.23	330	212967	118.27	ng	0.00
45) 2-Fluorobiphenyl	13.36	172	819444	74.84	ng	0.00
79) Terphenyl-d14	20.08	244	1281276	73.87	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102418\
Data File : BG037513.D
Acq On : 24 Oct 2018 16:09
Operator : JU/SJ
Sample : PB114123BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB114123BL

Quant Time: Oct 25 08:07:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 18 14:06:42 2018
Response via : Initial Calibration

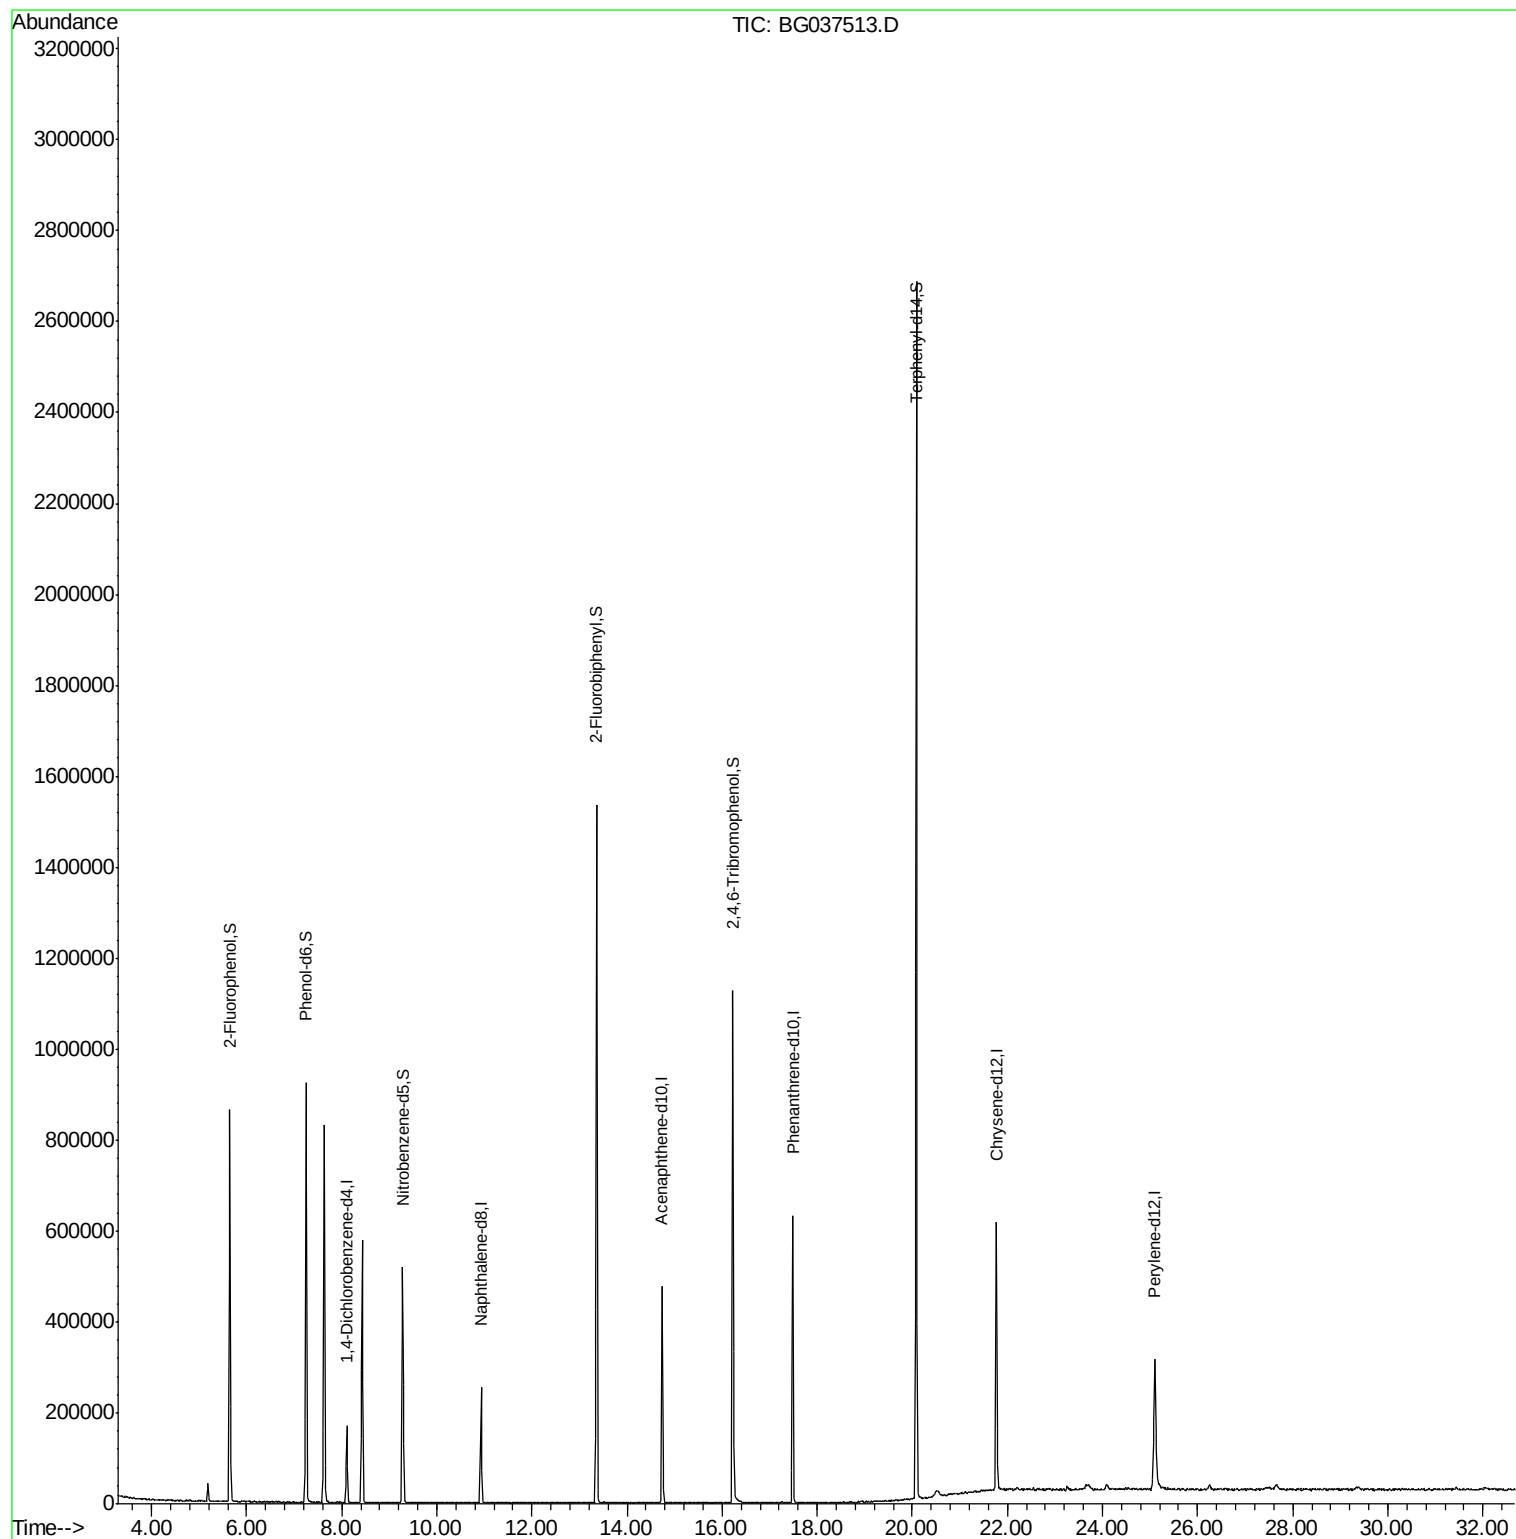

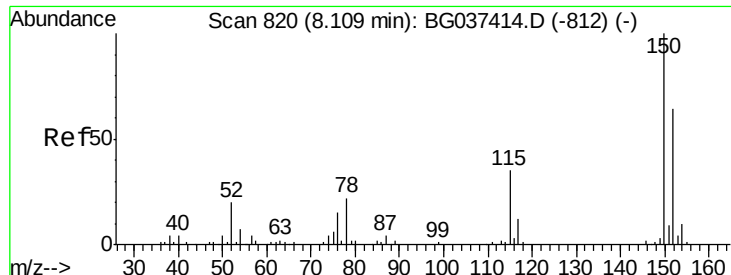


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.10 min Scan# 819
Delta R.T. -0.01 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Instrument :
BNA_G
ClientSampleId :
PB114123BL

Tgt Ion:152 Resp: 52092
Ion Ratio Lower Upper
152 100
150 162.9 126.0 189.0
115 54.1 45.5 68.3

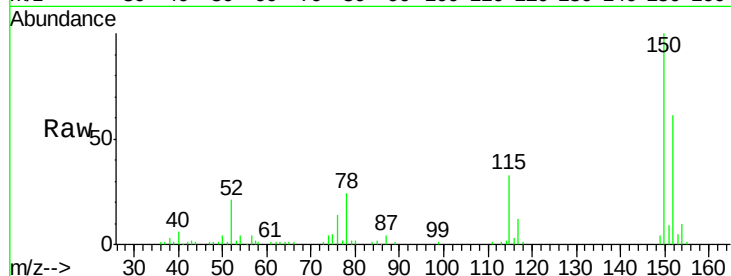


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

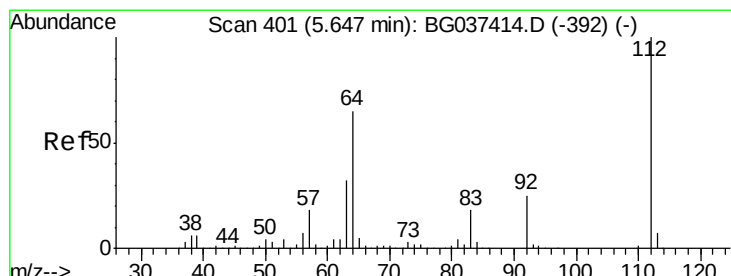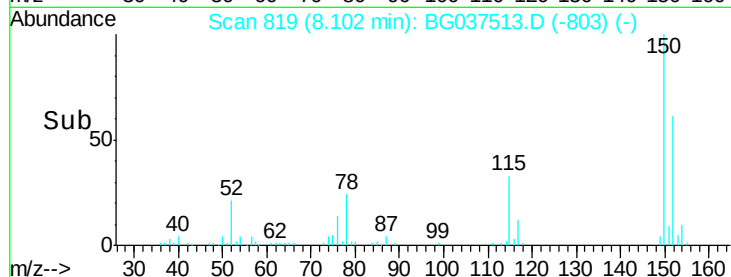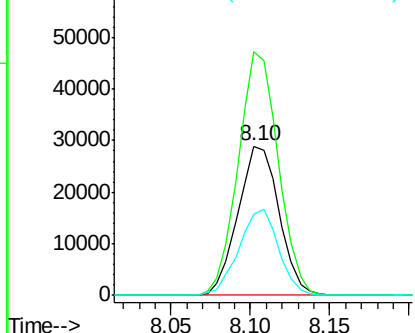



#5


2-Fluorophenol
Concen: 125.273 ng
RT: 5.65 min Scan# 401
Delta R.T. -0.00 min
Lab File: BG037513.D
Acq: 24 Oct 2018 16:09

Tgt Ion:112 Resp: 390328
Ion Ratio Lower Upper
112 100
64 66.5 53.1 79.7
63 32.8 27.3 40.9

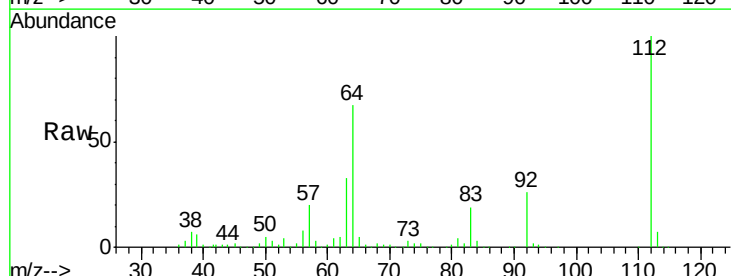

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

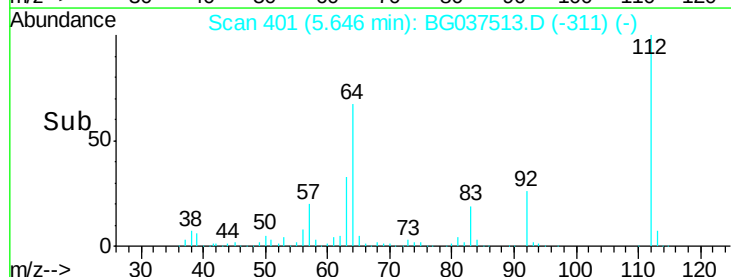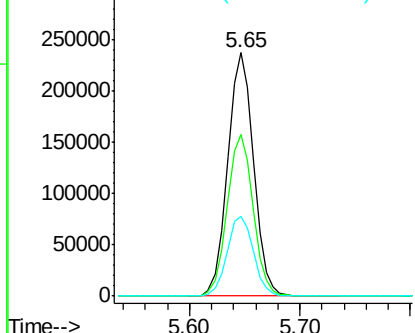

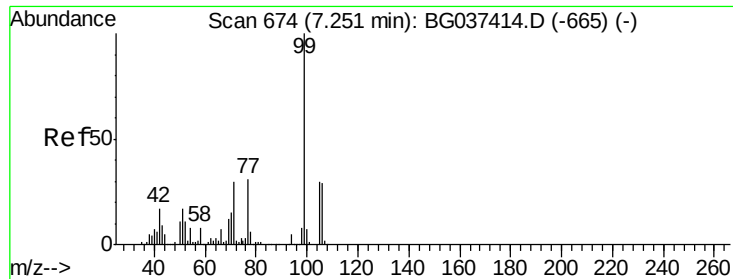

#7

Phenol-d6

Concen: 123.293 ng

RT: 7.25 min Scan# 674

Delta R.T. -0.00 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampleId :

PB114123BL


Tgt Ion: 99 Resp: 580899

Ion Ratio Lower Upper




99 100

42 18.2 15.0 22.4

71 30.1 25.5 38.3

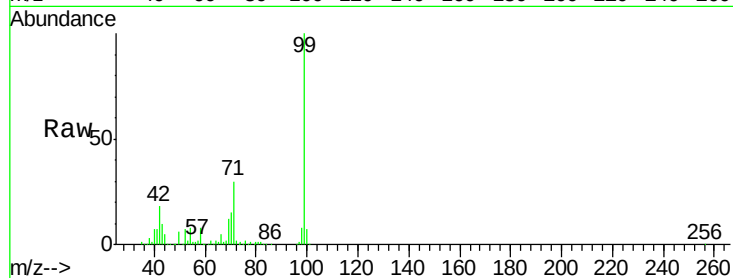

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

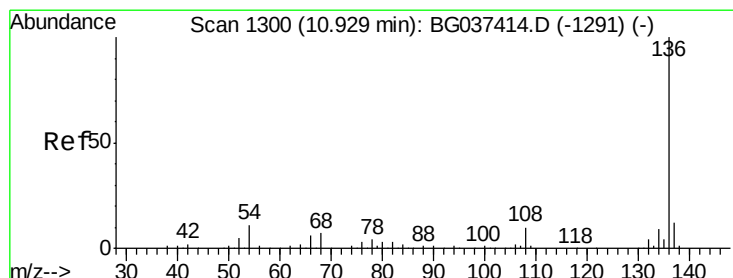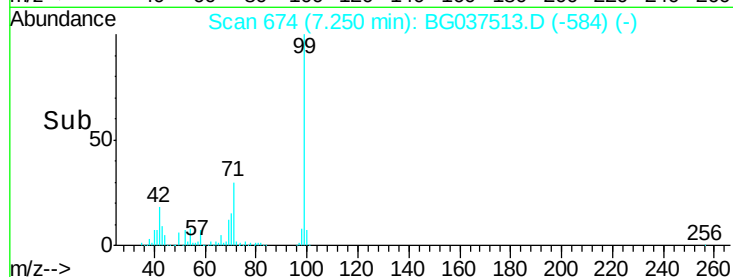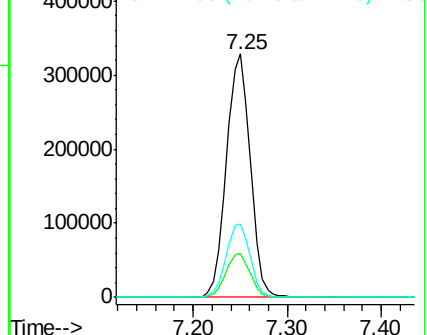

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.93 min Scan# 1300

Delta R.T. -0.00 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Tgt Ion: 136 Resp: 232383


Ion Ratio Lower Upper

136 100



137 11.8 9.6 14.4


54 9.9 7.9 11.9

68 6.1 4.8 7.2

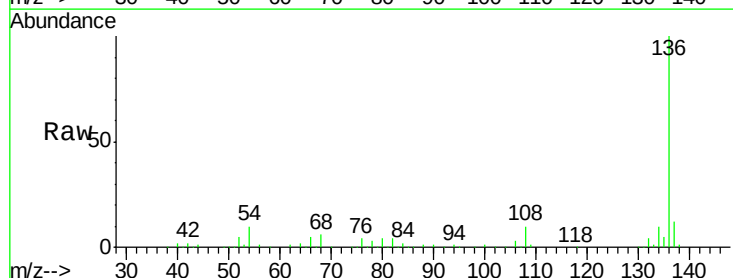

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

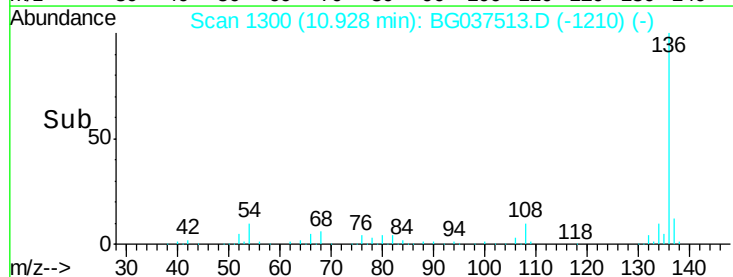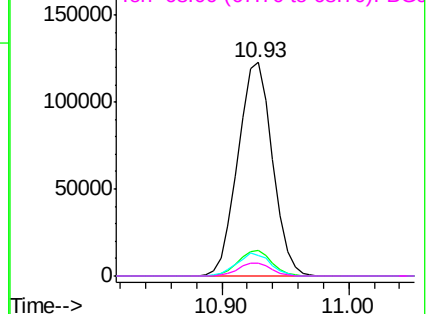


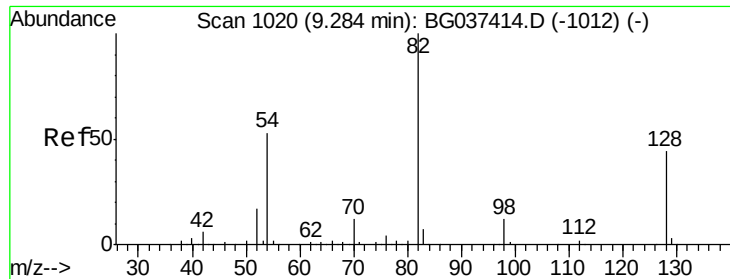




#23
 Nitrobenzene-d5
 Concen: 79.271 ng
 RT: 9.28 min Scan# 1020
 Delta R.T. -0.00 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09

Instrument :
 BNA_G
 ClientSampleId :
 PB114123BL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	45.1	34.6	51.8
54	54.4	45.3	67.9

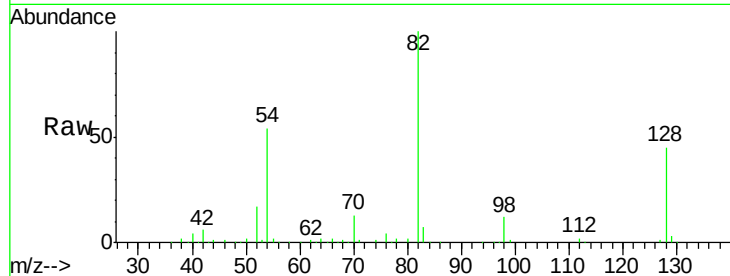


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

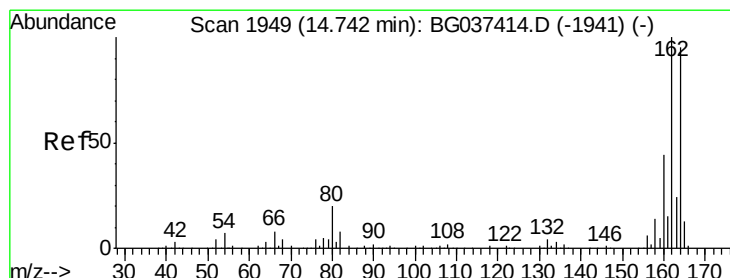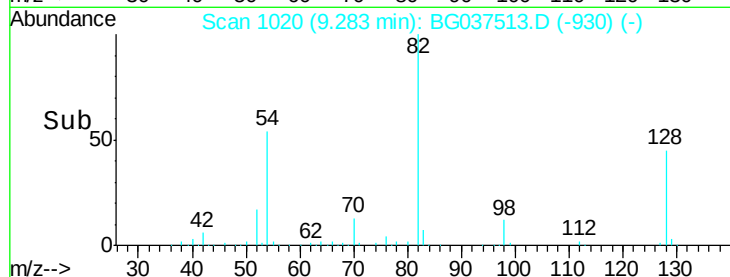
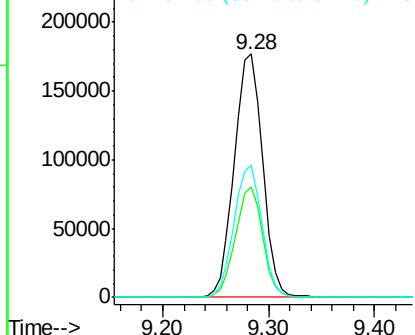



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.74 min Scan# 1948
 Delta R.T. -0.01 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.3	81.3	121.9
160	44.9	36.3	54.5

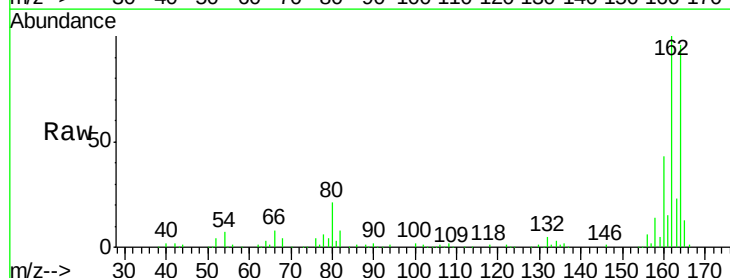

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC



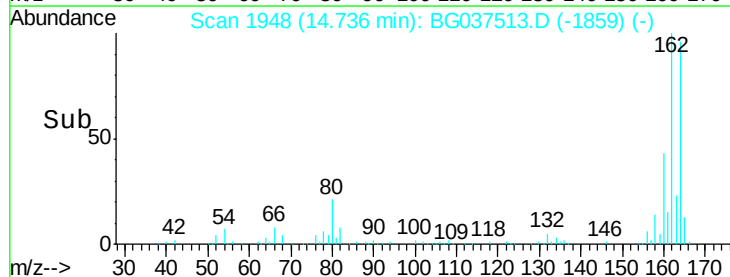
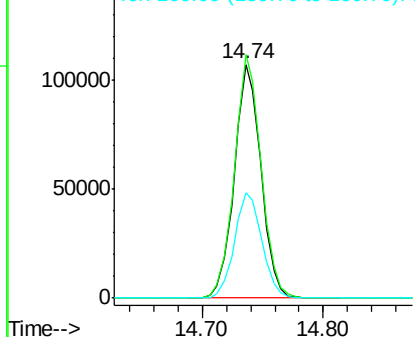


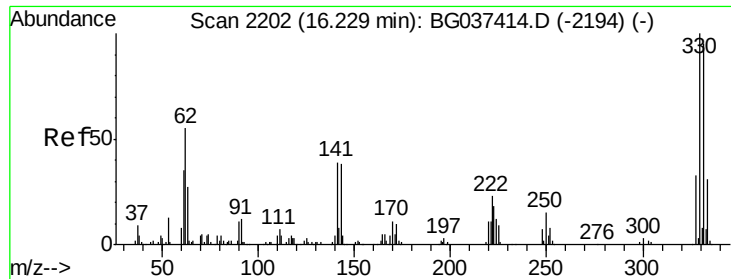

#42
 2,4,6-Tribromophenol
 Concen: 118.266 ng
 RT: 16.23 min Scan# 2202
 Delta R.T. -0.00 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09




Instrument :
 BNA_G
 ClientSampleId :
 PB114123BL


Tgt Ion:330 Resp: 212967
 Ion Ratio Lower Upper
 330 100
 332 96.8 78.4 117.6
 141 40.3 32.2 48.2

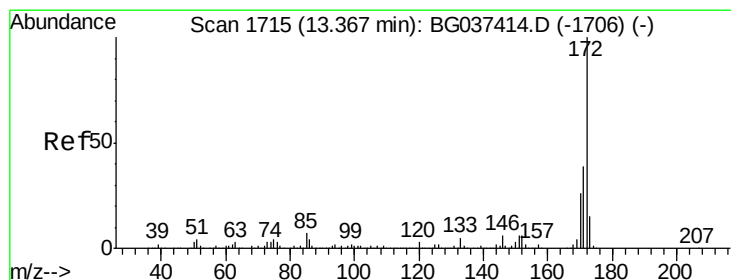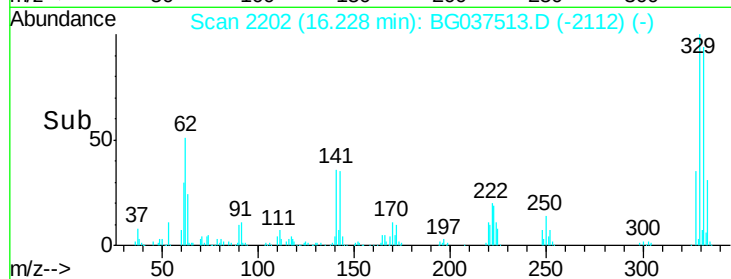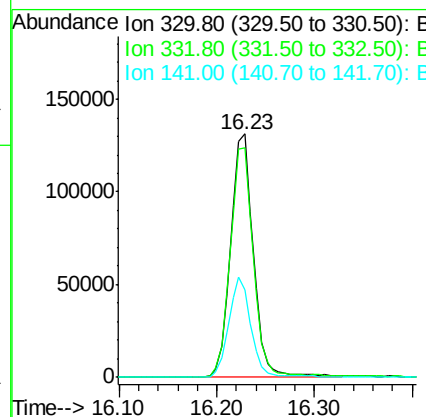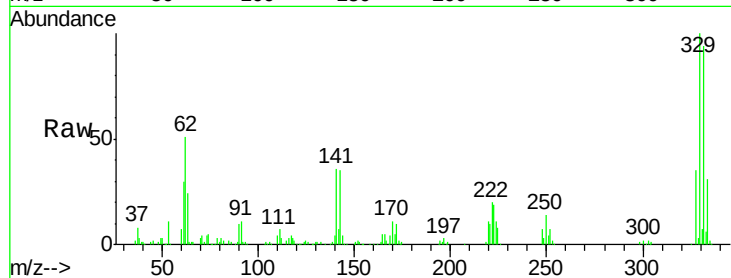

#45
 2-Fluorobiphenyl
 Concen: 74.844 ng
 RT: 13.36 min Scan# 1714
 Delta R.T. -0.01 min
 Lab File: BG037513.D
 Acq: 24 Oct 2018 16:09

Tgt Ion:172 Resp: 819444
 Ion Ratio Lower Upper
 172 100
 171 39.0 31.0 46.4
 170 25.8 20.2 30.2

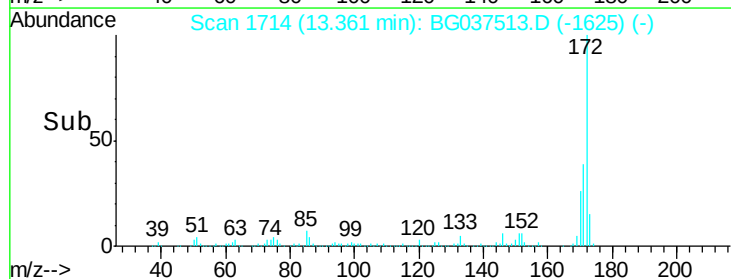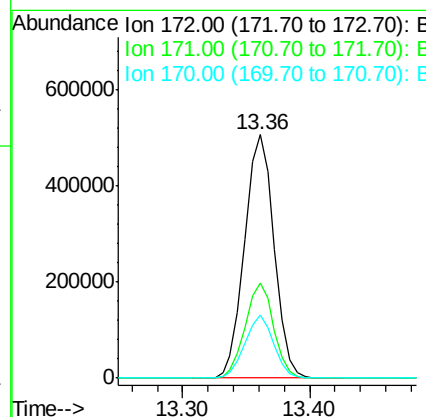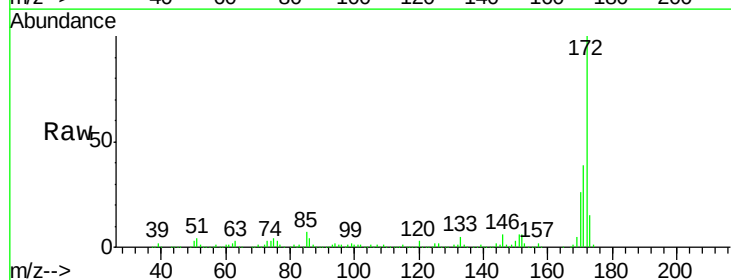

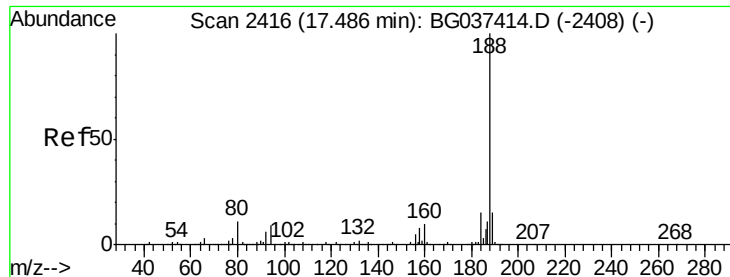

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.49 min Scan# 2416

Delta R.T. -0.00 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampleId :

PB114123BL


Tgt Ion:188 Resp: 403960

Ion Ratio Lower Upper

188 100

94 8.7 7.2 10.8




80 9.9 7.7 11.5

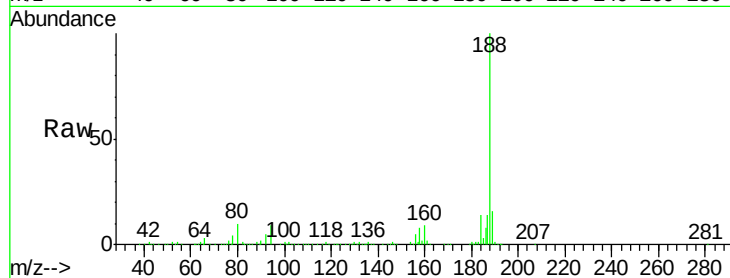

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

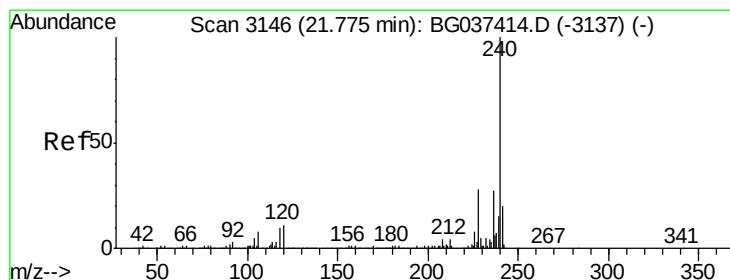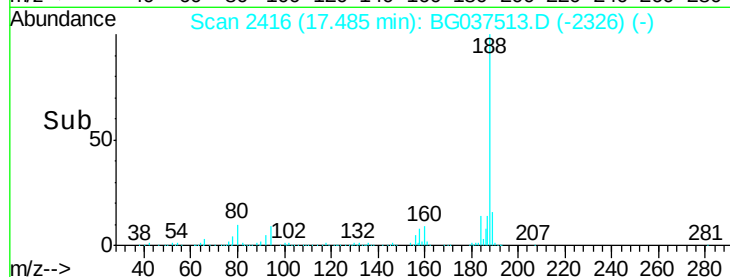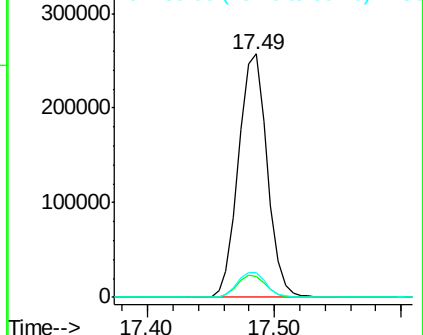

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.77 min Scan# 3145

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09


Tgt Ion:240 Resp: 370607

Ion Ratio Lower Upper

240 100

120 10.2 8.1 12.1



236 25.8 21.4 32.0

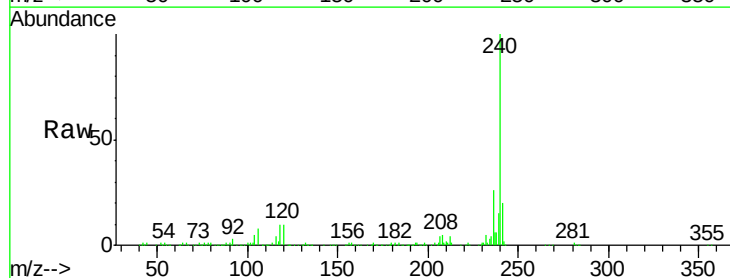


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

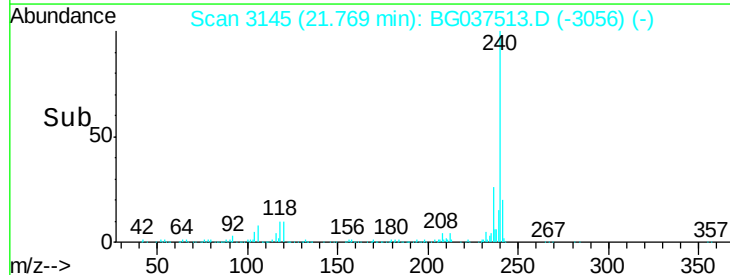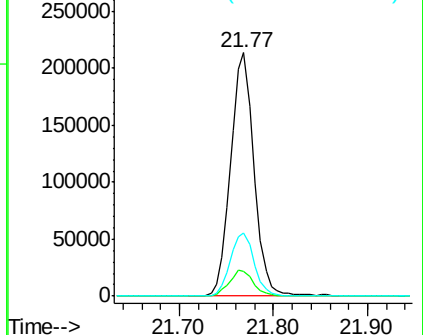

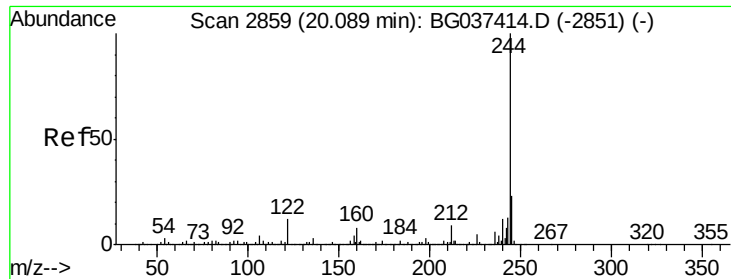

#79

Terphenyl-d14

Concen: 73.873 ng

RT: 20.08 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09

Instrument :

BNA_G

ClientSampleId :

PB114123BL


Tgt Ion:244 Resp: 1281276

Ion Ratio Lower Upper

244 100

212 8.5 6.5 9.7




122 11.7 9.0 13.4

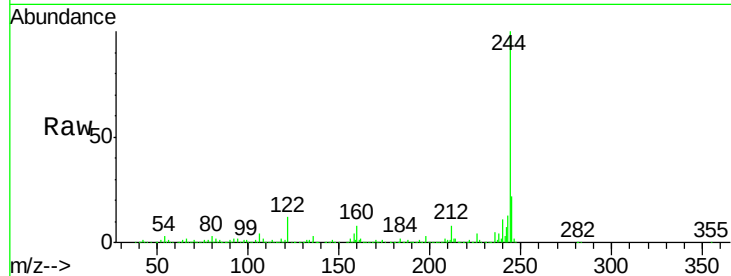

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

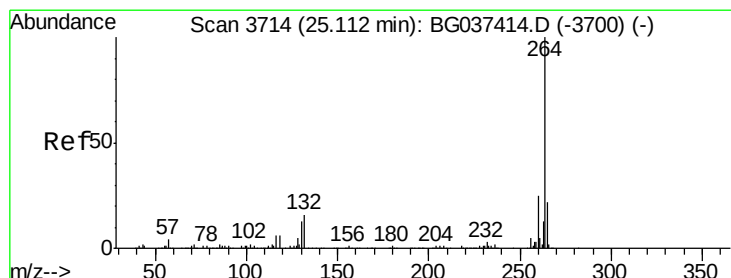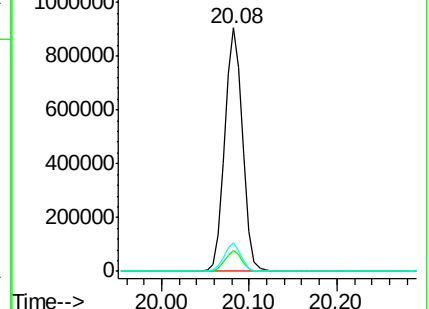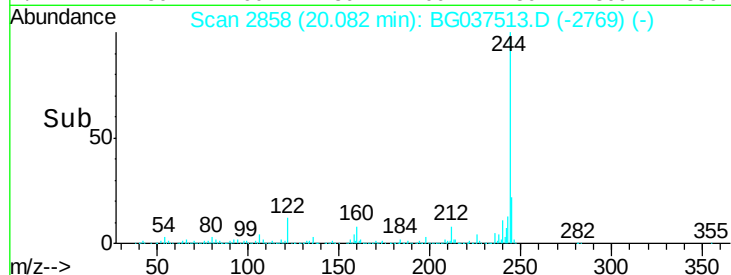

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.10 min Scan# 3712

Delta R.T. -0.01 min

Lab File: BG037513.D

Acq: 24 Oct 2018 16:09


Tgt Ion:264 Resp: 358856

Ion Ratio Lower Upper

264 100

260 23.5 18.2 27.4

265 22.0 17.9 26.9

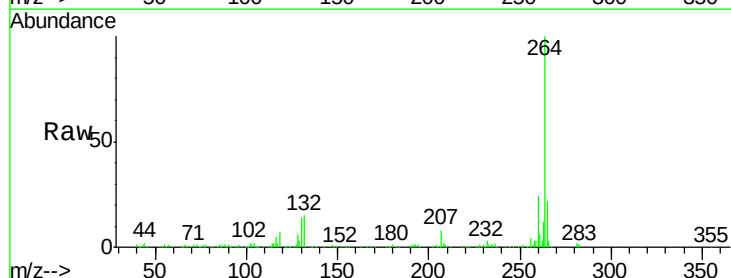

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

