


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102418\
 Data File : BG037510.D
 Acq On : 24 Oct 2018 14:12
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 18 14:06:42 2018

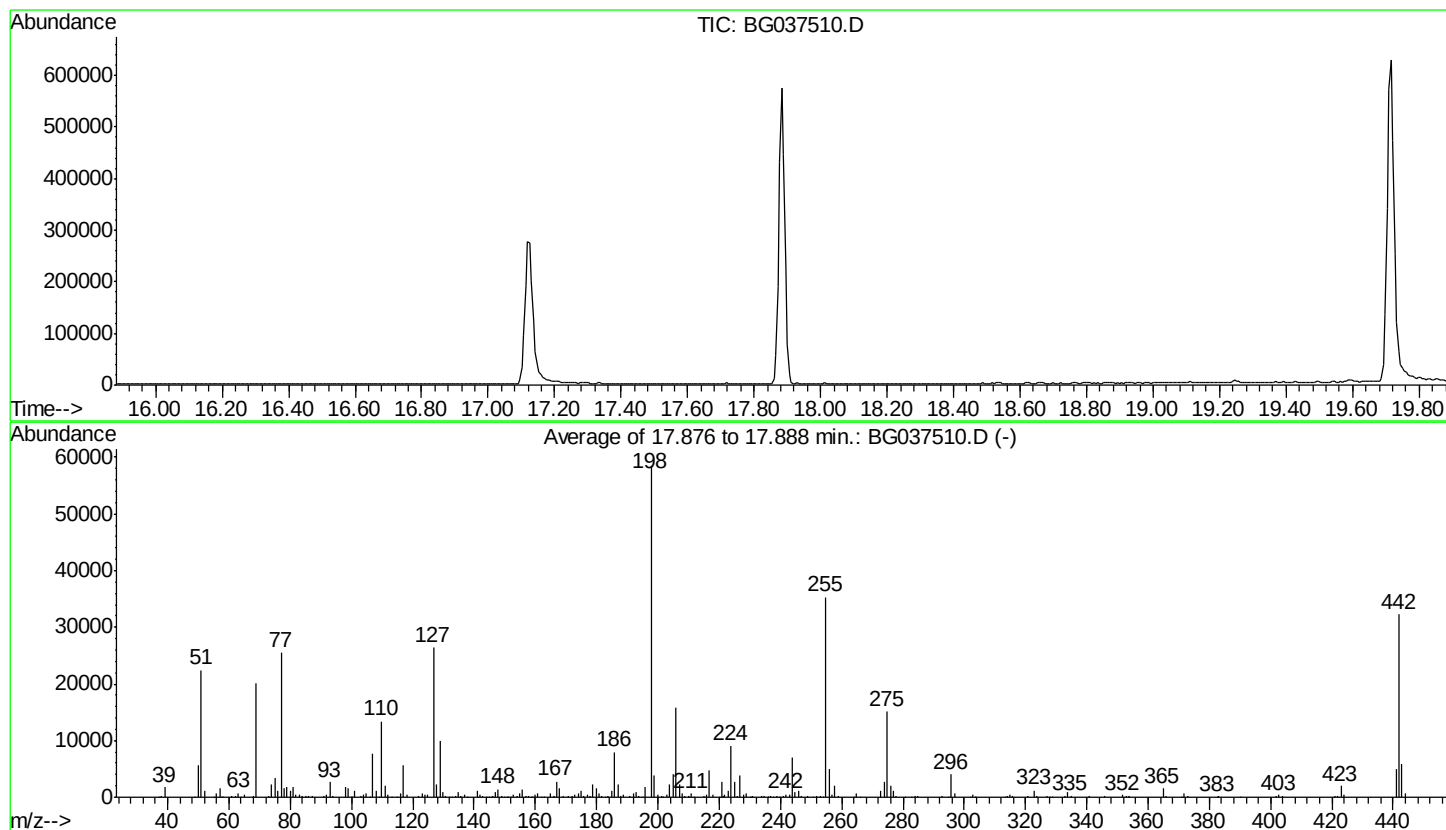

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	22373	PASS
68	69	0.00	2	0.8	166	PASS
69	198	0.00	100	34.3	20091	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.0	26338	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58522	PASS
199	198	5	9	6.8	3961	PASS
275	198	10	60	25.7	15040	PASS
365	198	1	100	2.7	1576	PASS
441	198	0.01	100	8.6	5062	PASS
442	198	50	100	55.2	32282	PASS
443	442	15	24	18.1	5856	PASS