


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102418\
Data File : BG037529.D
Acq On : 25 Oct 2018 3:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG101818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Oct 18 14:06:42 2018

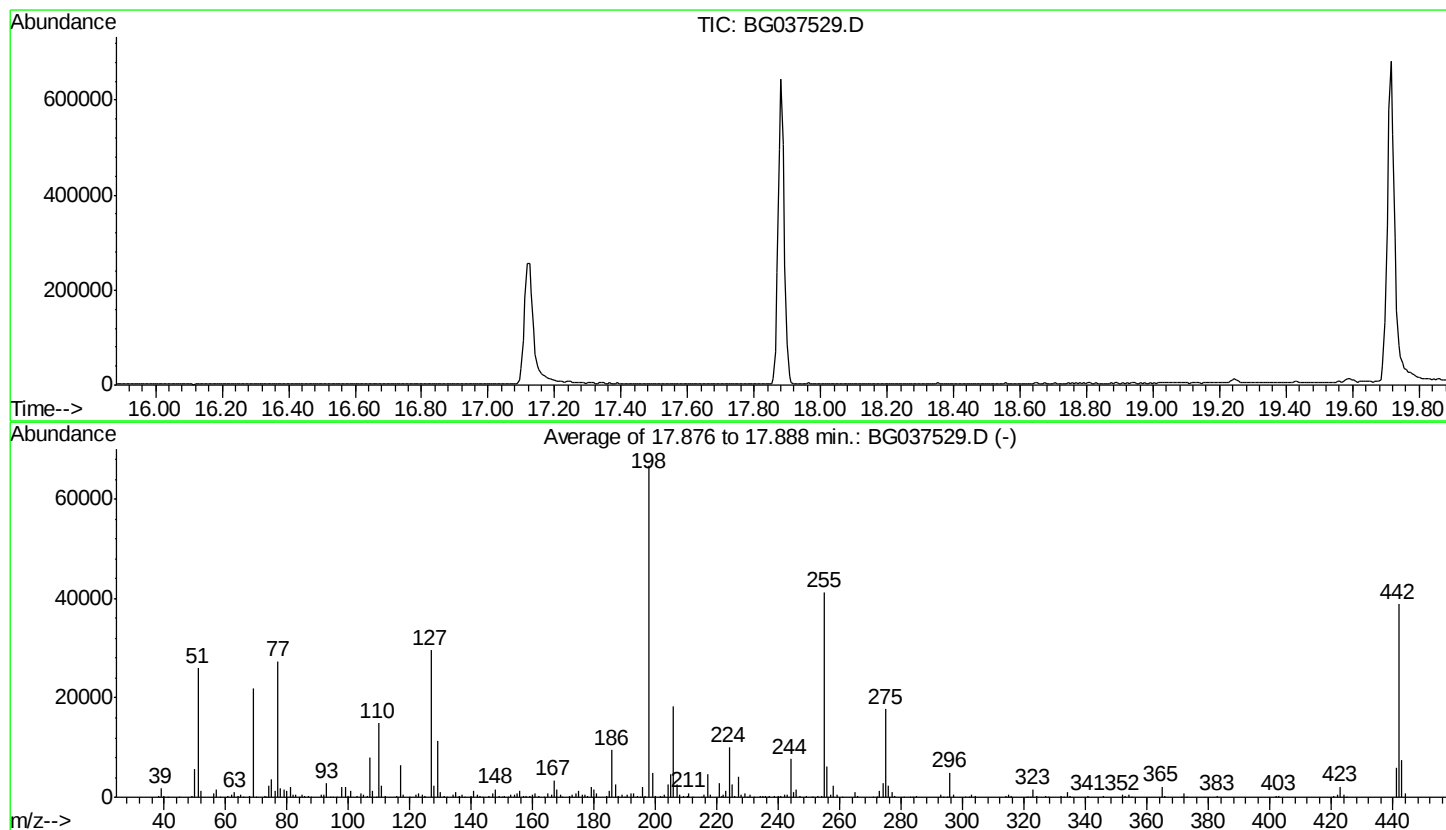

AutoFind: Scans 2483, 2484, 2485; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	25954	PASS
68	69	0.00	2	1.8	389	PASS
69	198	0.00	100	32.7	21866	PASS
70	69	0.00	2	0.2	52	PASS
127	198	10	80	44.4	29642	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	66821	PASS
199	198	5	9	7.2	4812	PASS
275	198	10	60	26.5	17717	PASS
365	198	1	100	3.2	2123	PASS
441	198	0.01	100	9.0	6032	PASS
442	198	50	100	58.2	38906	PASS
443	442	15	24	19.2	7488	PASS