
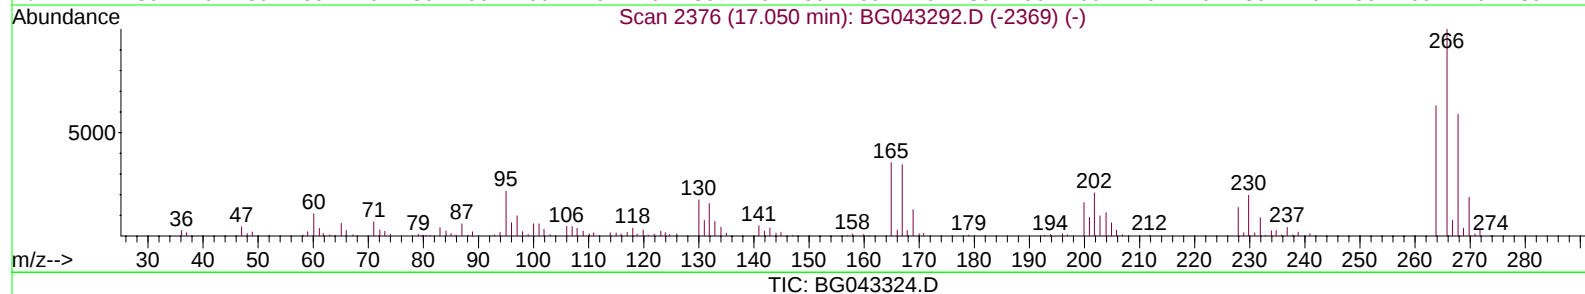
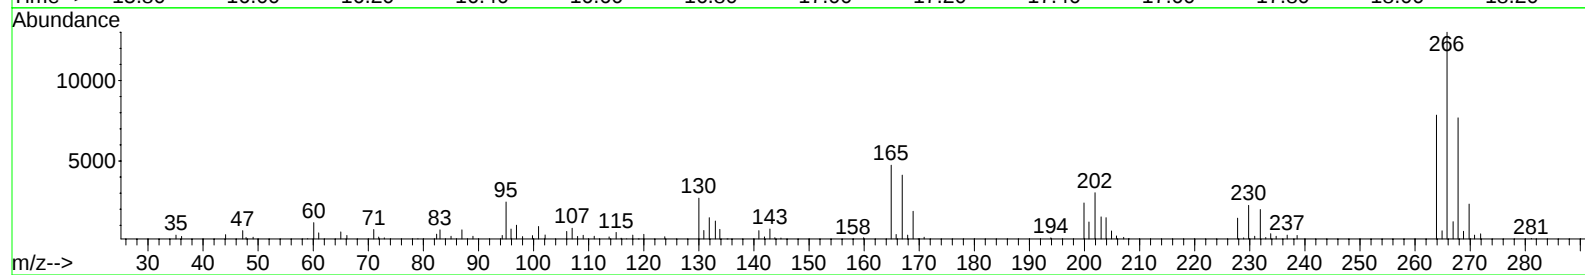


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102419\
Data File : BG043324.D
Acq On : 24 Oct 2019 9:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 19:41:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

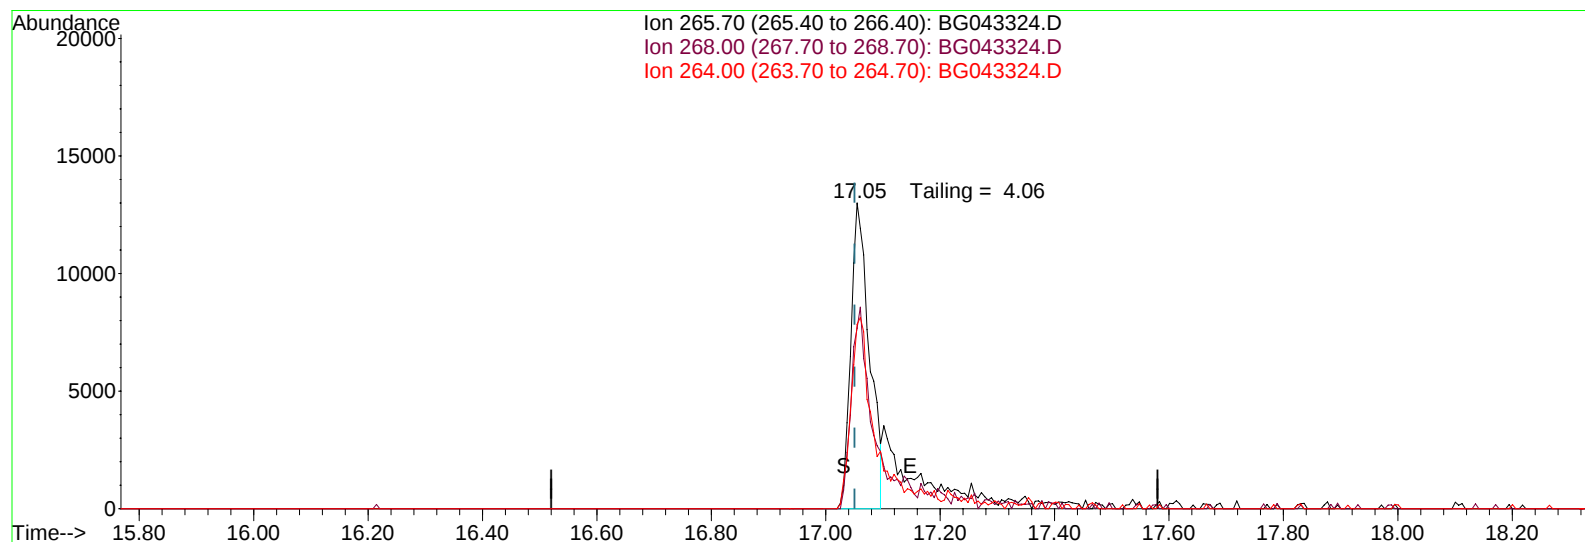

(70) Pentachlorophenol (C)




17.055min (+0.004) 12970.65ng m

response 29490

Ion	Exp%	Act%
265.70	100	100
268.00	58.90	59.07
264.00	63.00	60.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG102419\
Data File : BG043324.D
Acq On : 24 Oct 2019 9:46
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 19:41:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 16:37:43 2019
Response via : Initial Calibration

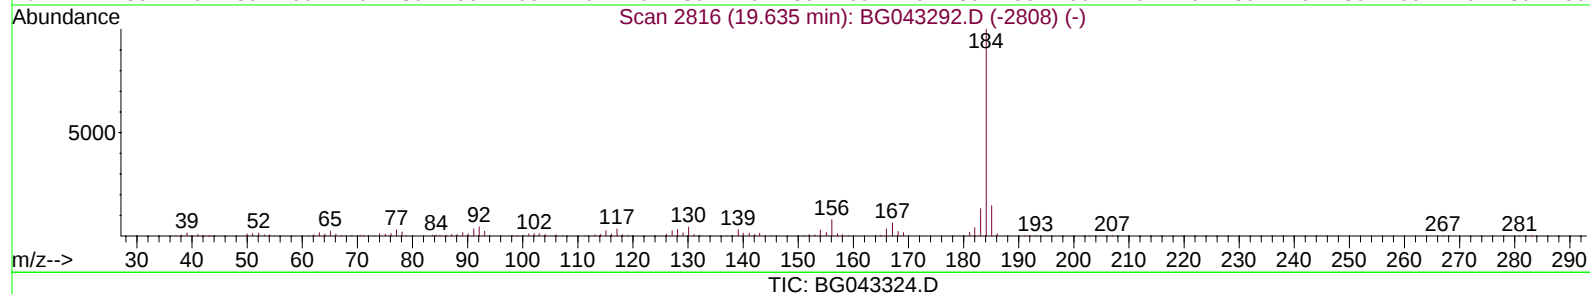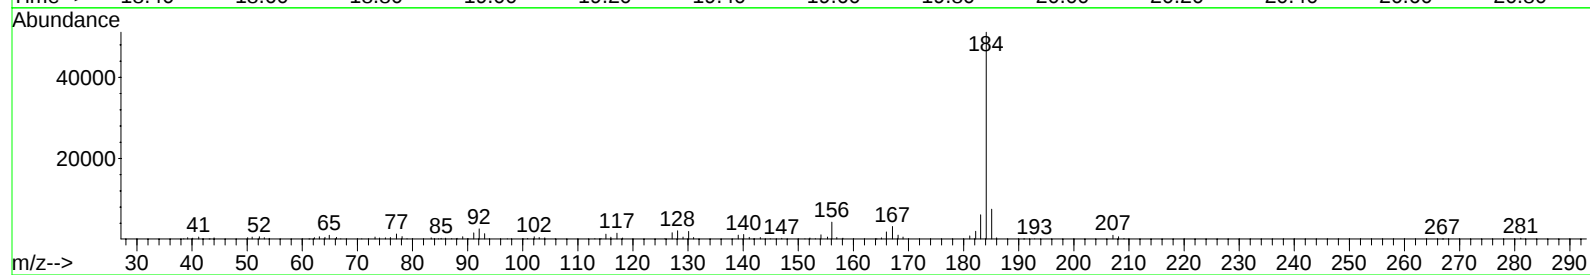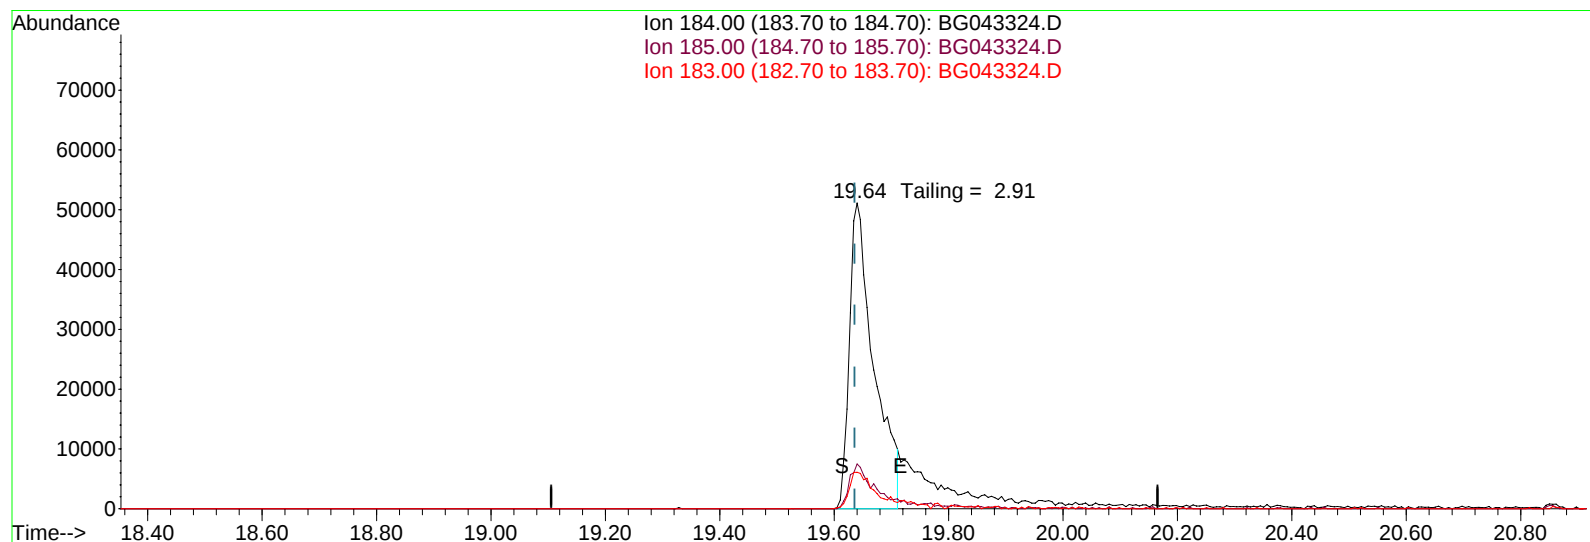

(77) Benzidine

19.640min (+0.004) 0.00ng m

response 152346

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.67
183.00	13.30	11.91
0.00	0.00	0.00