

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
Data File : BG043328.D
Acq On : 24 Oct 2019 13:04
Operator : JU
Sample : PB124226BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124226BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.603	421	428	441	rBV	397797	705586	18.82%	5.171%
2	7.196	691	699	713	rBV	408113	776131	20.70%	5.688%
3	7.560	753	761	771	rBV	438738	787631	21.01%	5.773%
4	8.024	831	840	850	rBV	126718	229897	6.13%	1.685%
5	8.347	886	895	907	rBV	512400	915115	24.41%	6.707%
6	9.188	1030	1038	1050	rBV	302213	654634	17.46%	4.798%
7	10.833	1311	1318	1330	rBV	113285	263870	7.04%	1.934%
8	13.271	1726	1733	1750	rBV	1018702	1785015	47.61%	13.082%
9	14.652	1959	1968	1982	rBV2	250412	445642	11.89%	3.266%
10	16.138	2214	2221	2235	rBV	539770	1029693	27.47%	7.547%
11	17.396	2429	2435	2448	rBV	316307	600645	16.02%	4.402%
12	20.004	2873	2879	2895	rBV	2668522	3748887	100.00%	27.476%
13	21.661	3152	3161	3180	rBV2	404386	837932	22.35%	6.141%
14	24.863	3694	3706	3724	rBV2	269277	863677	23.04%	6.330%


Sum of corrected areas: 13644355

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
Data File : BG043328.D
Acq On : 24 Oct 2019 13:04
Operator : JU
Sample : PB124226BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124226BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

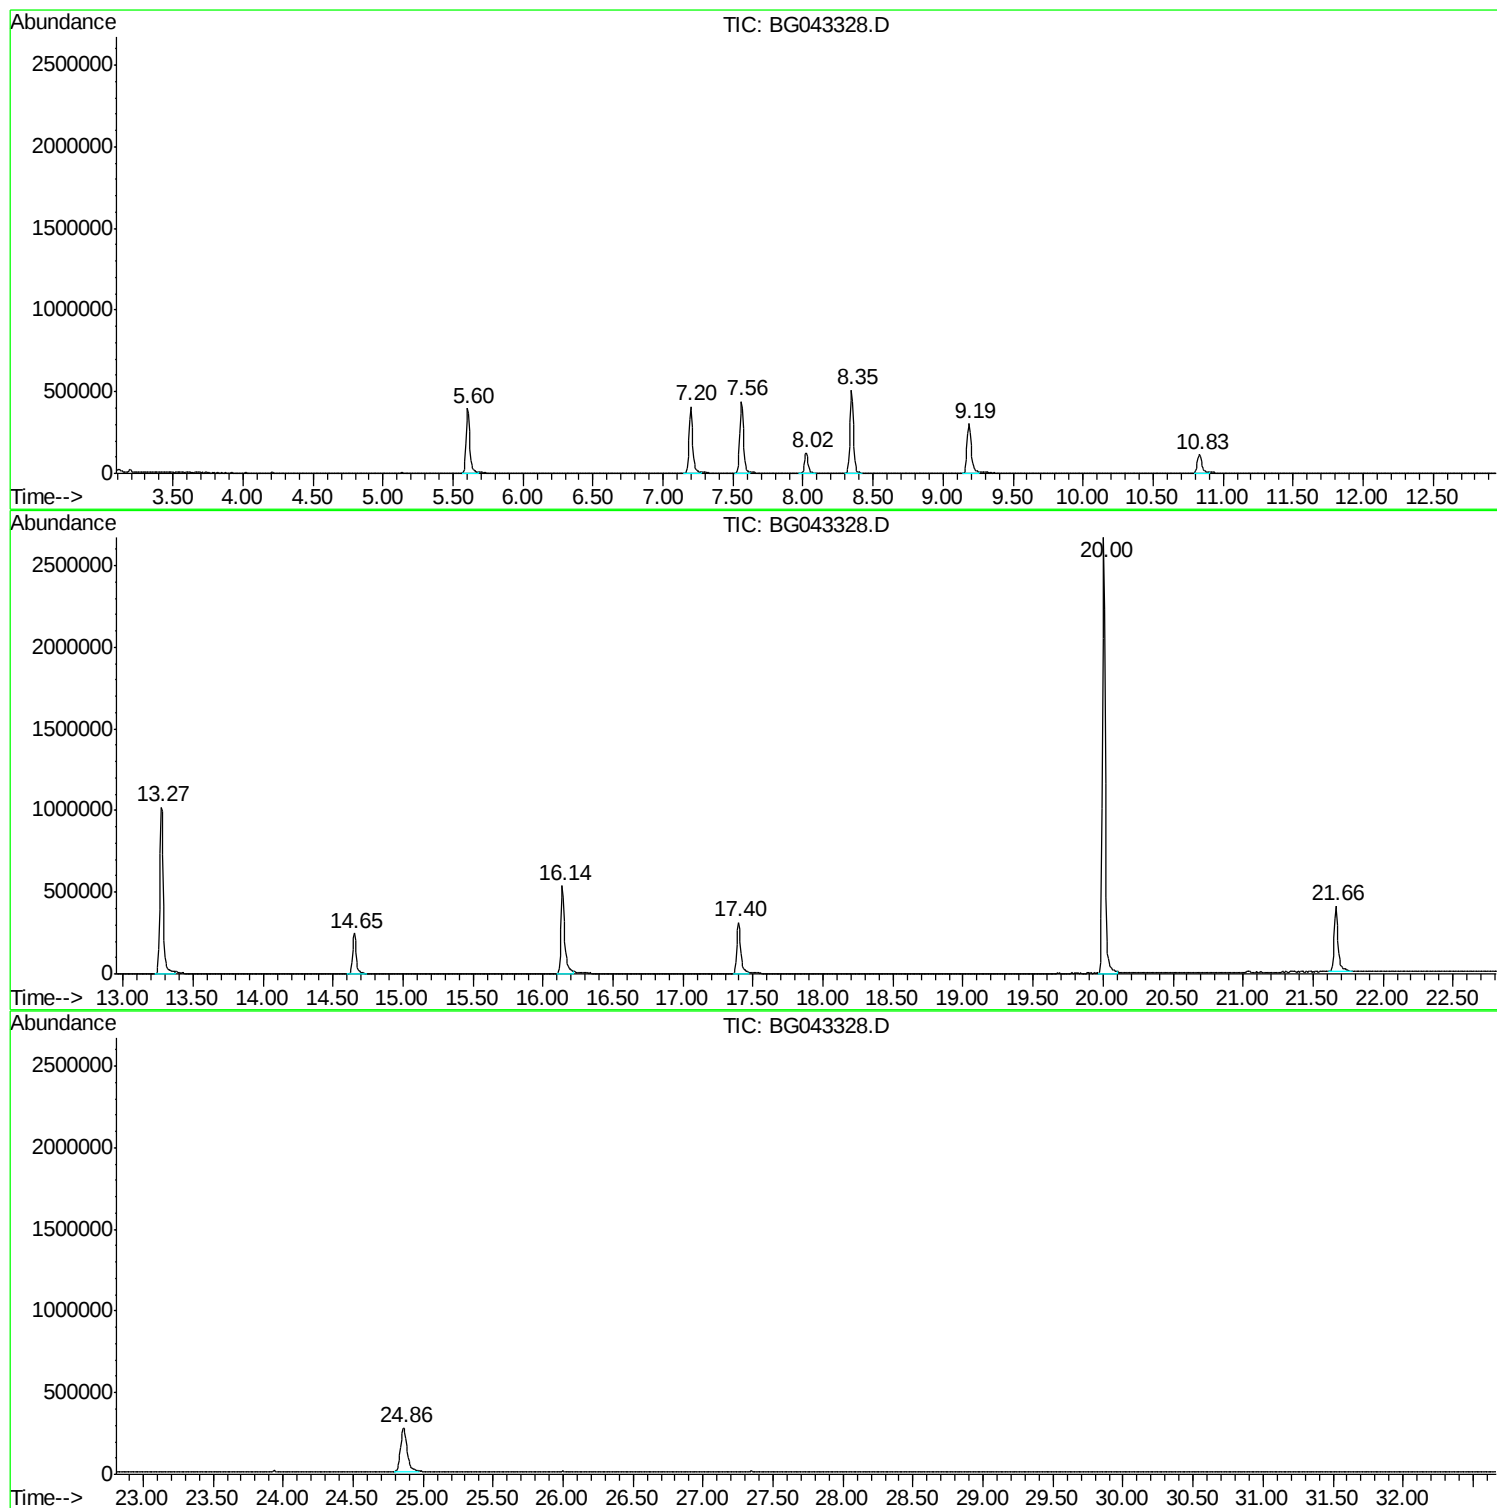

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
Data File : BG043328.D
Acq On : 24 Oct 2019 13:04
Operator : JU
Sample : PB124226BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124226BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.56 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.56	68.52 ng	787631	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		N-(-3,4-Methylenedioxyphenylisopropyl)-N-methyl-2-pyrrolidinone	267	C17H17NO2	1000378-96-6	10
4		Tranvlcypropane-propionyl	189	C12H15NO	1000123-86-3	10
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

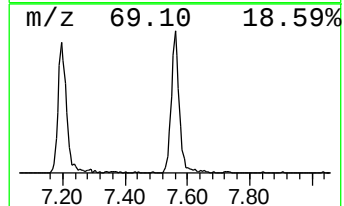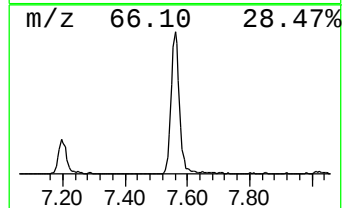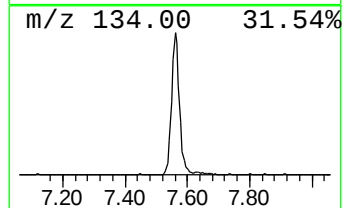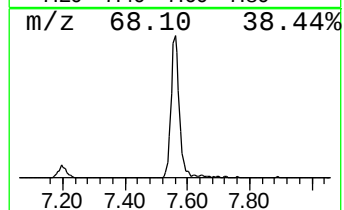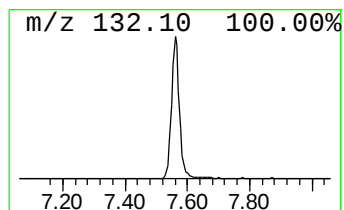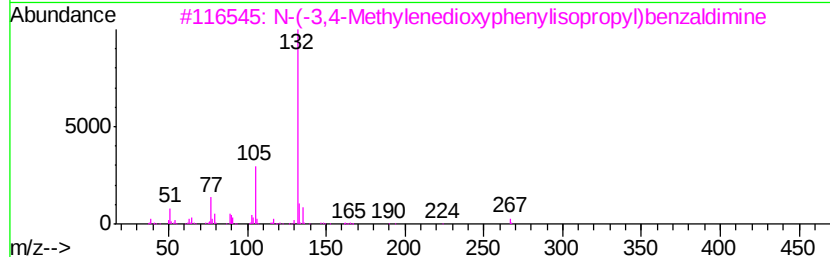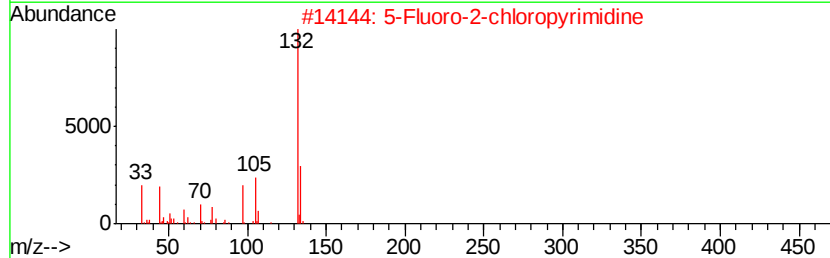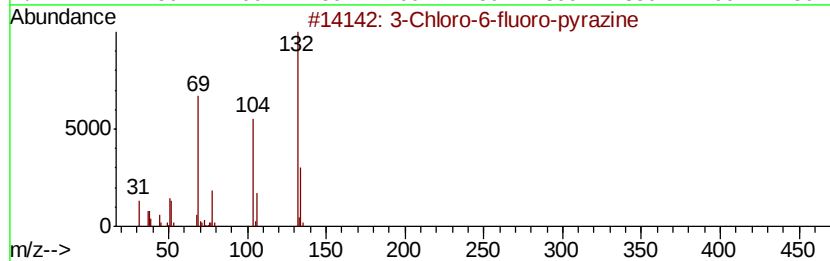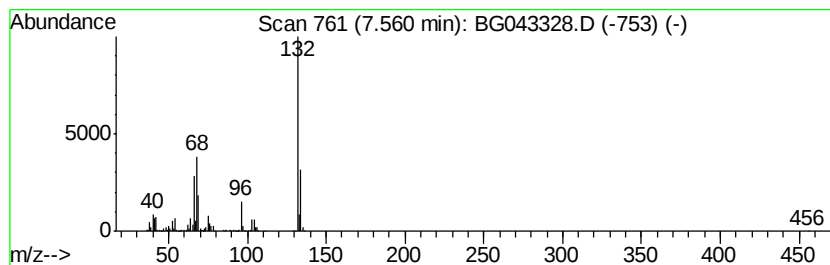

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102419\
Data File : BG043328.D
Acq On : 24 Oct 2019 13:04
Operator : JU
Sample : PB124226BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124226BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.56	7.56	68.5	ng	787631	1	8.02	229897	20.0