

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
 Data File : BG043332.D
 Acq On : 24 Oct 2019 15:37
 Operator : JU
 Sample : PB124252BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB124252BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.602	422	428	442	rBV	598376	1056137	25.13%	6.532%
2	7.200	691	700	720	rBV	622354	1179177	28.05%	7.293%
3	7.558	754	761	772	rBV	653163	1175223	27.96%	7.269%
4	8.022	832	840	849	rBV	119570	219970	5.23%	1.360%
5	8.346	888	895	908	rBV	505932	932649	22.19%	5.768%
6	9.186	1030	1038	1054	rBV	322459	698569	16.62%	4.321%
7	10.831	1311	1318	1329	rBV	112989	257952	6.14%	1.595%
8	13.275	1727	1734	1749	rBV	1064610	1859621	44.24%	11.501%
9	14.650	1962	1968	1980	rBV2	243054	437617	10.41%	2.707%
10	16.136	2214	2221	2244	rBV	943291	1720372	40.93%	10.640%
11	17.394	2428	2435	2448	rBV2	324637	606858	14.44%	3.753%
12	20.008	2873	2880	2896	rBV	2841432	4203325	100.00%	25.997%
13	21.659	3154	3161	3180	rBV	428876	897407	21.35%	5.550%
14	24.867	3694	3707	3724	rBV2	288426	923811	21.98%	5.714%


Sum of corrected areas: 16168688

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
Data File : BG043332.D
Acq On : 24 Oct 2019 15:37
Operator : JU
Sample : PB124252BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124252BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

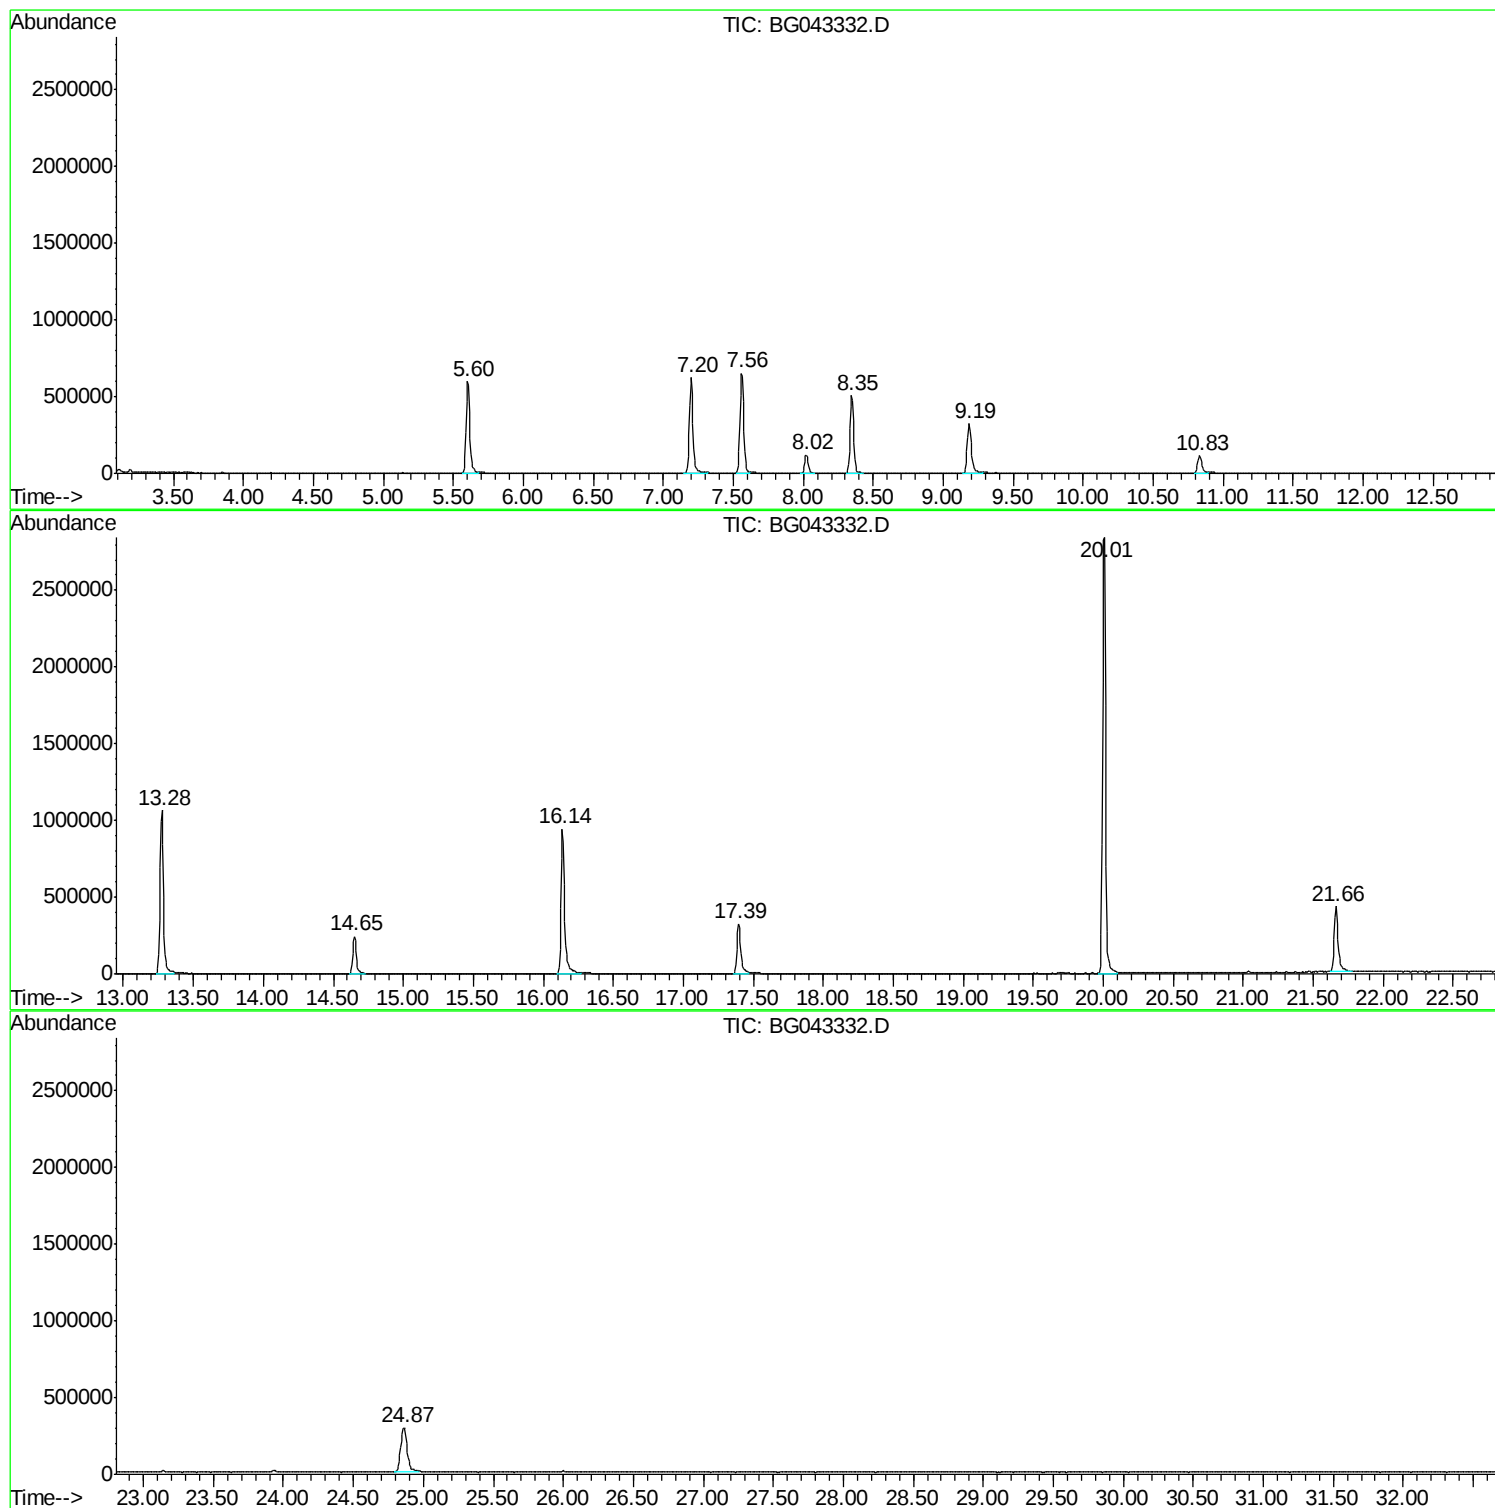

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
Data File : BG043332.D
Acq On : 24 Oct 2019 15:37
Operator : JU
Sample : PB124252BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124252BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.56	106.85 ng	1175220	1,4-Dichlorobenzene-d4	8.02

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	27
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

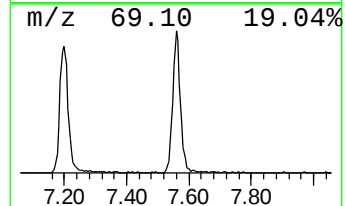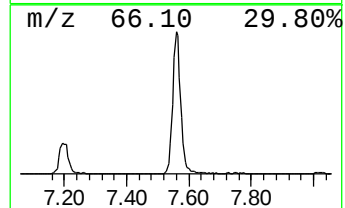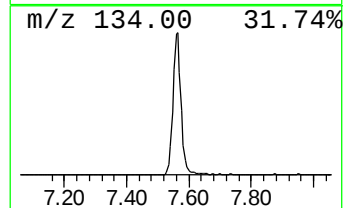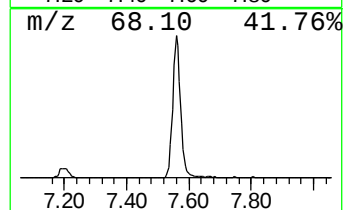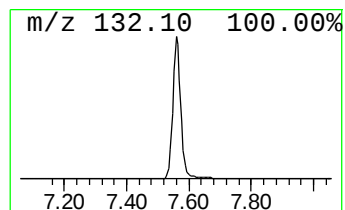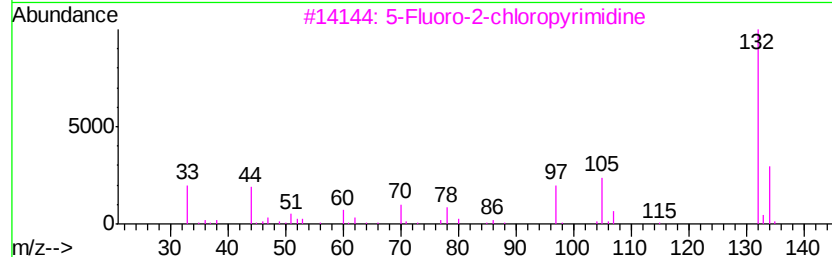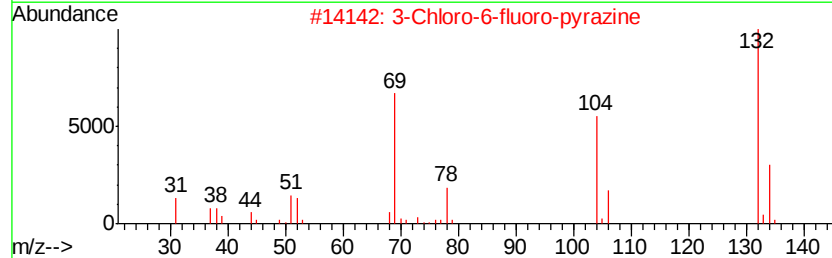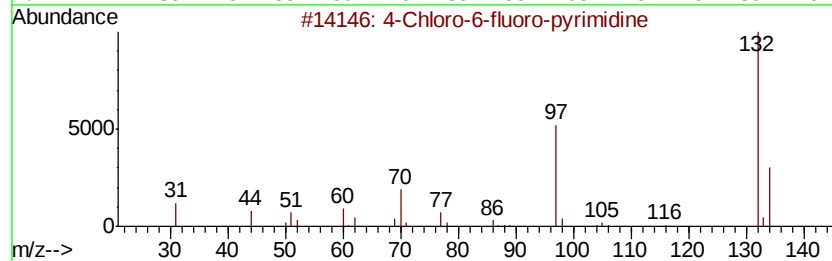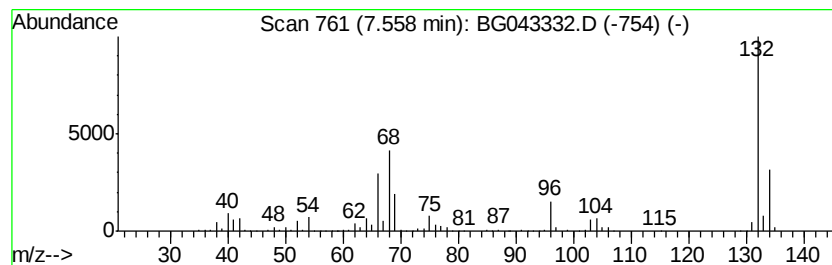

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG102419\
Data File : BG043332.D
Acq On : 24 Oct 2019 15:37
Operator : JU
Sample : PB124252BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB124252BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.56	7.56	106.8	ng	1175220	1	8.02	219970	20.0