


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG102419\
 Data File : BG043324.D
 Acq On : 24 Oct 2019 9:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG102119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 21 16:37:43 2019

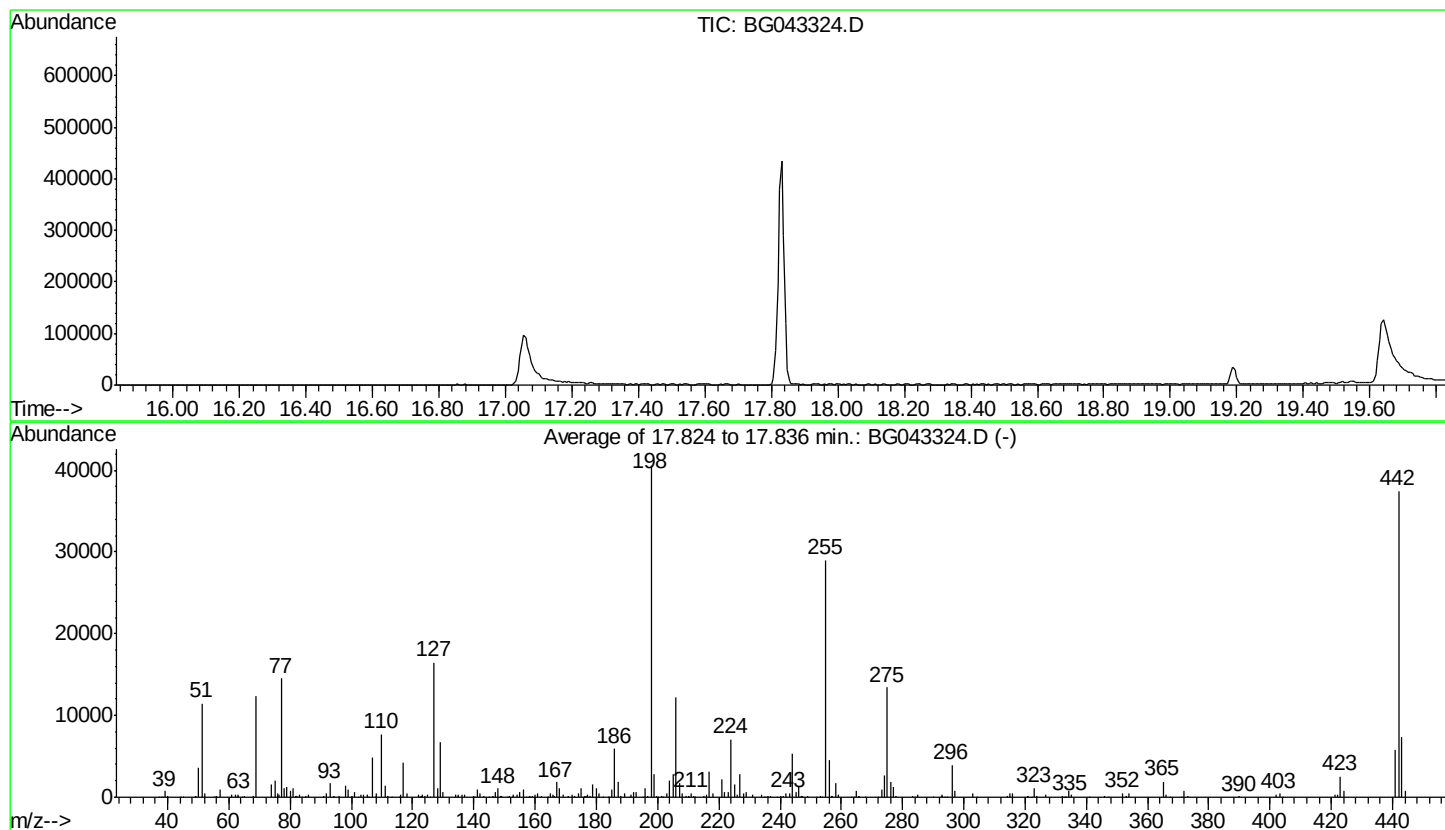

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	11501	PASS
68	69	0.00	2	0.7	92	PASS
69	198	0.00	100	30.5	12361	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.7	16503	PASS
197	198	0.00	2	0.2	91	PASS
198	198	100	100	100.0	40570	PASS
199	198	5	9	7.0	2839	PASS
275	198	10	60	33.1	13410	PASS
365	198	1	100	4.7	1914	PASS
441	198	0.01	100	14.5	5876	PASS
442	198	50	100	92.4	37493	PASS
443	442	15	24	19.8	7411	PASS