


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102422\
 Data File : BG055250.D
 Acq On : 24 Oct 2022 10:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 24 16:54:05 2022

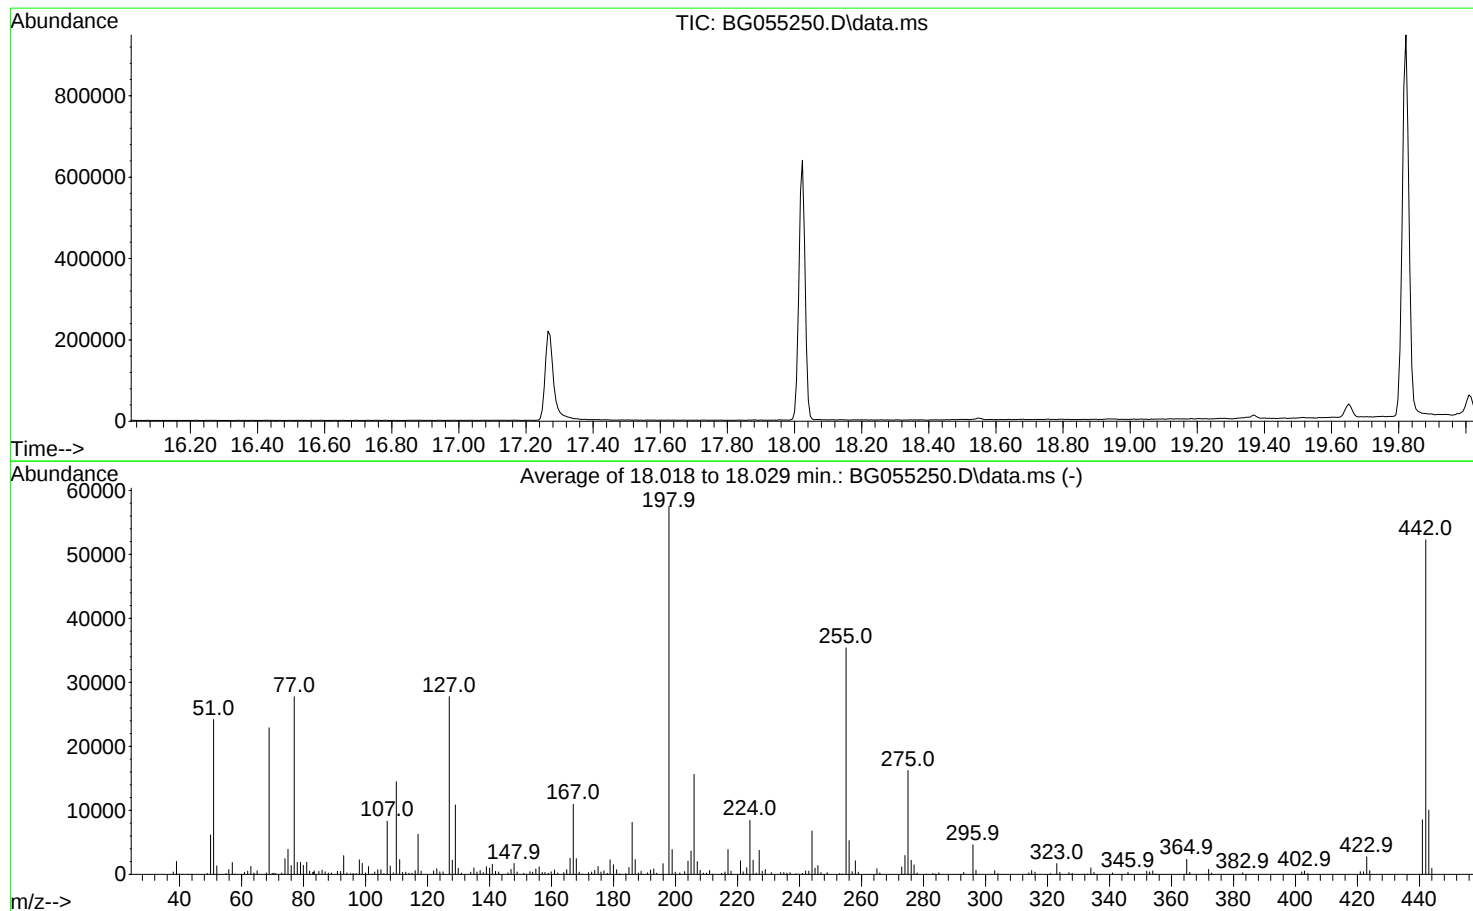




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	24197	PASS
68	69	0.00	2	1.0	222	PASS
69	198	0.00	100	39.8	22895	PASS
70	69	0.00	2	0.8	183	PASS
127	198	10	80	48.3	27776	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	57488	PASS
199	198	5	9	6.8	3884	PASS
275	198	10	60	28.2	16219	PASS
365	198	1	100	4.1	2359	PASS
441	198	0.01	100	14.8	8532	PASS
442	442	50	100	100.0	52291	PASS
443	442	15	24	19.2	10064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102422\
Data File : BG055250.D
Acq On : 24 Oct 2022 10:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 02:06:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

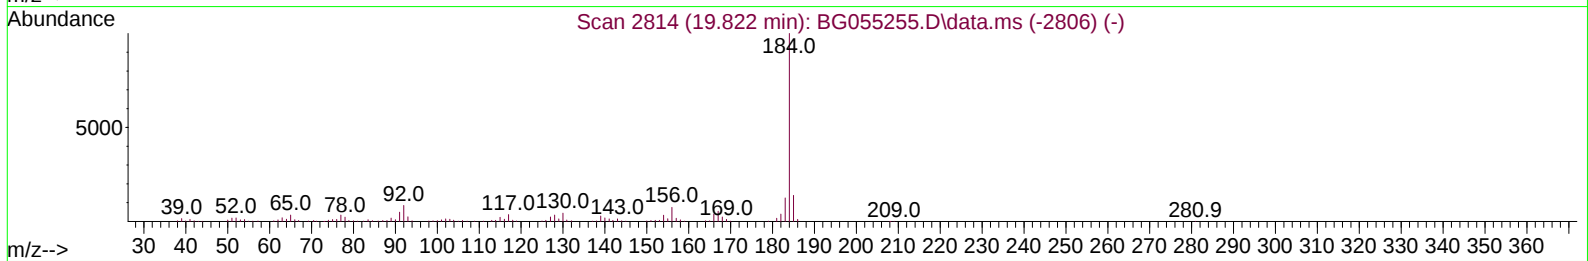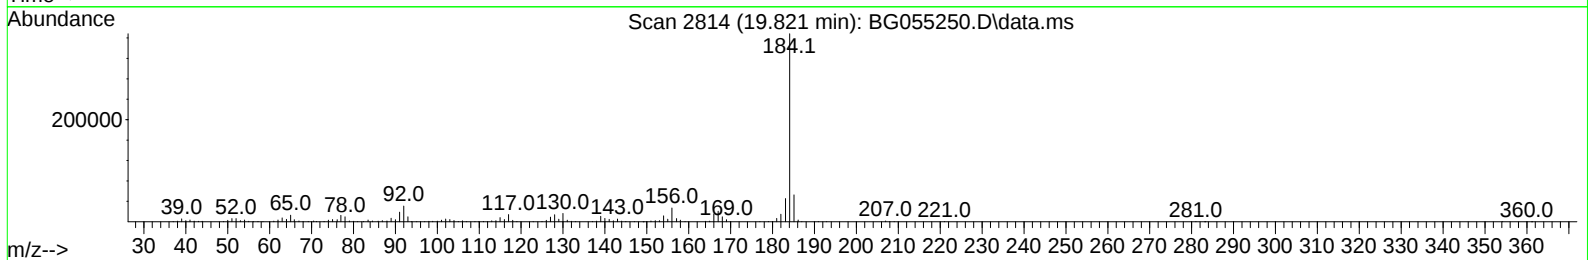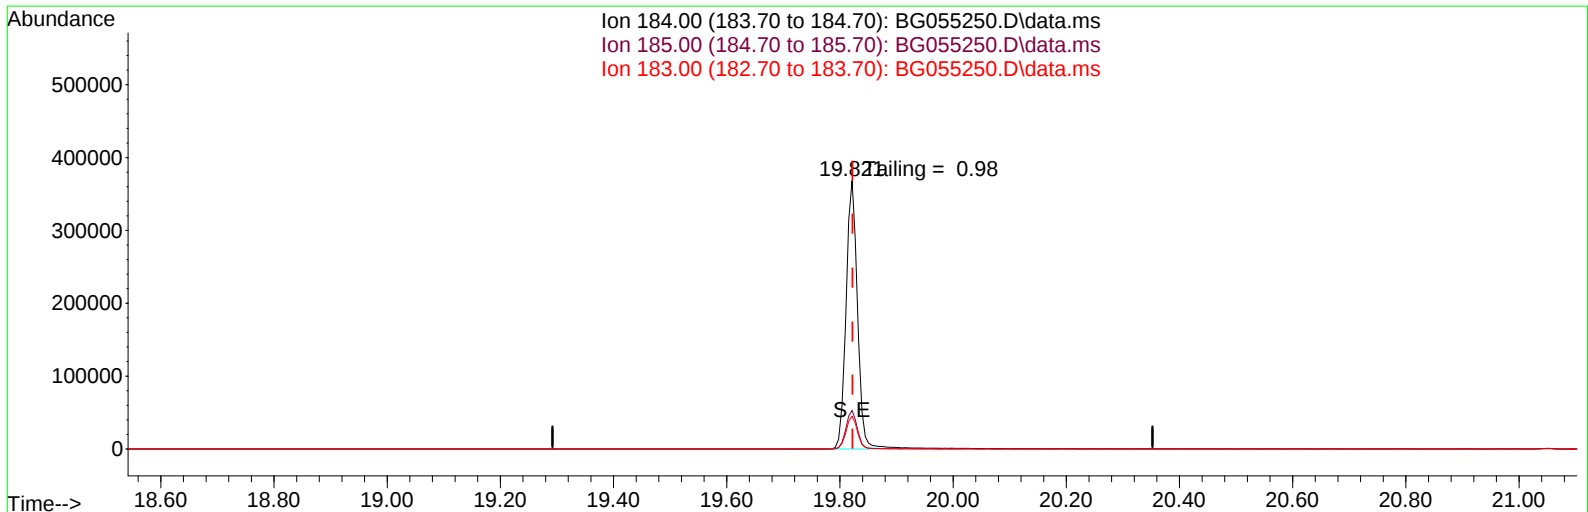

TIC: BG055250.D\data.ms

(77) Benzidine

19.821min (-0.001) 15393.00 ng




response 521046

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.33
183.00	12.50	12.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102422\
Data File : BG055250.D
Acq On : 24 Oct 2022 10:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 02:06:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

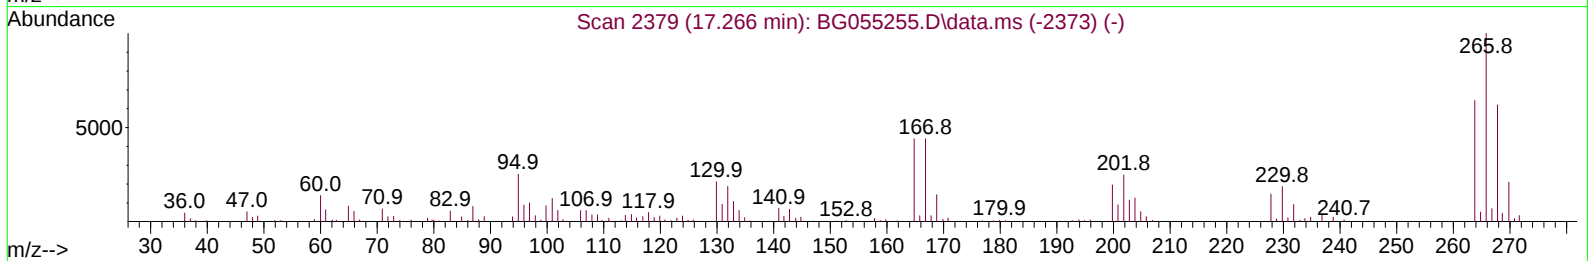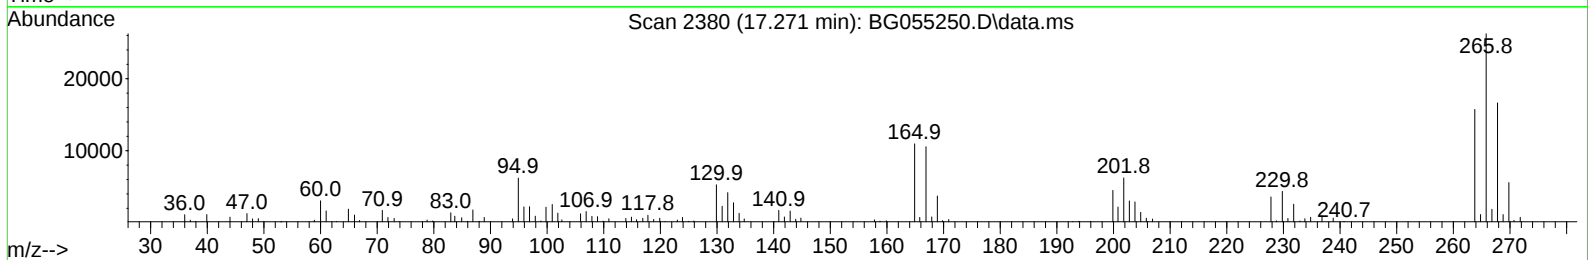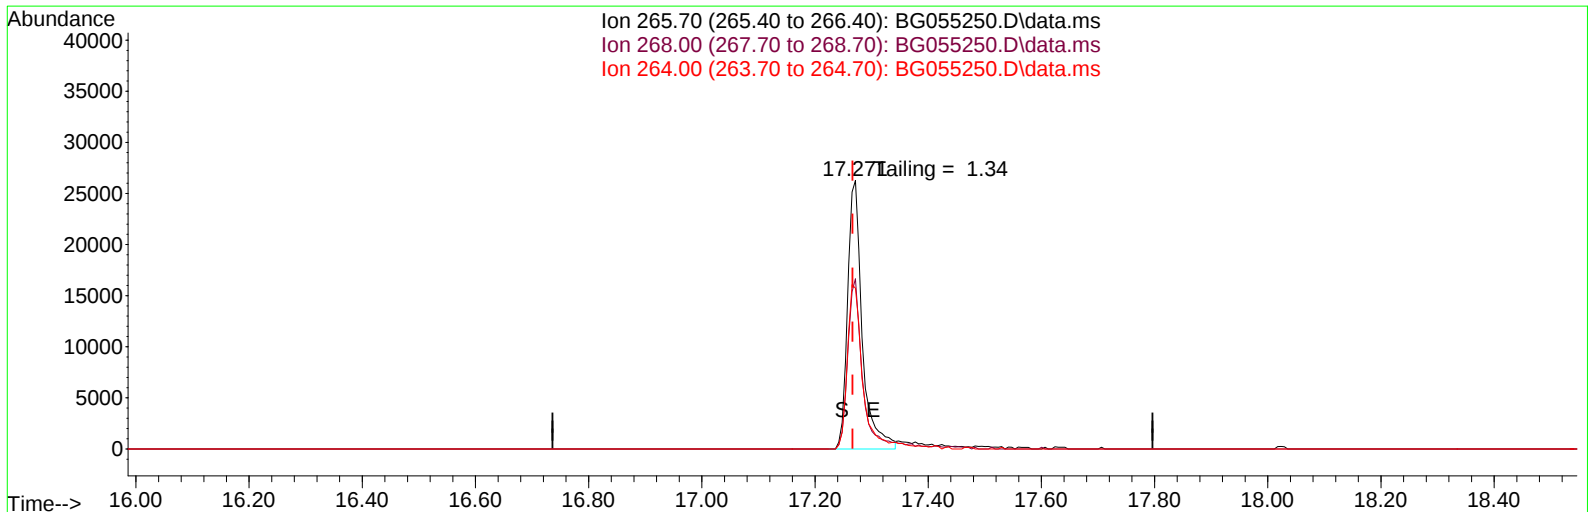

TIC: BG055250.D\data.ms

(70) Pentachlorophenol (C)

17.271min (+ 0.005) 25164.40 ng

response 48383

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	63.42
264.00	64.40	59.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/24/2022	BNA_G	BG055250.D
Compound Name	Response	Retention Time
DDT	213779	21.049
DDD	1914	20656
DDE	125	20.197
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2039	215818	0.94

Instrument :
BNA_G
ClientSampleId :
DFTPP