
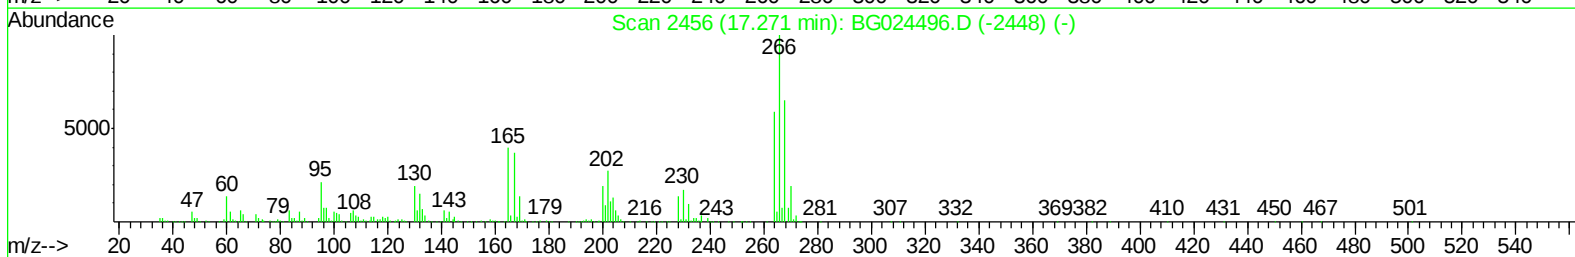
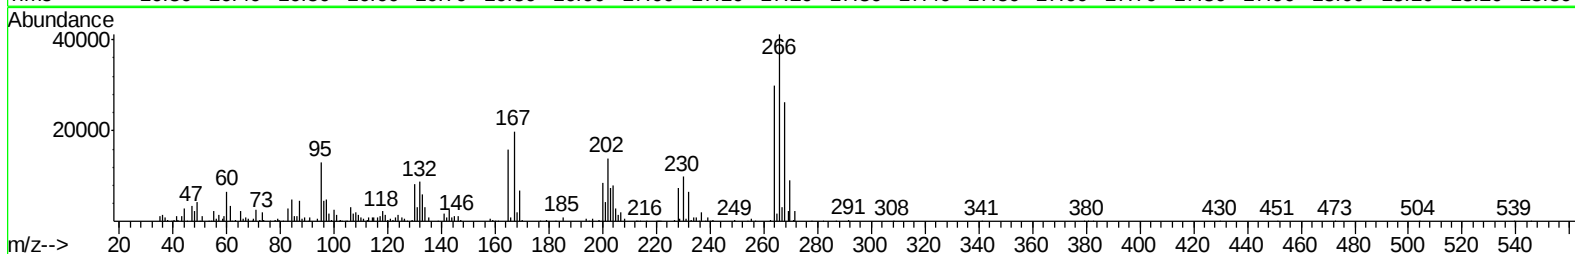


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102516\
Data File : BG024491.D
Acq On : 25 Oct 2016 11:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:59:46 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:25:08 2016
Response via : Initial Calibration

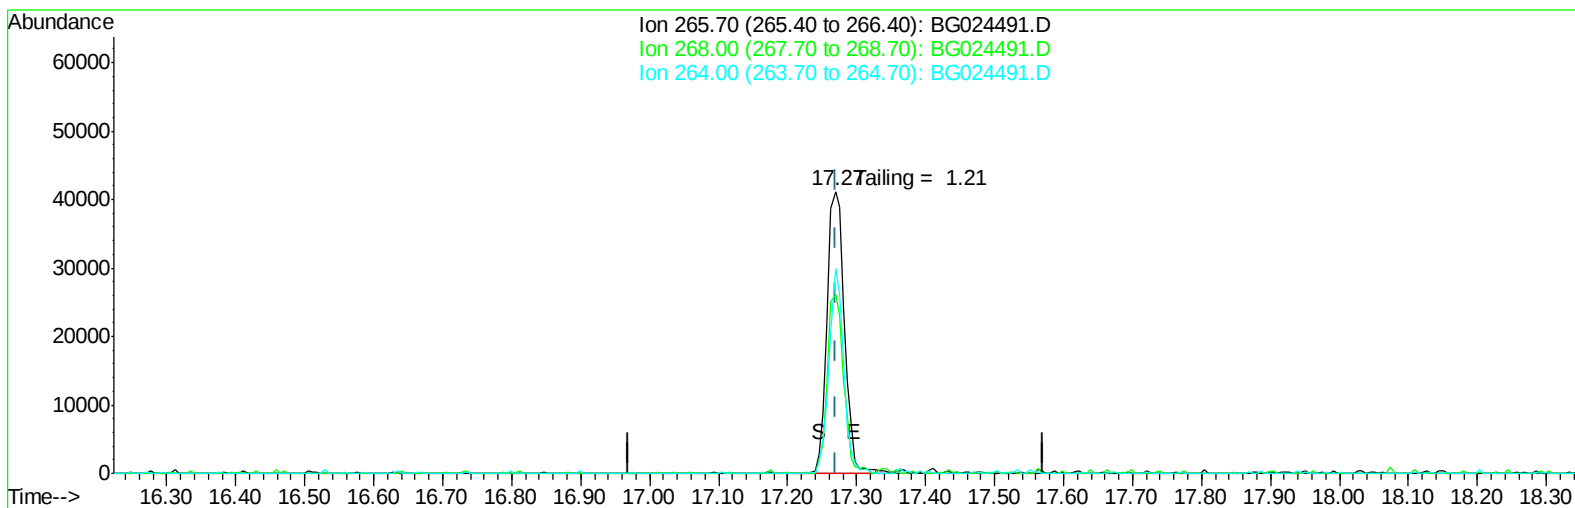

TIC: BG024491.D

(69) Pentachlorophenol (C)




17.269min (-0.002) 34233.58ng

response 71814

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.59
264.00	62.60	72.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102516\
Data File : BG024491.D
Acq On : 25 Oct 2016 11:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:59:46 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:25:08 2016
Response via : Initial Calibration

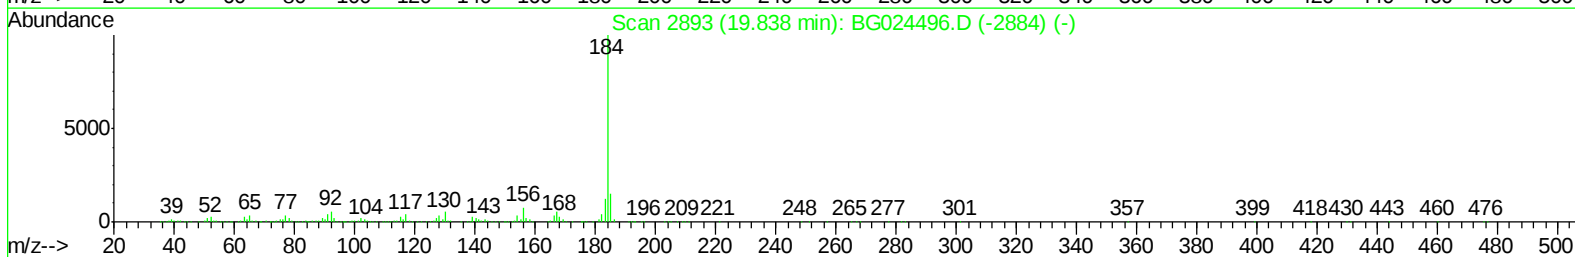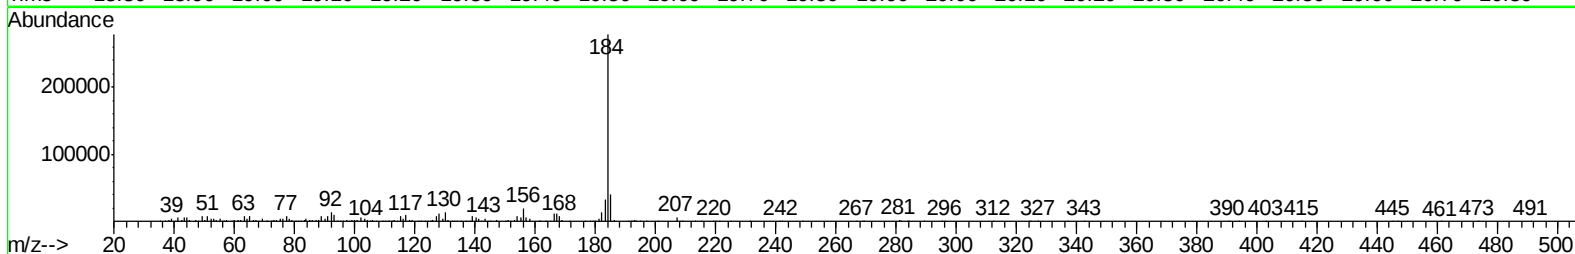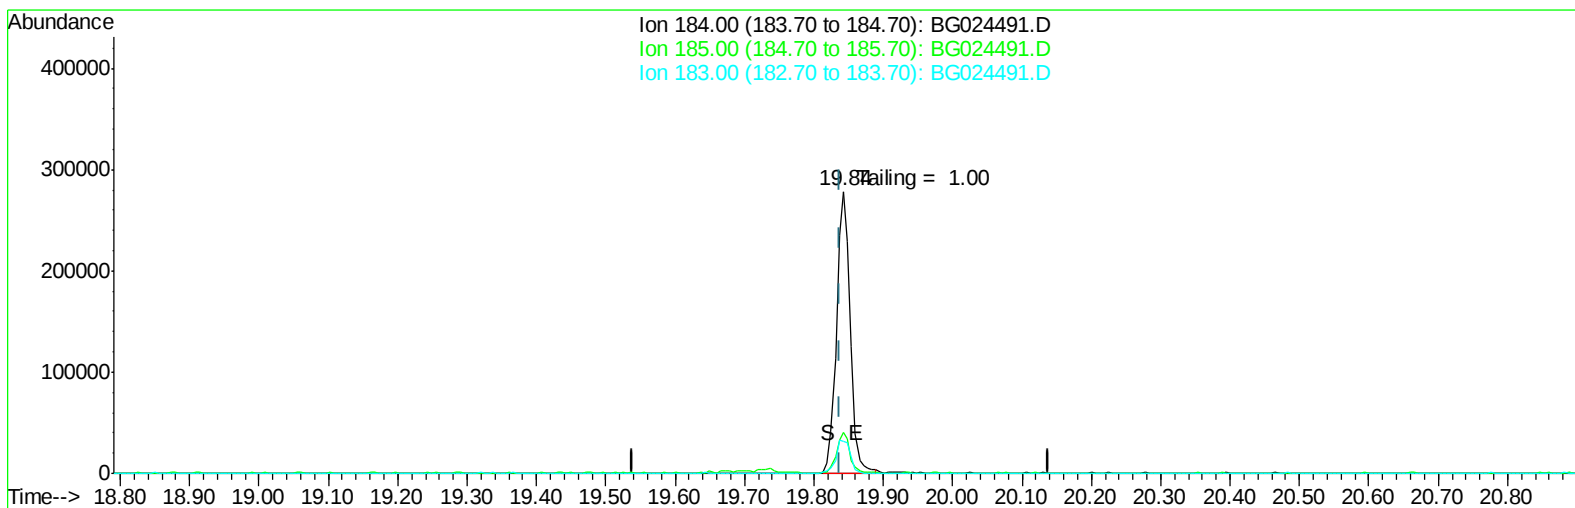

TIC: BG024491.D

(76) Benzidine




19.842min (+0.004) 75805.21ng

response 391147

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.53
183.00	13.80	11.40
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102516\
Data File : BG024491.D
Acq On : 25 Oct 2016 11:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:59:46 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:25:08 2016
Response via : Initial Calibration

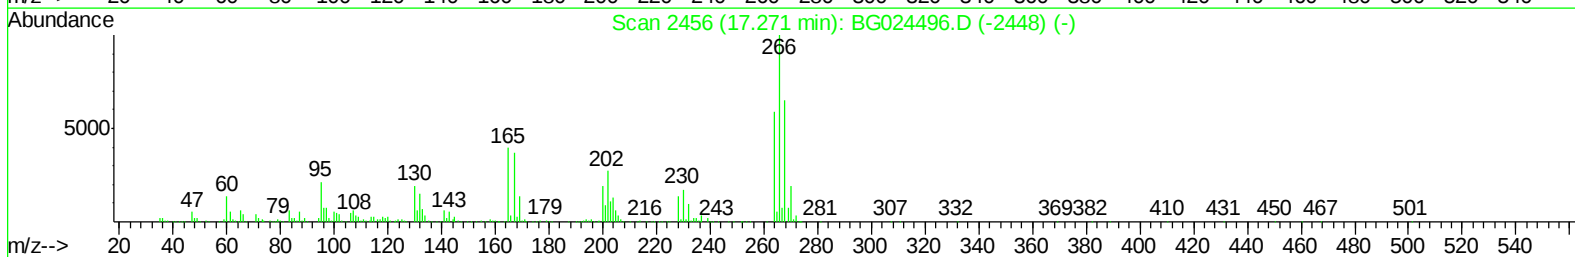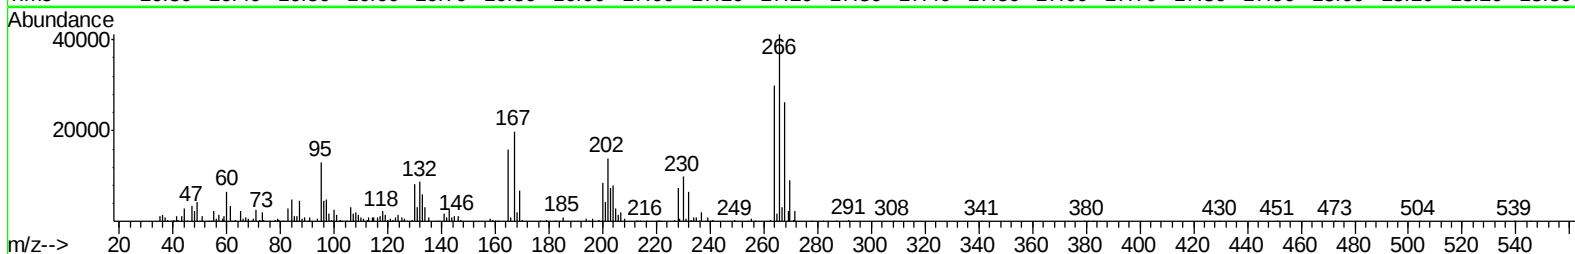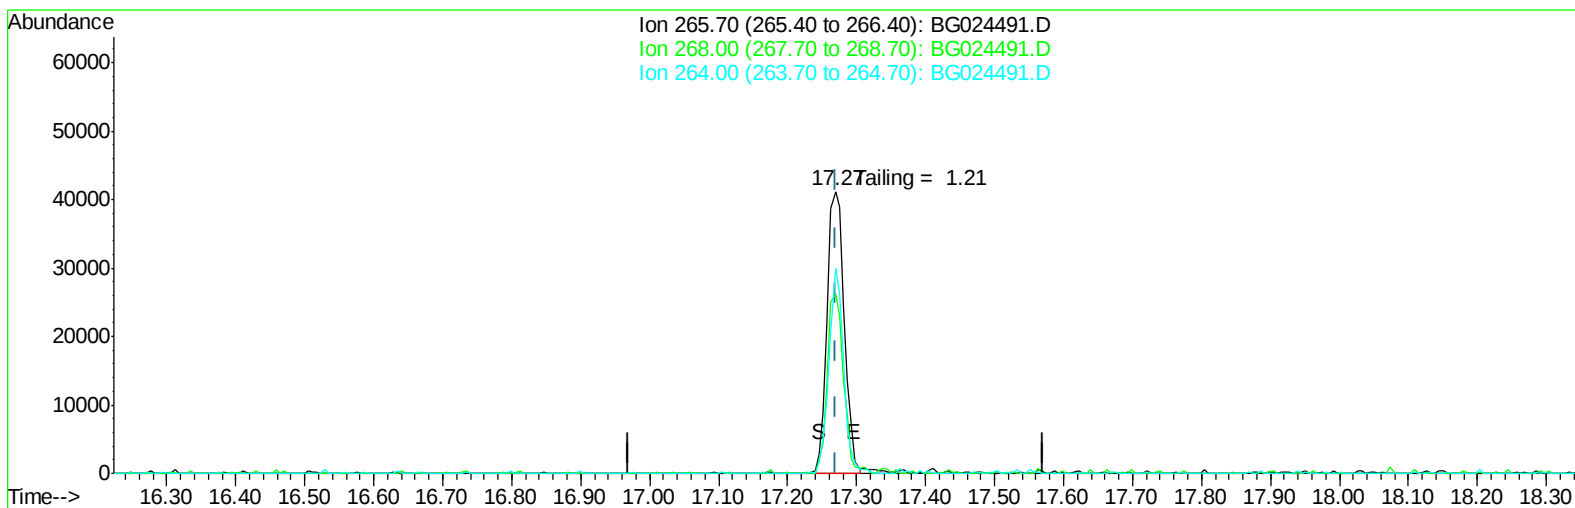

TIC: BG024491.D

(69) Pentachlorophenol (C)




17.269min (-0.002) 34233.58ng

response 71814

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.59
264.00	62.60	72.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102516\
 Data File : BG024491.D
 Acq On : 25 Oct 2016 11:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 18:59:46 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG102516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 25 17:25:08 2016
 Response via : Initial Calibration

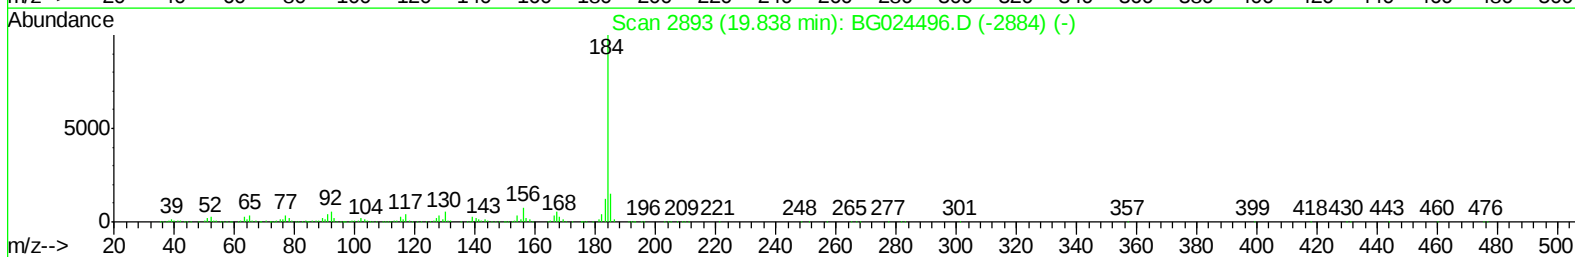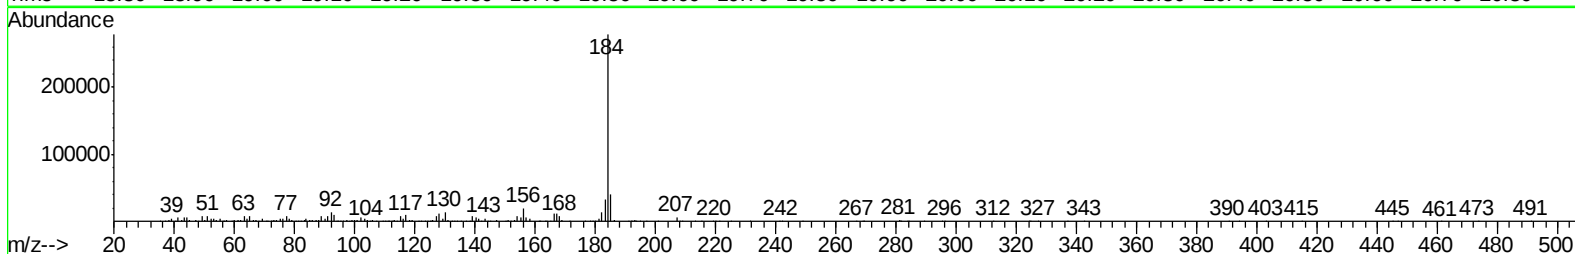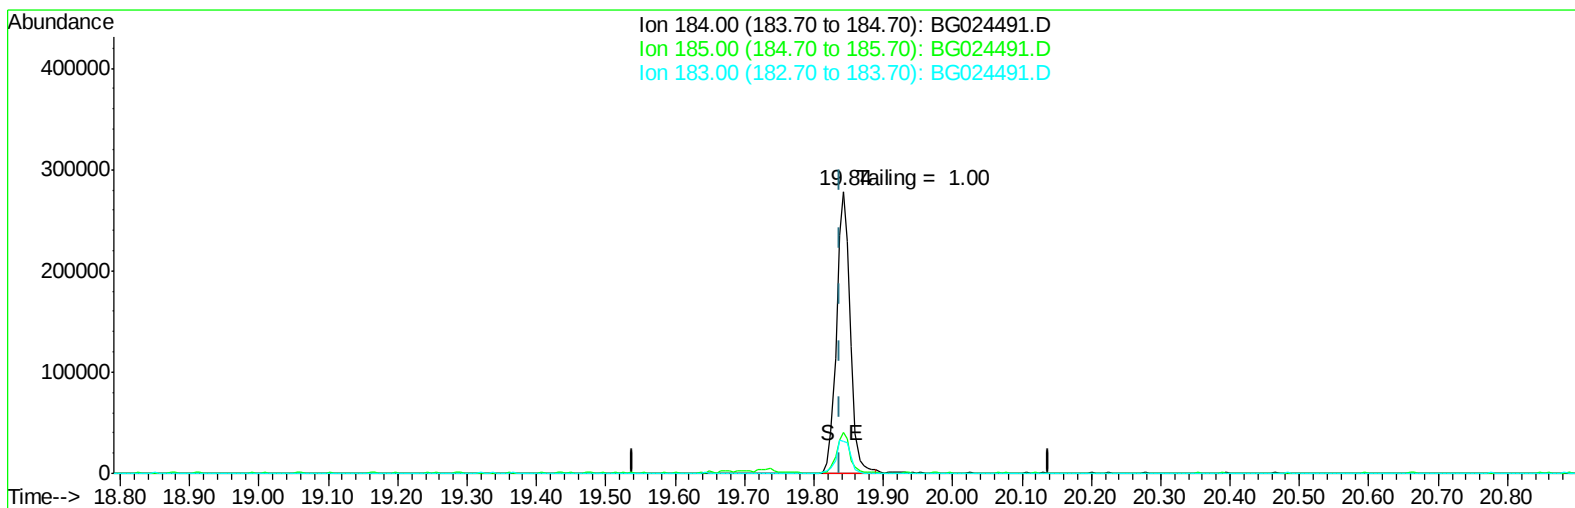

TIC: BG024491.D

(76) Benzidine

19.842min (+0.004) 75805.21ng

response 391147

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.53
183.00	13.80	11.40
0.00	0.00	0.00