
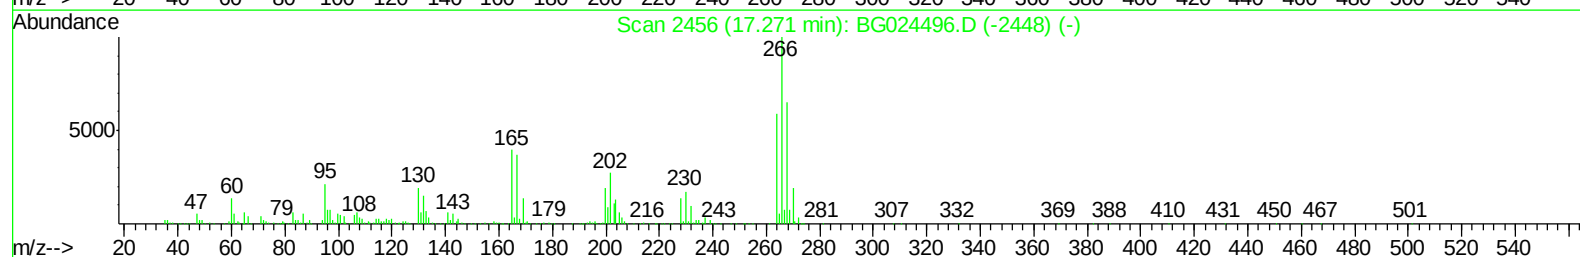
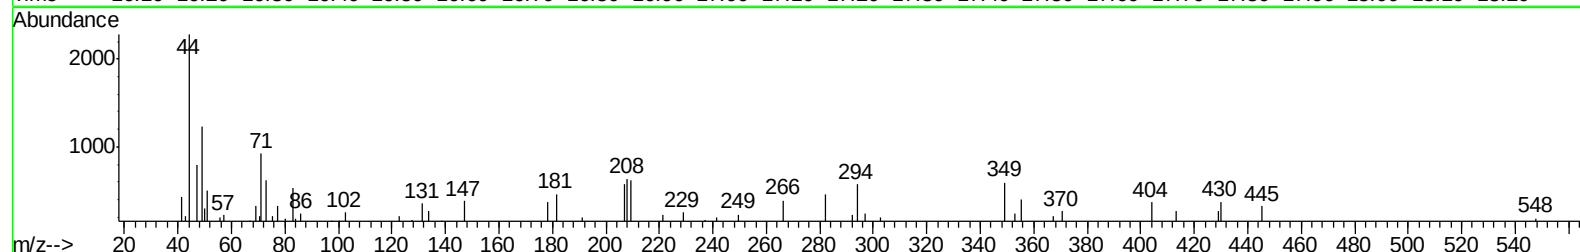


Data Path : Z:\HPCHEM1\BNA_G\Data\BG102516\
Data File : BG024501.D
Acq On : 25 Oct 2016 17:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 06:45:25 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:25:08 2016
Response via : Initial Calibration

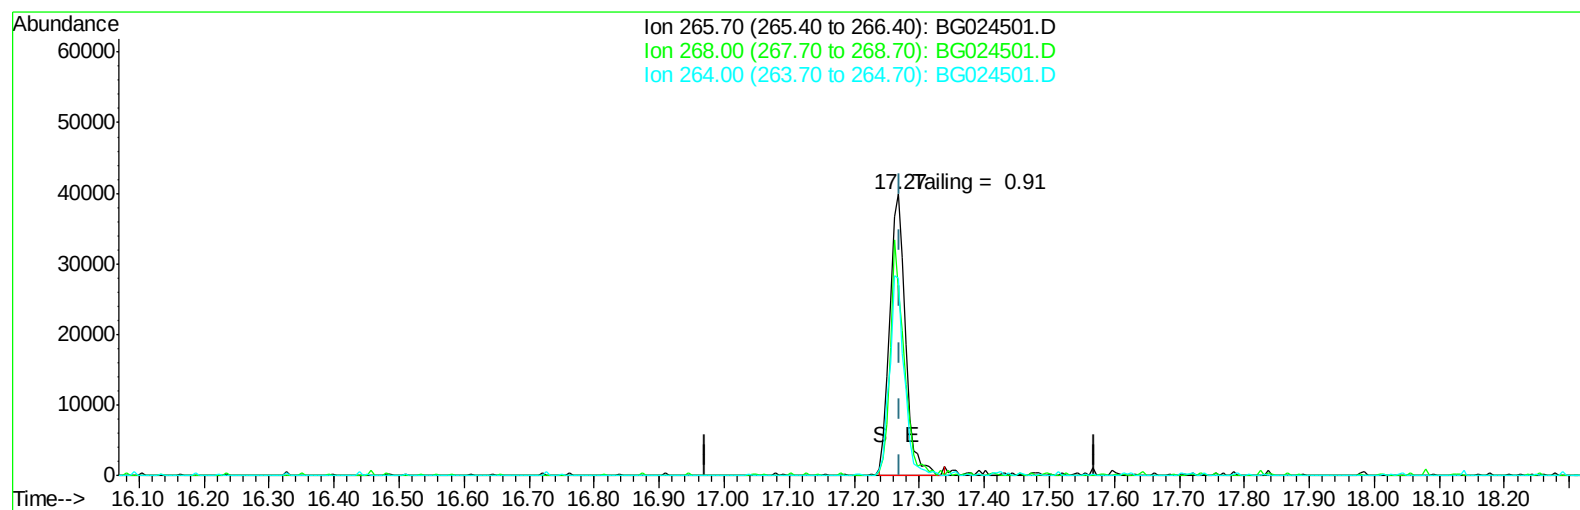

TIC: BG024501.D

(69) Pentachlorophenol (C)




17.080min (-0.191) 112.98ng

response 204

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG102516\
Data File : BG024501.D
Acq On : 25 Oct 2016 17:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 06:45:25 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 25 17:25:08 2016
Response via : Initial Calibration

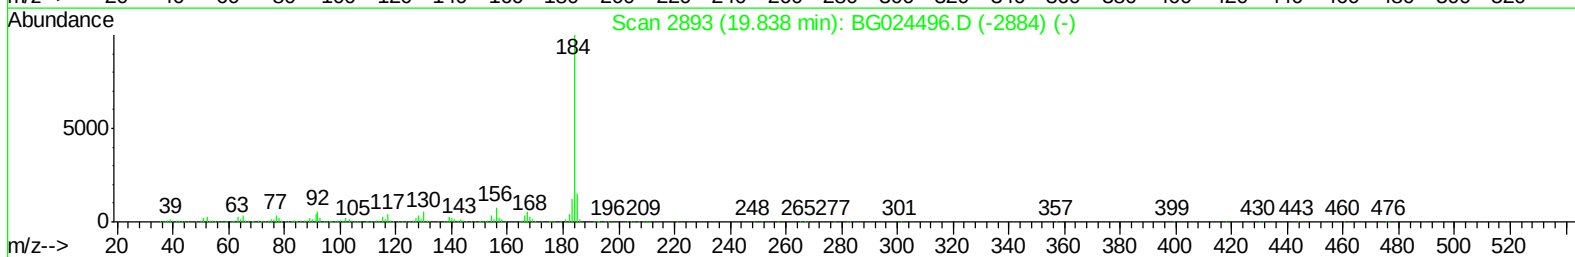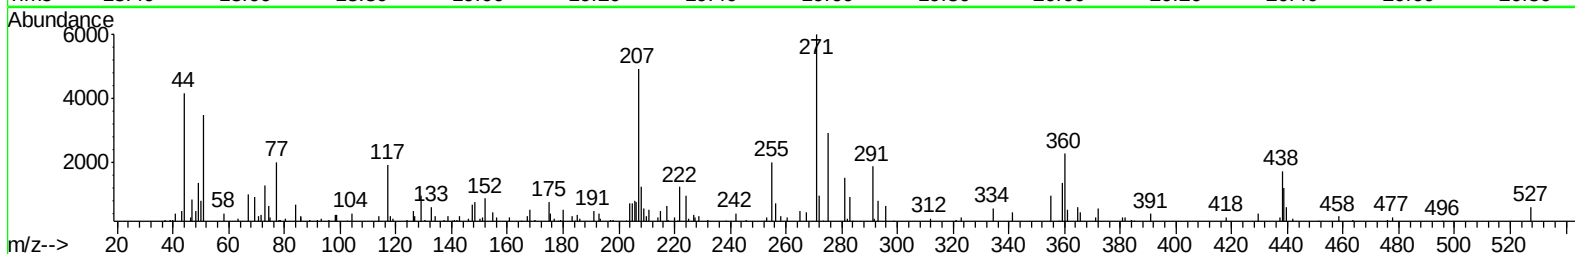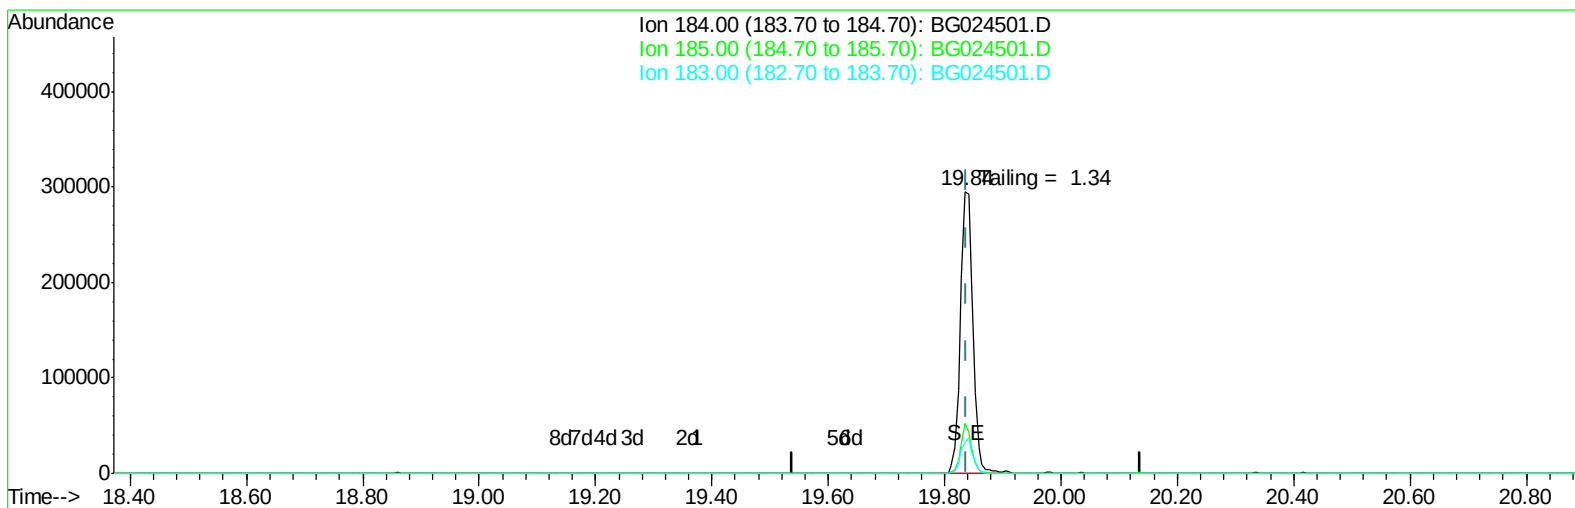

TIC: BG024501.D

(76) Benzidine

19.377min (-0.462) 26.53ng

response 55

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	222.29#
183.00	13.80	192.36#
0.00	0.00	0.00