


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102516\
 Data File : BG024491.D
 Acq On : 25 Oct 2016 11:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

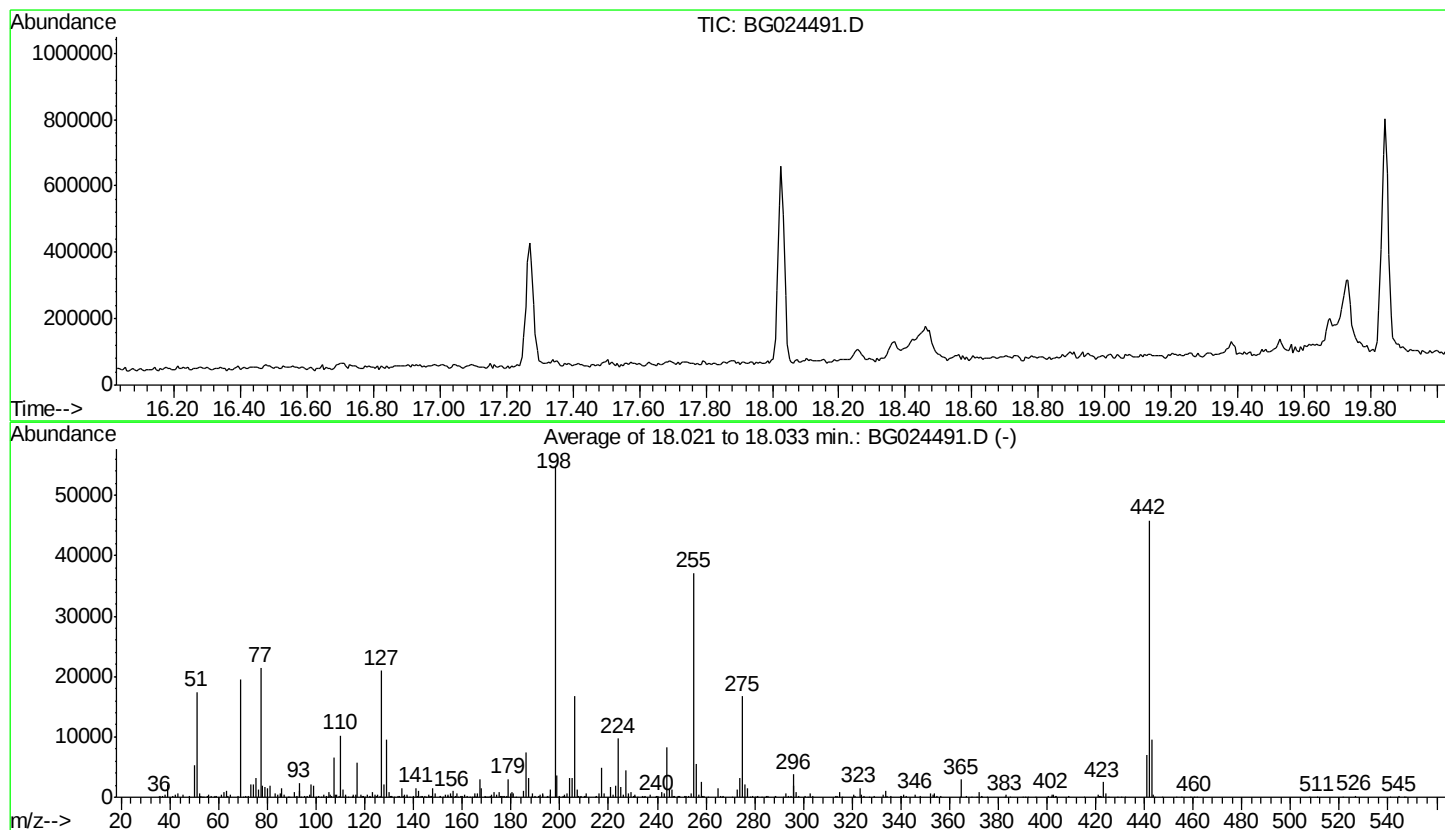

AutoFind: Scans 2584, 2585, 2586; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	17410	PASS
68	69	0.00	2	1.4	272	PASS
69	198	0.00	100	35.5	19503	PASS
70	69	0.00	2	0.2	42	PASS
127	198	10	80	38.1	20939	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54922	PASS
199	198	5	9	6.5	3586	PASS
275	198	10	60	30.4	16711	PASS
365	198	1	100	5.3	2891	PASS
441	442	0.01	24	15.4	7075	PASS
442	198	50	100	83.5	45834	PASS
443	442	15	24	21.0	9632	PASS