

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
 Data File : BG029437.D
 Acq On : 25 Oct 2017 11:20
 Operator : SJ/JU
 Sample : I5793-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0D55

Quant Time: Oct 26 06:51:10 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 05:48:30 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	86786	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	406995	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.78	164	266271	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.52	188	638474	20.00	ng/ul	0.00
75) Chrysene-d12	21.80	240	685896	20.00	ng/ul	0.00
83) Perylene-d12	25.10	264	688975	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.55	96	3719	1.74	ng/uL	0.00
5) Phenol-d5	7.31	99	79825	9.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	45805	8.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	64534	10.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	59849	8.90	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	30803	10.54	ng/ul	0.00
22) 2-Nitrophenol-d4	10.05	143	36536	12.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	72816	10.67	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	70103	8.85	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	236887	10.41	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	294536	10.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	20354	4.84	ng/ul	0.00
57) Fluorene-d10	15.77	176	218655	11.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	25444	8.16	ng/ul	0.00
70) Anthracene-d10	17.62	188	325063	10.77	ng/ul	0.00
76) Pyrene-d10	19.89	212	381870	10.76	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.87	264	346721	10.63	ng/ul	-0.01


Target Compounds					Ovalue	
6) Phenol	7.34	94	11587	1.344	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
Data File : BG029437.D
Acq On : 25 Oct 2017 11:20
Operator : SJ/JU
Sample : I5793-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0D55

Quant Time: Oct 26 06:51:10 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 05:48:30 2017
Response via : Initial Calibration

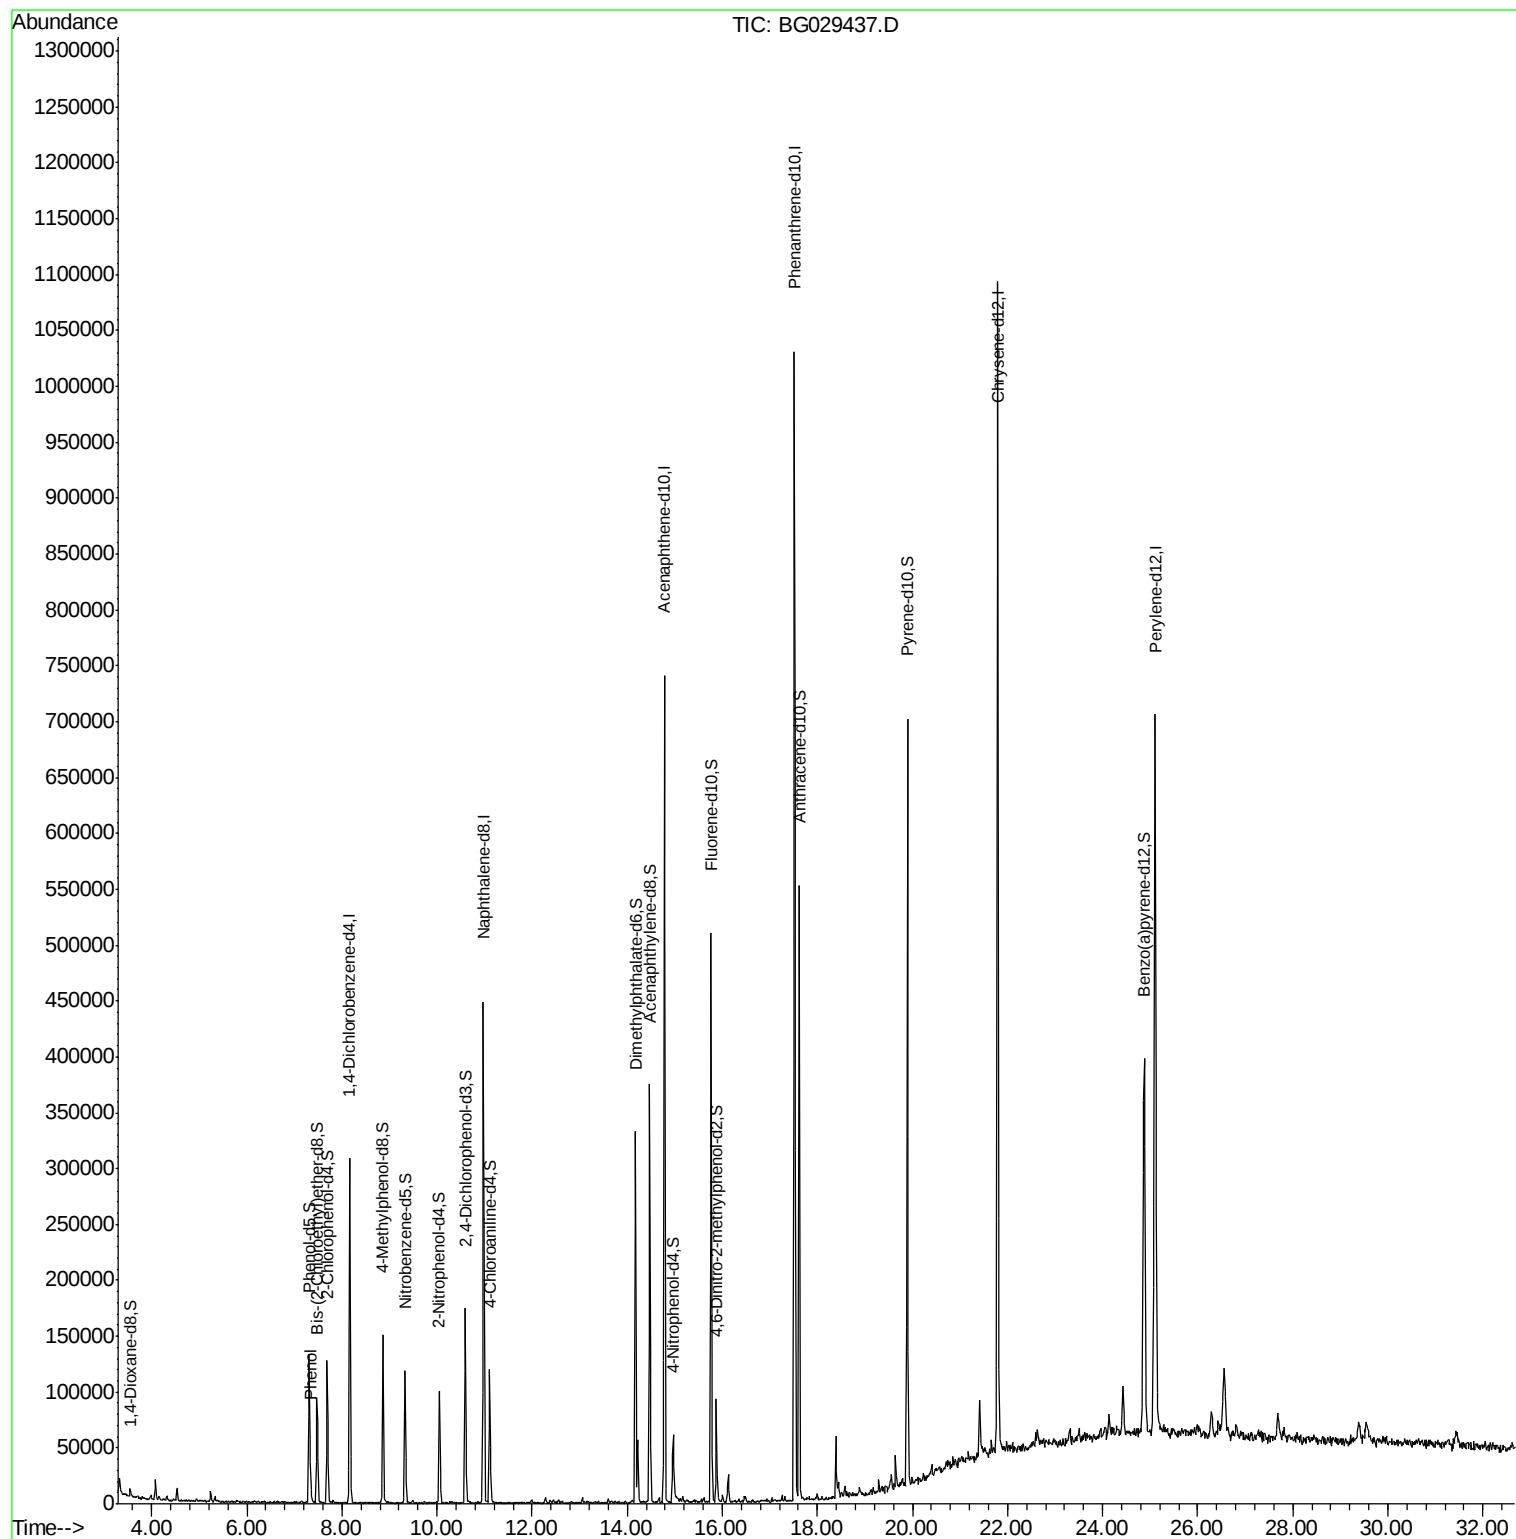

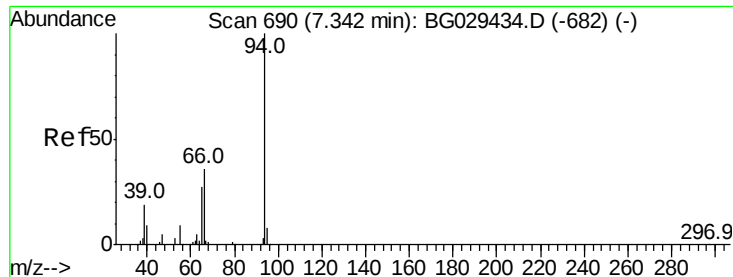

#6

Phenol

Concen: 1.344 ng/ul

RT: 7.34 min Scan# 690

Delta R.T. 0.00 min

Lab File: BG029437.D

Acq: 25 Oct 2017 11:20

Instrument :

BNA_G

ClientSampleId :

B0D55

Tot Ion: 94 Resp: 11587

Ion Ratio Lower Upper

94 100

65 27.5 27.1 40.7

66 39.5 34.6 52.0

