

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
 Data File : BG029440.D
 Acq On : 25 Oct 2017 13:18
 Operator : SJ/JU
 Sample : I5793-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0D64

Quant Time: Oct 26 06:49:13 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 05:48:30 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.16	152	93050	20.00	ng/ul	0.00
18) Naphthalene-d8	10.98	136	432630	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	286942	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.52	188	673220	20.00	ng/ul	0.00
75) Chrysene-d12	21.79	240	714486	20.00	ng/ul	0.00
83) Perylene-d12	25.11	264	720563	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	7448	3.25	ng/uL	0.00
5) Phenol-d5	7.32	99	168752	18.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	99696	17.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.69	132	135372	21.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.86	113	145584	20.18	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	68494	22.05	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	83163	26.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	150026	20.69	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	192126	22.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.18	166	502000	20.46	ng/ul	0.00
46) Acenaphthylene-d8	14.48	160	626074	20.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	66472	14.68	ng/ul	0.00
57) Fluorene-d10	15.77	176	460246	22.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.88	200	60459	18.40	ng/ul	0.00
70) Anthracene-d10	17.62	188	706054	22.18	ng/ul	0.00
76) Pyrene-d10	19.90	212	810586	21.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.88	264	771738	22.61	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	7.34	94	20098	2.175	ng/ul# 81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
Data File : BG029440.D
Acq On : 25 Oct 2017 13:18
Operator : SJ/JU
Sample : I5793-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
B0D64

Quant Time: Oct 26 06:49:13 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 05:48:30 2017
Response via : Initial Calibration

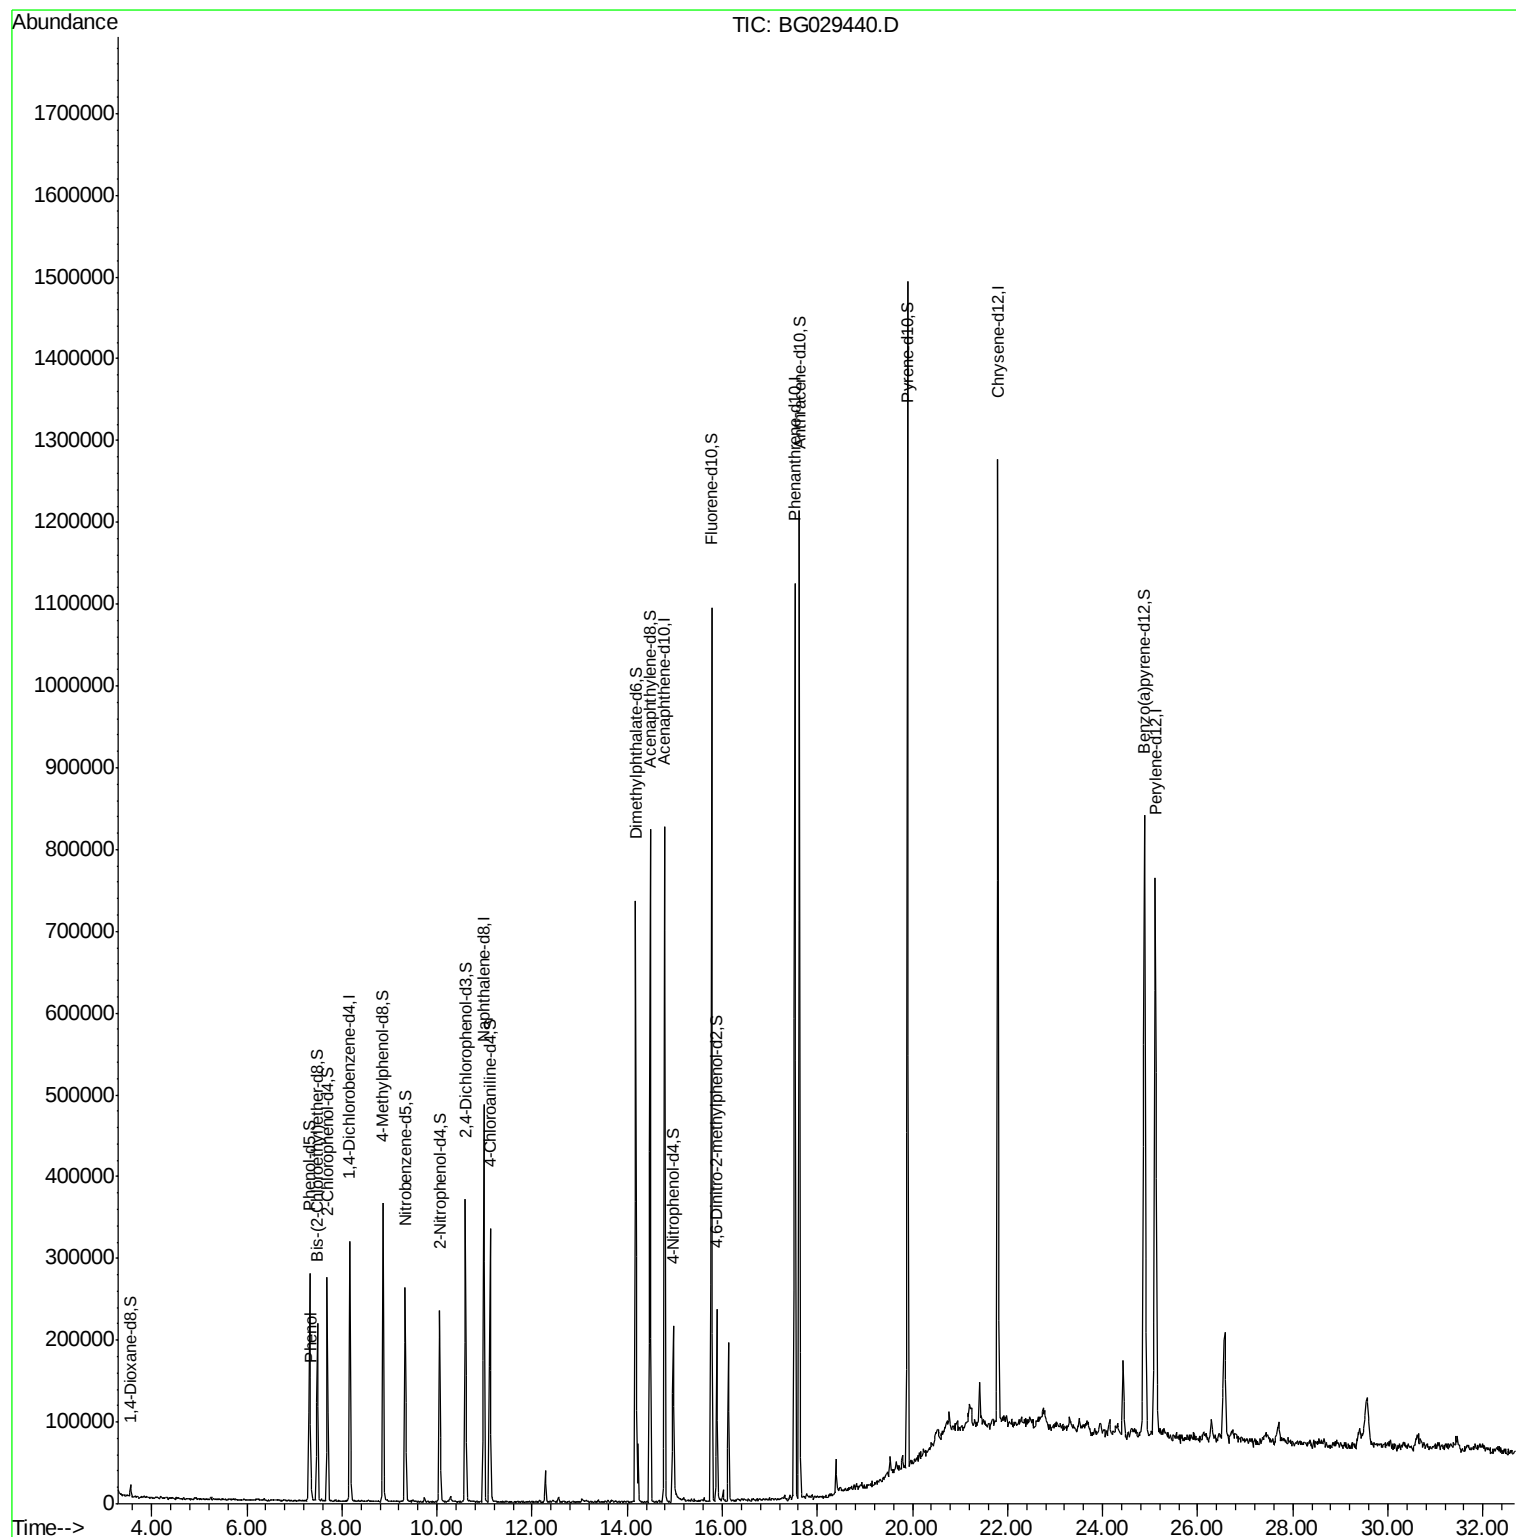

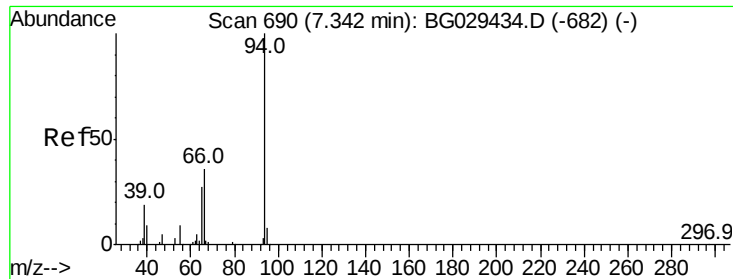

#6

Phenol

Concen: 2.175 ng/ul

RT: 7.34 min Scan# 690

Delta R.T. -0.00 min

Lab File: BG029440.D

Acq: 25 Oct 2017 13:18

Instrument :

BNA_G

ClientSampleId :

B0D64


Tot Ion: 94 Resp: 20098

Ion Ratio Lower Upper

94 100

65 21.6 27.1 40.7#

66 32.9 34.6 52.0#

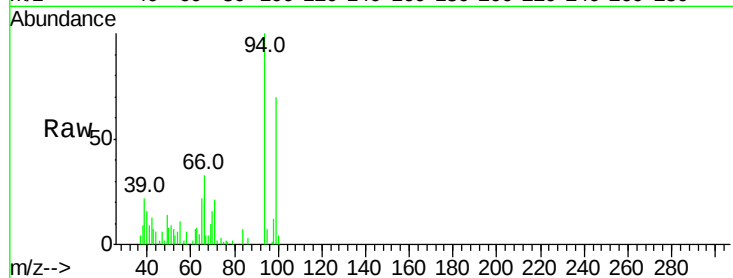

Abundance Ion 94.00 (93.70 to 94.70): BGC
 Ion 65.00 (64.70 to 65.70): BGC
 Ion 66.00 (65.70 to 66.70): BGC

