

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
 Data File : BG029470.D
 Acq On : 26 Oct 2017 9:39
 Operator : SJ/JU
 Sample : I5792-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0D21

Manual Integrations
 APPROVED

Sohil
 10/27/2017 5:32:35 PM

Quant Time: Oct 26 17:15:38 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 09:08:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	103799	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	478437	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	286911	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	605181	20.00	ng/ul	0.00
75) Chrysene-d12	21.81	240	618391	20.00	ng/ul	0.00
83) Perylene-d12	25.13	264	625975	20.00	ng/ul	0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.55	96	10895	4.27	ng/uL	0.00
5) Phenol-d5	7.32	99	259759	26.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.49	67	153653	24.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	212574	30.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.88	113	213054	26.48	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	107422	31.28	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	130208	37.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	235552	29.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.12	131	198469	21.30	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	688826	28.08	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	880716	29.52	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	90902	20.07	ng/ul	0.00
57) Fluorene-d10	15.78	176	611715	30.45	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.89	200	61075	20.67	ng/ul	0.00
70) Anthracene-d10	17.63	188	856108	29.91	ng/ul	0.00
76) Pyrene-d10	19.90	212	938723	29.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.90	264	918985	31.00	ng/ul	0.02
Target Compounds						
6) Phenol	7.35	94	29566	2.868	ng/ul	91
44) Dimethylphthalate	14.23	163	49994	2.090	ng/ul	97
69) Phenanthrene	17.57	178	72319	2.211	ng/ul	96
74) Fluoranthene	19.57	202	145145	3.970	ng/ul	99
77) Pyrene	19.93	202	158850	3.833	ng/ul	97
80) Benzo(a)anthracene	21.78	228	100151m	2.584	ng/ul	
82) Chrysene	21.85	228	99334	2.821	ng/ul#	95
85) Benzo(b)fluoranthene	24.07	252	116617m	3.103	ng/ul	
88) Benzo(a)pyrene	24.97	252	91880	2.512	ng/ul#	89
89) Indeno(1,2,3-cd)pyrene	28.92	276	45750	1.105	ng/ul#	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
Data File : BG029470.D
Acq On : 26 Oct 2017 9:39
Operator : SJ/JU
Sample : I5792-11
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
B0D21

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:35 PM

Quant Time: Oct 26 17:15:38 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 09:08:53 2017
Response via : Initial Calibration

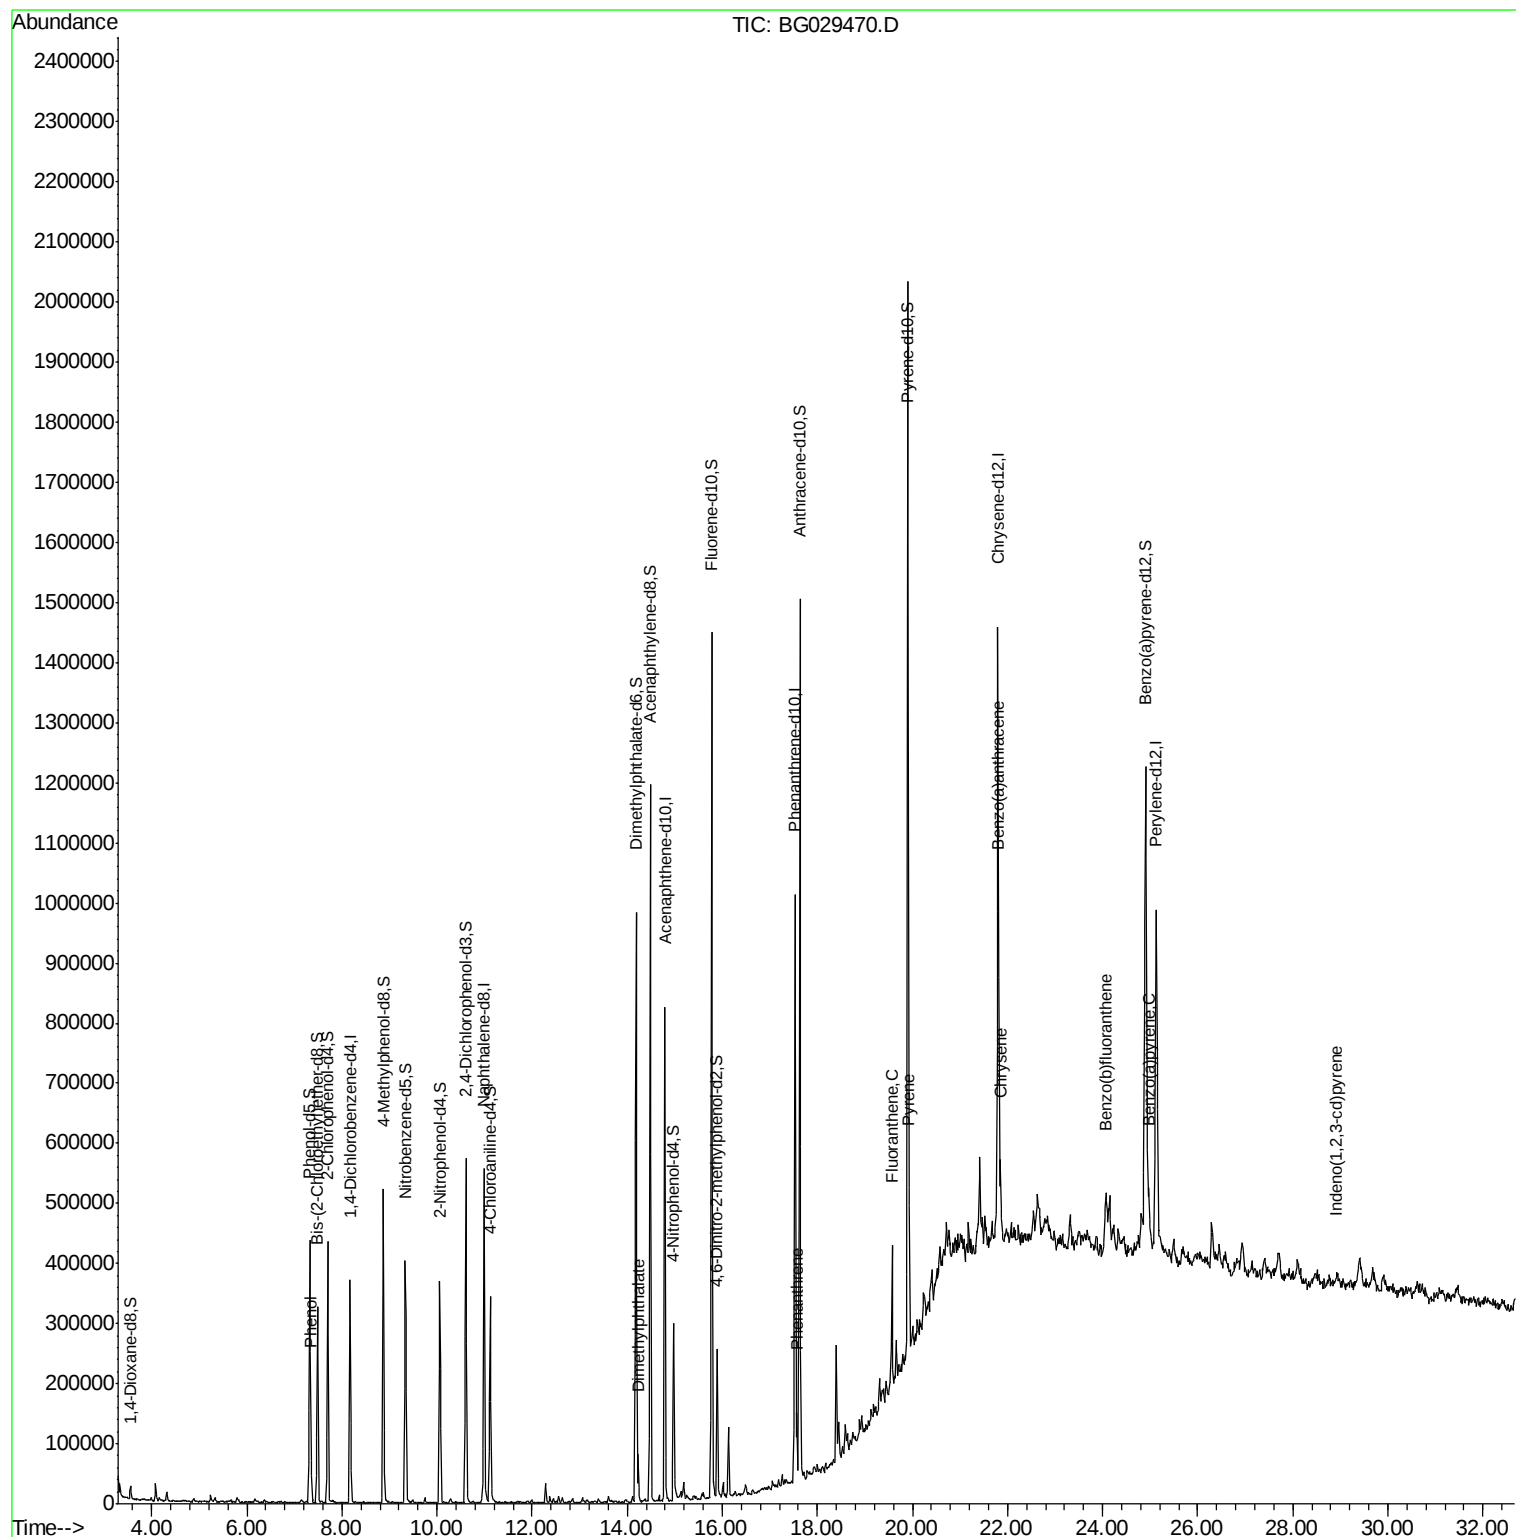

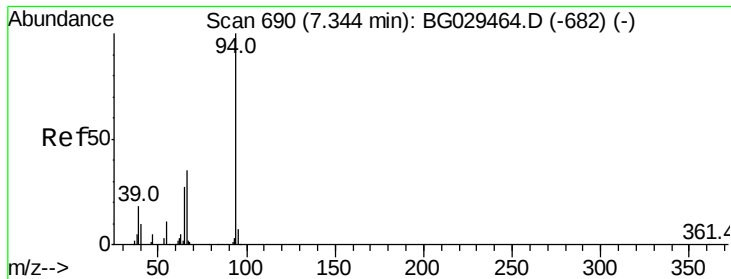

#6

Phenol

Concen: 2.868 ng/ul

RT: 7.35 min Scan# 691

Delta R.T. 0.00 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Instrument :

BNA_G





ClientSampleId :

B0D21

Tot Ion	94	Resp:	29566
Ion Ratio	Lower	Upper	
94	100		
65	29.0	27.1	40.7
66	37.3	34.6	52.0

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:35 PM

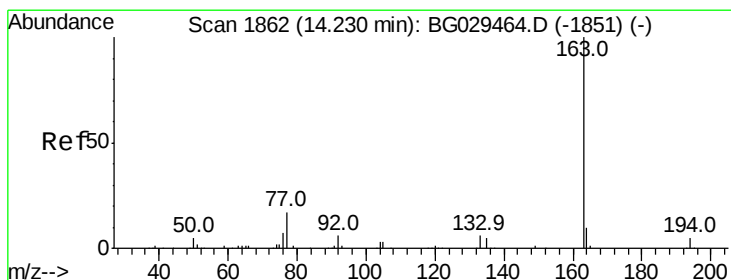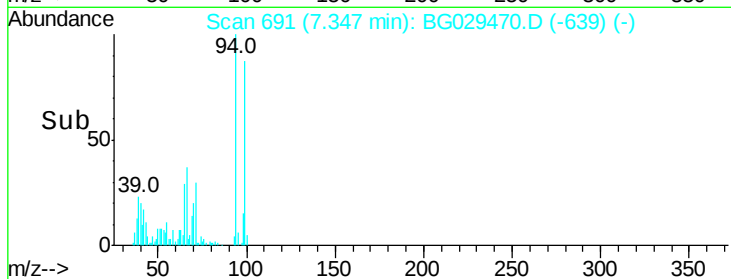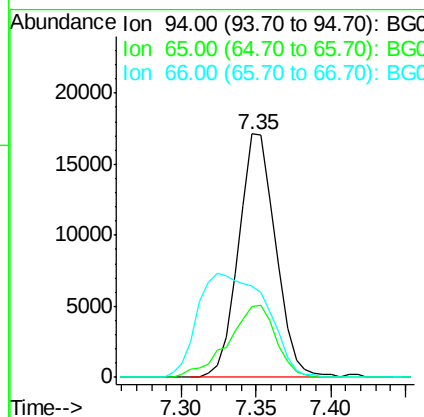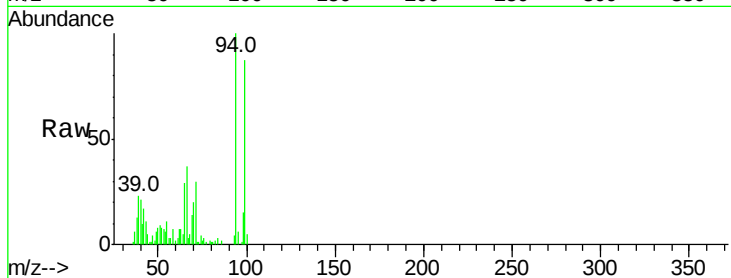

#44

Dimethylphthalate

Concen: 2.090 ng/ul




RT: 14.23 min Scan# 1862


Delta R.T. -0.00 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Tgt Ion	163	Resp:	49994
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.5	5.3
164	10.6	7.6	11.4

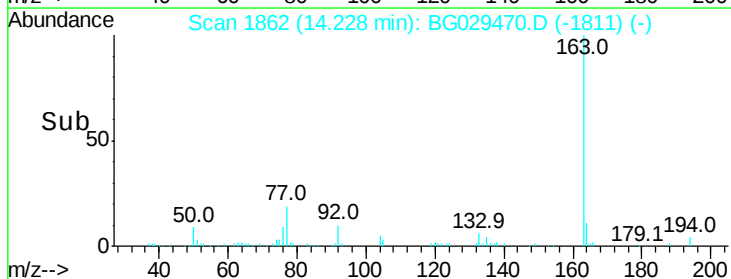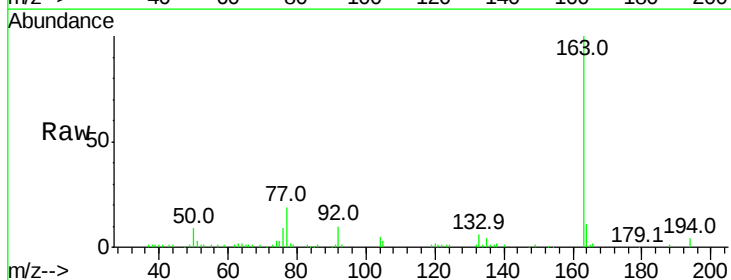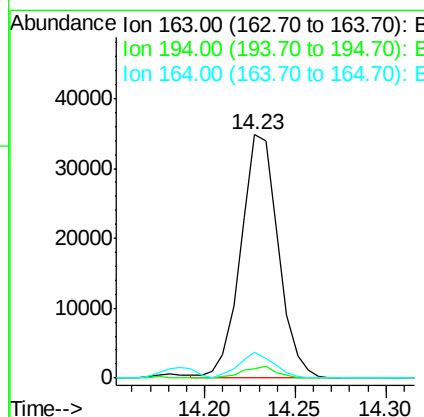

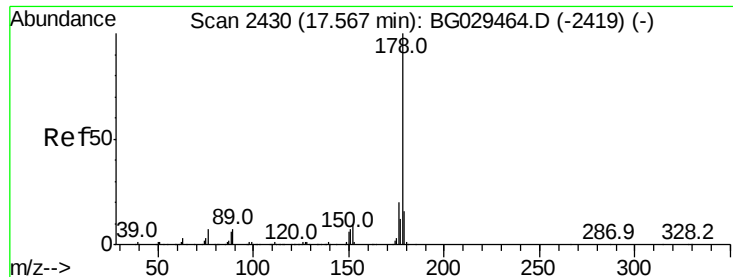





#69
Phenanthrene
Concen: 2.211 ng/ul
RT: 17.57 min Scan# 2431
Delta R.T. 0.00 min
Lab File: BG029470.D
Acq: 26 Oct 2017 9:39

Instrument :
BNA_G
ClientSampleId :
B0D21

Tot Ion	Ratio	Lower	Upper
178	100		
179	14.6	13.0	19.6
176	17.3	15.3	22.9




Manual Integrations
APPROVED


Sohil
10/27/2017 5:32:35 PM

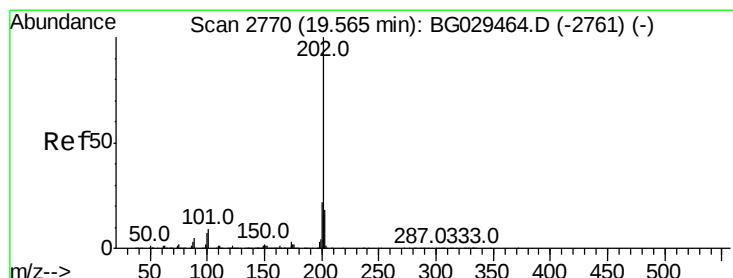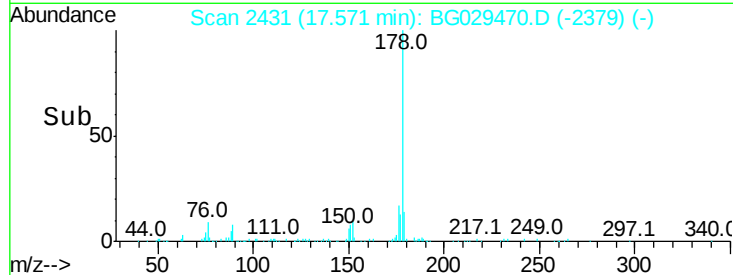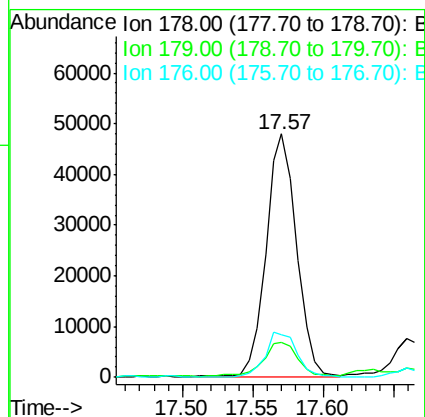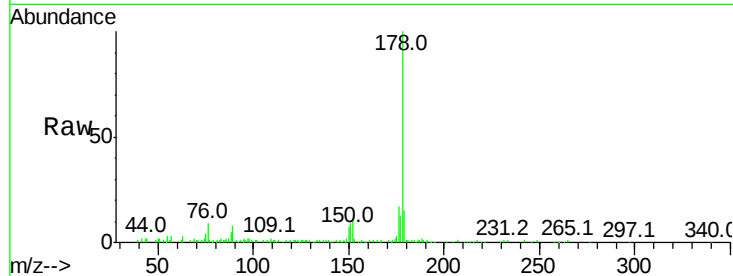

#74
Fluoranthene
Concen: 3.970 ng/ul
RT: 19.57 min Scan# 2771
Delta R.T. 0.00 min
Lab File: BG029470.D
Acq: 26 Oct 2017 9:39

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.9	7.4	11.2
100	6.7	5.6	8.4

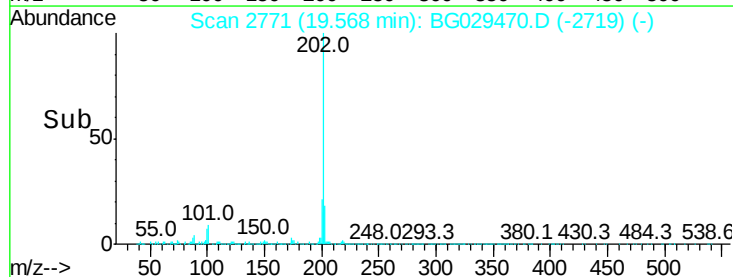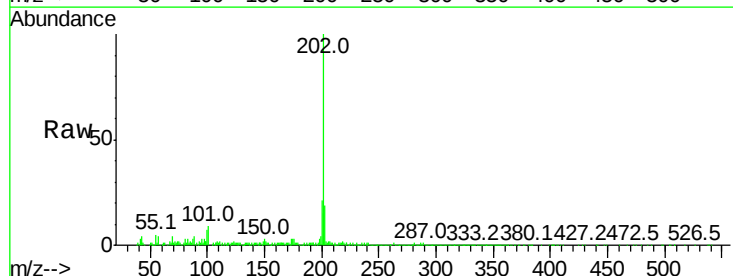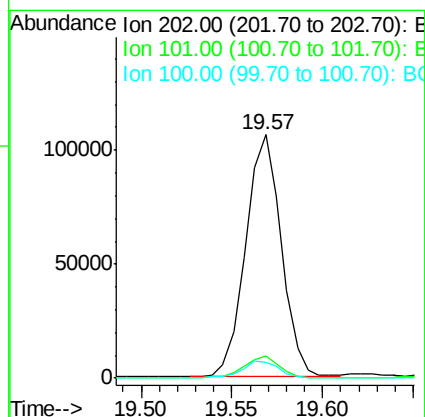

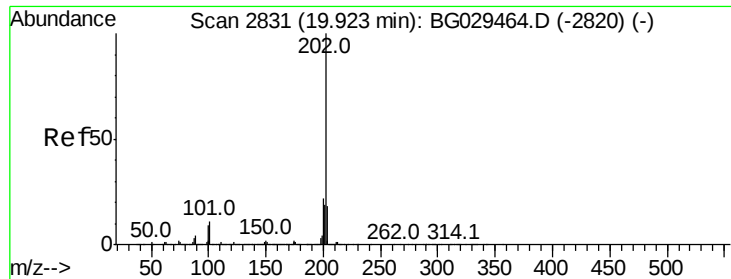





#77
 Pvrene
 Concen: 3.833 ng/ul
 RT: 19.93 min Scan# 2833
 Delta R.T. 0.01 min
 Lab File: BG029470.D
 Acq: 26 Oct 2017 9:39

Instrument :
 BNA_G
 ClientSampleId :
 B0D21

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	9.1	8.4	12.6
100	9.7	7.0	10.6




Manual Integrations
 APPROVED


Sohil
 10/27/2017 5:32:35 PM

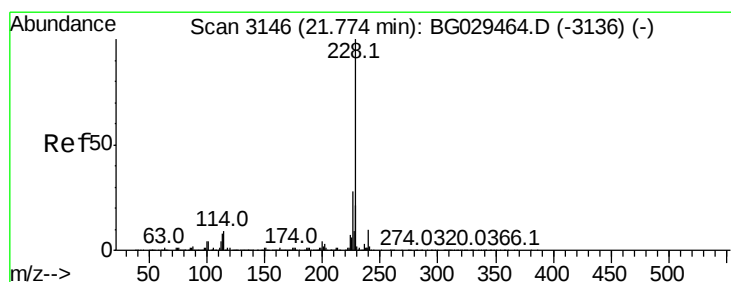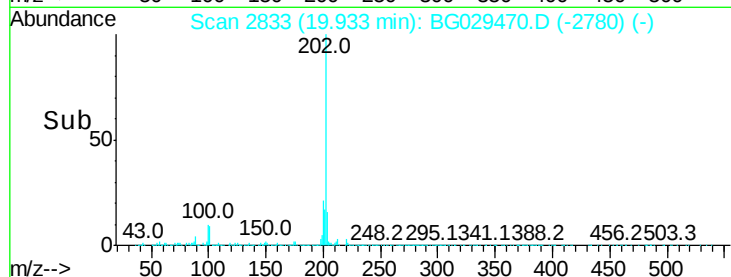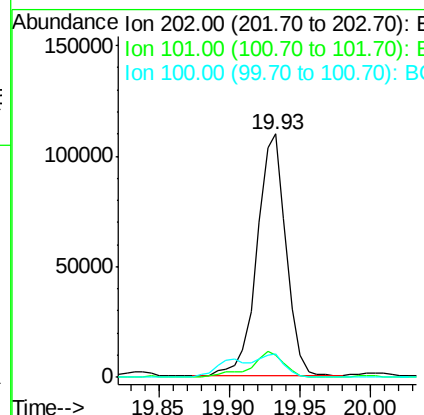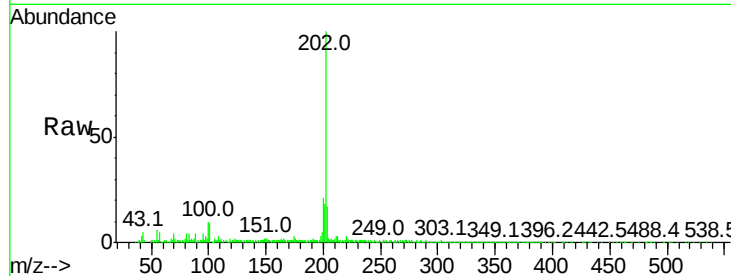

#80
 Benzo(a)anthracene
 Concen: 2.584 ng/ul m
 RT: 21.78 min Scan# 3148
 Delta R.T. 0.01 min
 Lab File: BG029470.D
 Acq: 26 Oct 2017 9:39

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	25.1	16.2	24.4#
226	30.1	22.2	33.2

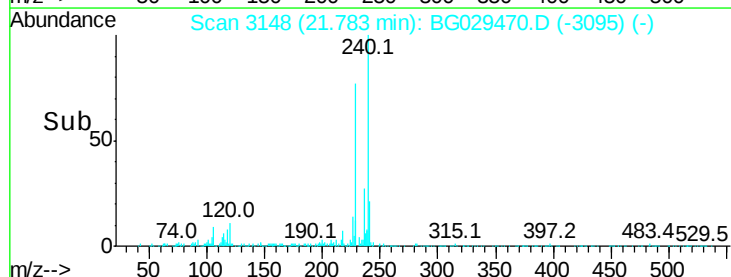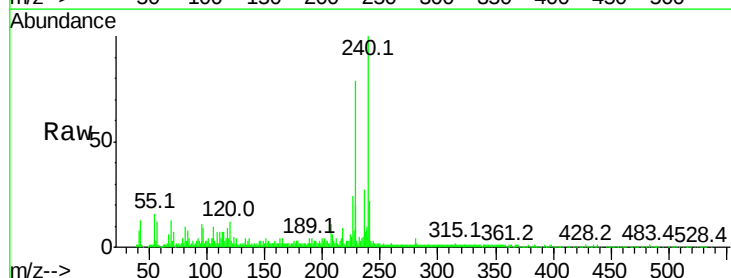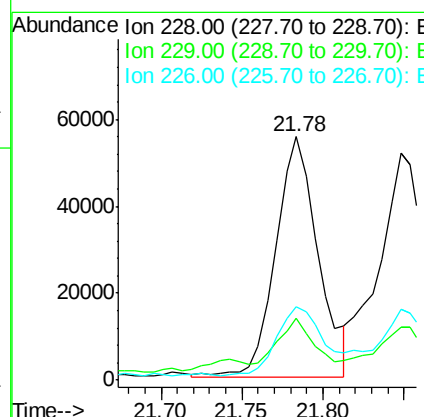

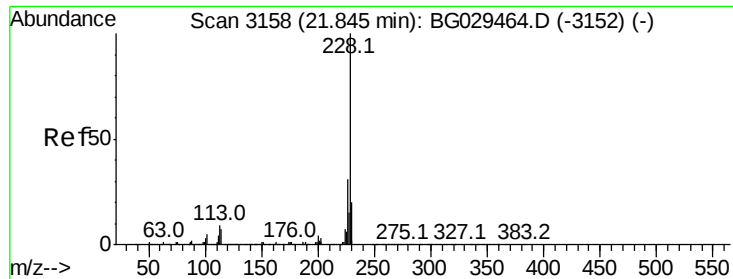

#82

Chrysene

Concen: 2.821 ng/ul

RT: 21.85 min Scan# 3159

Delta R.T. 0.00 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Instrument :

BNA_G





ClientSampled :

B0D21

Tot Ion:	228	Resp:	99334
Ion Ratio	Lower	Upper	
228	100		
226	31.1	24.2	36.2
229	23.0	15.2	22.8#

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:35 PM

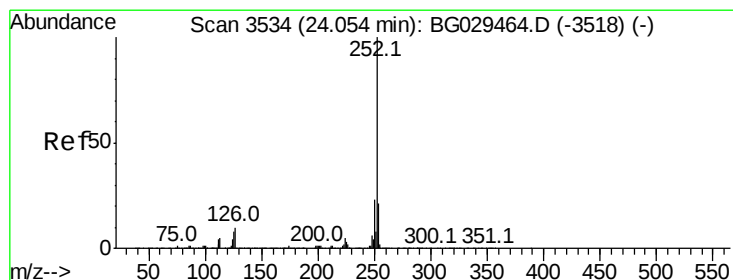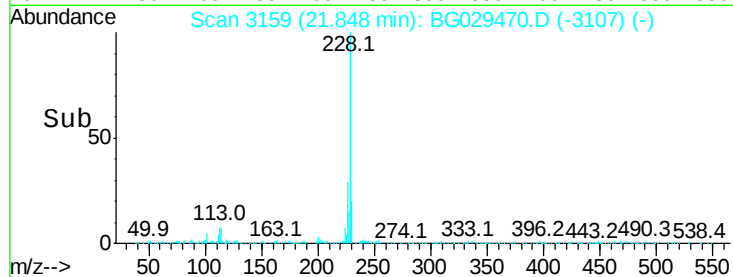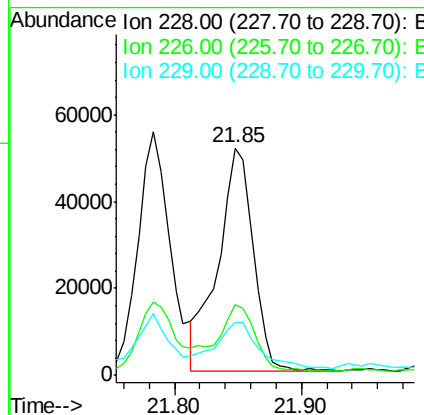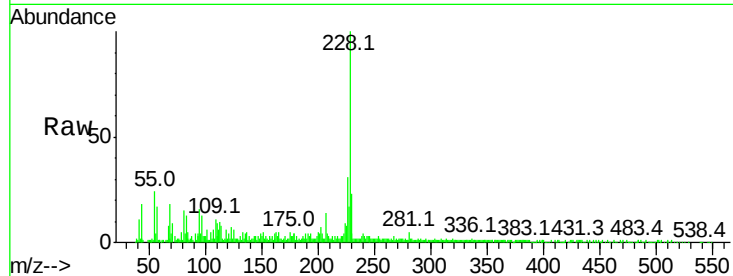

#85

Benzo(b)fluoranthene

Concen: 3.103 ng/ul m




RT: 24.07 min Scan# 3537


Delta R.T. 0.02 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Tgt Ion:	252	Resp:	116617
Ion Ratio	Lower	Upper	
252	100		
253	26.1	17.0	25.4#
125	14.0	7.5	11.3#

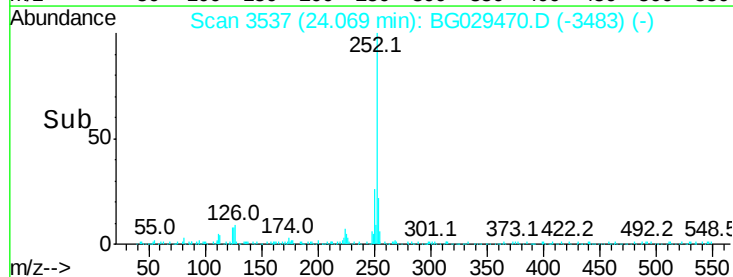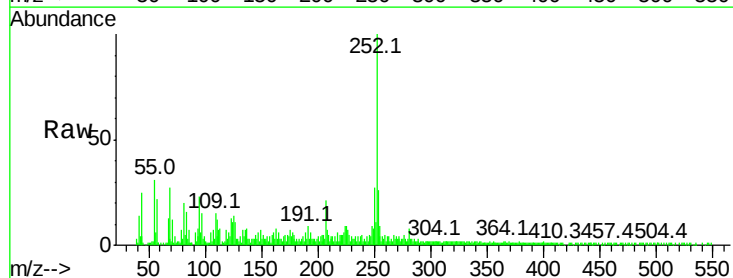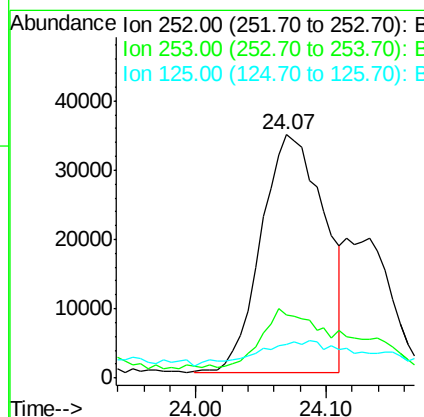

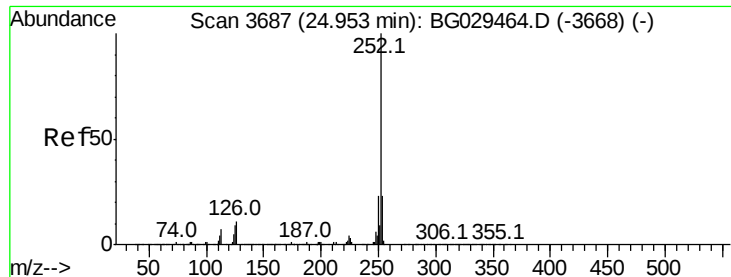

#88

Benzo(a)pyrene

Concen: 2.512 ng/ul

RT: 24.97 min Scan# 3691

Delta R.T. 0.02 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Instrument :

BNA_G





ClientSampled :

B0D21

Tot Ion	Ratio	Lower	Upper
252	100		
253	27.3	17.1	25.7#
125	12.9	7.8	11.8#

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:35 PM

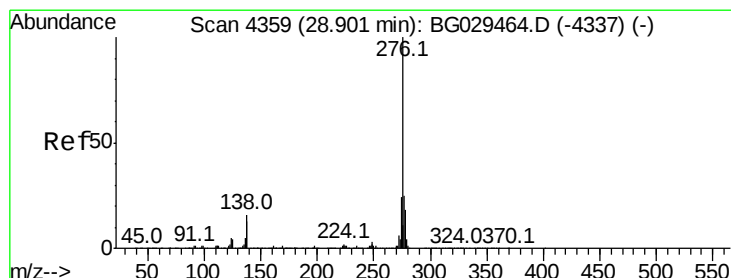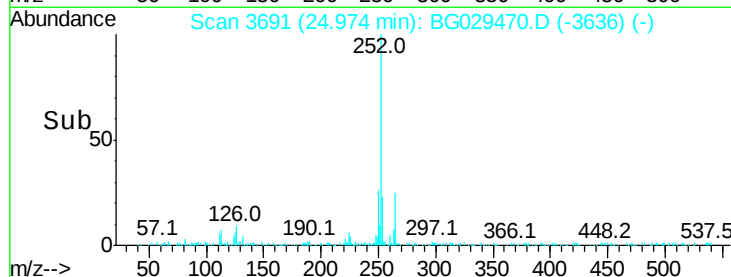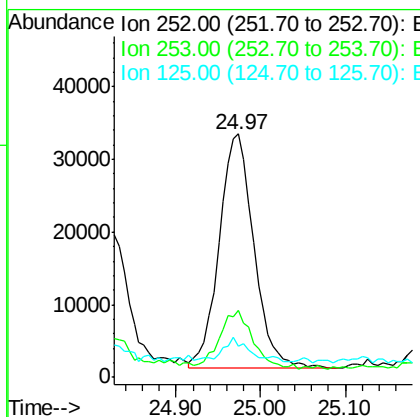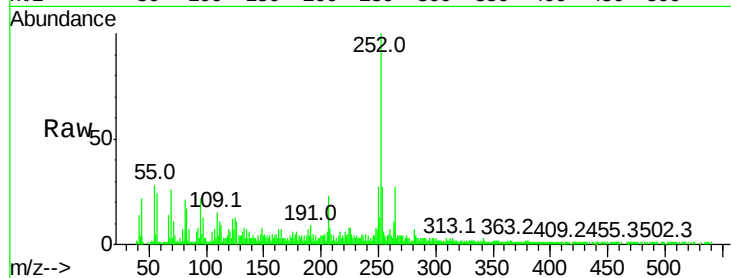

#89

Indeno(1,2,3-cd)pyrene

Concen: 1.105 ng/ul

RT: 28.92 min Scan# 4362

Delta R.T. 0.02 min

Lab File: BG029470.D

Acq: 26 Oct 2017 9:39

Tgt Ion	Ratio	Lower	Upper
276	100		
138	24.6	13.4	20.0#
277	30.4	18.6	28.0#

