

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
 Data File : BG029474.D
 Acq On : 26 Oct 2017 12:18
 Operator : SJ/JU
 Sample : I5792-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 B0D35

Manual Integrations
 APPROVED

Sohil
 10/27/2017 5:32:45 PM

Quant Time: Oct 26 17:29:18 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 09:08:53 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	90436	20.00	ng/ul	0.00
18) Naphthalene-d8	10.99	136	423101	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.79	164	264658	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.53	188	580459	20.00	ng/ul	0.00
75) Chrysene-d12	21.81	240	595462	20.00	ng/ul	0.00
83) Perylene-d12	25.13	264	589883	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	9763	4.39	ng/uL	0.00
5) Phenol-d5	7.32	99	227164	26.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.48	67	139779	25.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.70	132	188274	30.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.87	113	144100	20.55	ng/ul	0.00
19) Nitrobenzene-d5	9.33	128	98508	32.43	ng/ul	0.00
22) 2-Nitrophenol-d4	10.06	143	113282	36.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.60	165	204691	28.86	ng/ul	0.00
29) 4-Chloroaniline-d4	11.11	131	187823	22.80	ng/ul	0.00
43) Dimethylphthalate-d6	14.19	166	627416	27.73	ng/ul	0.00
46) Acenaphthylene-d8	14.49	160	827884	30.09	ng/ul	0.00
51) 4-Nitrophenol-d4	14.97	143	68243	16.34	ng/ul	0.00
57) Fluorene-d10	15.78	176	586137	31.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.89	200	48620	17.16	ng/ul	0.00
70) Anthracene-d10	17.63	188	836075	30.46	ng/ul	0.00
76) Pyrene-d10	19.90	212	939054	30.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.90	264	899886	32.21	ng/ul	0.02

Target Compounds

					Ovalue	
6) Phenol	7.35	94	24471	2.725	ng/ul#	87
44) Dimethylphthalate	14.23	163	44108	1.999	ng/ul	96
69) Phenanthrene	17.57	178	87071	2.775	ng/ul	96
74) Fluoranthene	19.57	202	147000	4.192	ng/ul	98
77) Pyrene	19.93	202	176106	4.413	ng/ul	98
80) Benzo(a)anthracene	21.78	228	91613	2.455	ng/ul	97
82) Chrysene	21.85	228	96130m	2.835	ng/ul	
85) Benzo(b)fluoranthene	24.07	252	106480	3.007	ng/ul#	92
88) Benzo(a)pyrene	24.97	252	81272	2.358	ng/ul#	95
89) Indeno(1,2,3-cd)pyrene	28.92	276	43893	1.125	ng/ul#	93
91) Benzo(g,h,i)perylene	30.13	276	41115	1.272	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102517\
Data File : BG029474.D
Acq On : 26 Oct 2017 12:18
Operator : SJ/JU
Sample : I5792-15
Misc :
ALS Vial : 18 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
B0D35

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:45 PM

Quant Time: Oct 26 17:29:18 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG101417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 09:08:53 2017
Response via : Initial Calibration

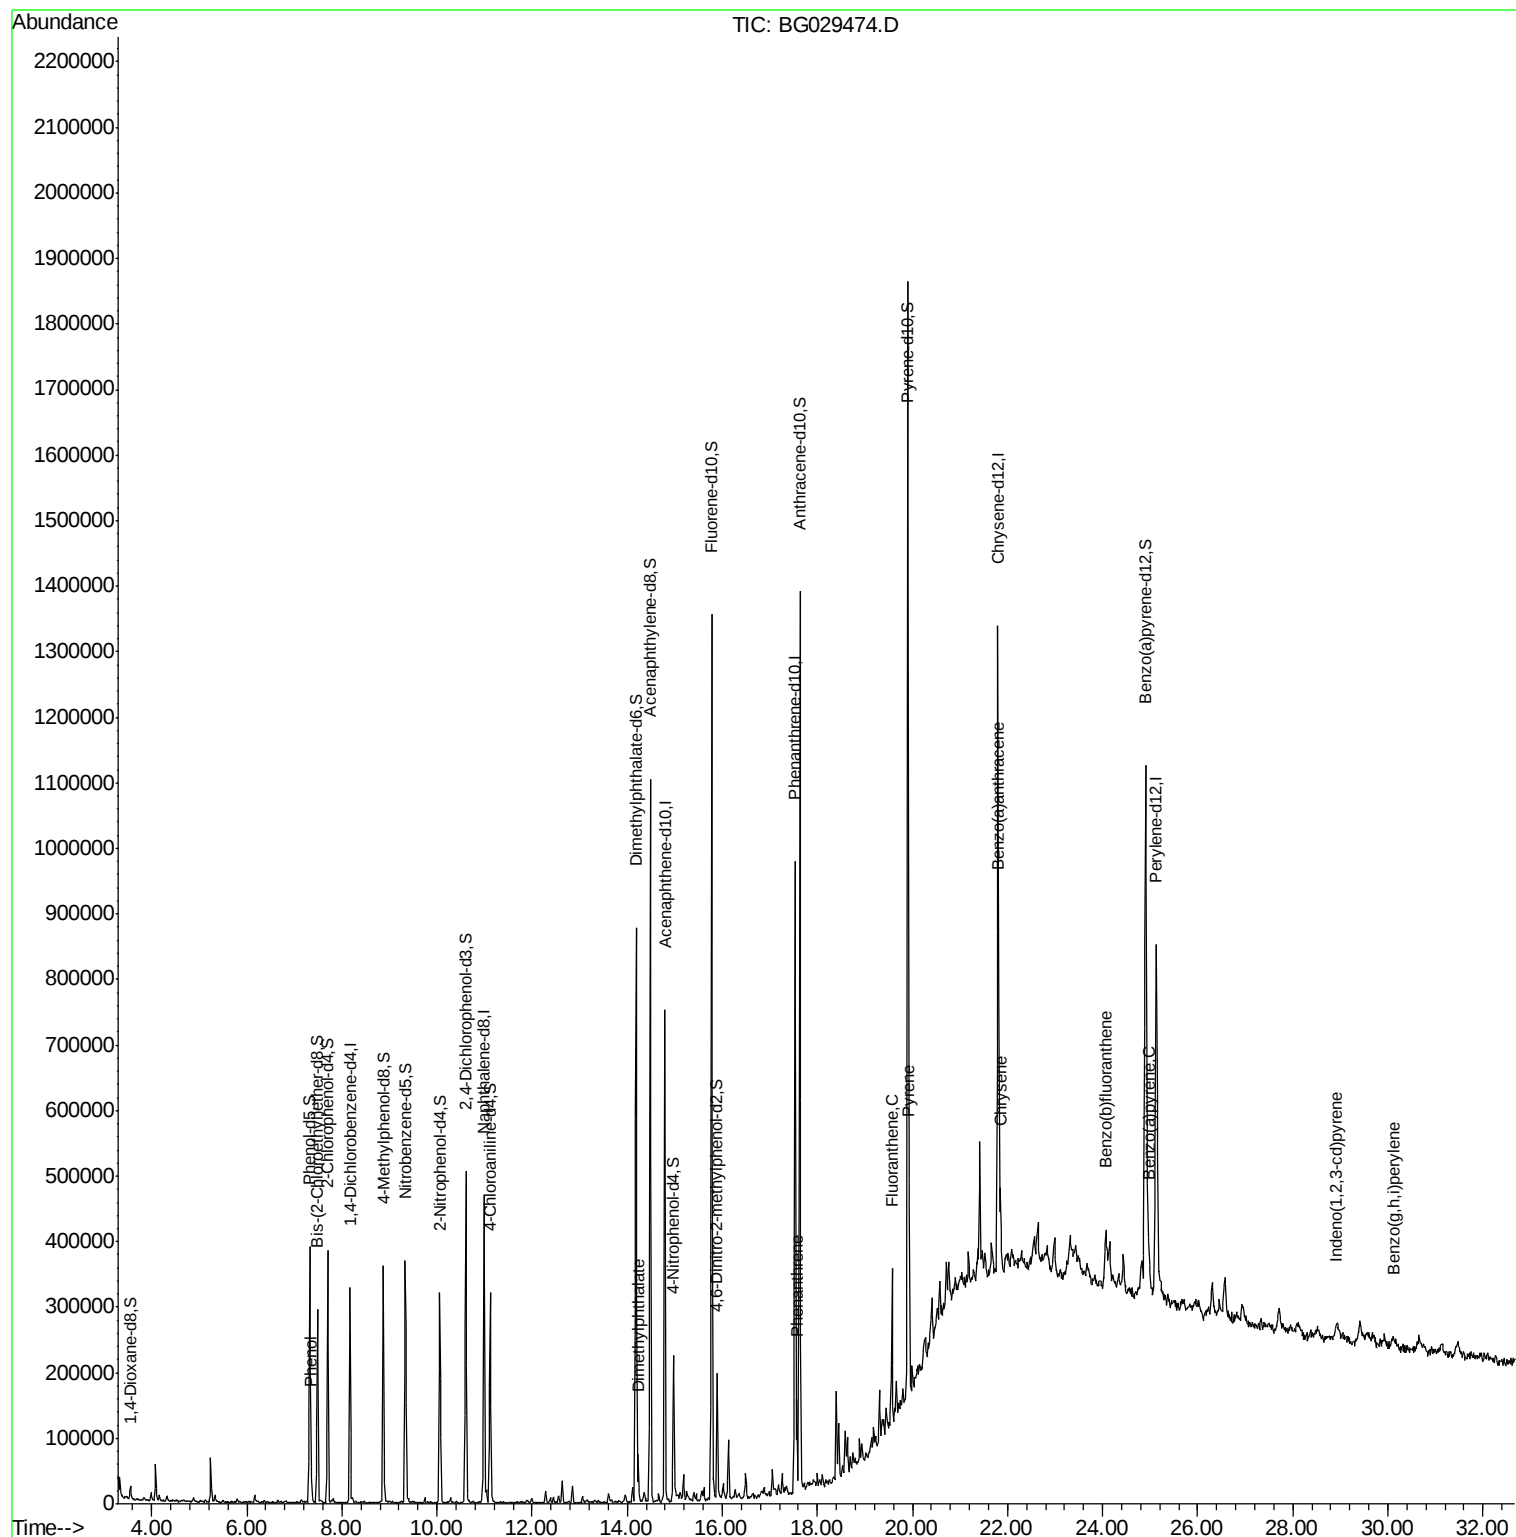

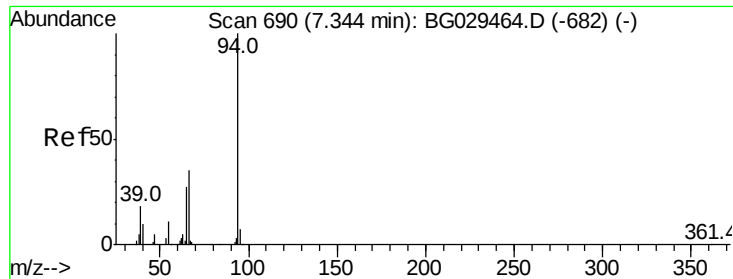

#6

Phenol

Concen: 2.725 ng/ul

RT: 7.35 min Scan# 692

Delta R.T. 0.01 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Instrument :

BNA_G





ClientSampled :

B0D35

Tot Ion:	94	Resp:	24471
Ion Ratio	Lower	Upper	
94	100		
65	28.1	27.1	40.7
66	34.0	34.6	52.0#

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:45 PM

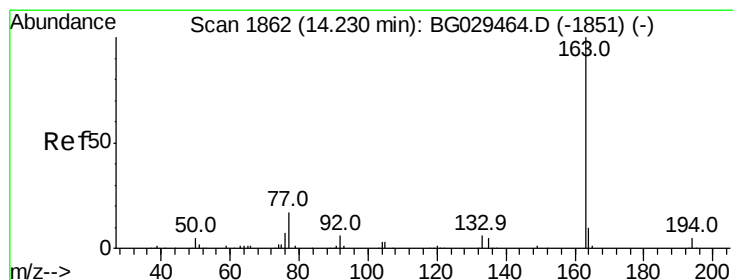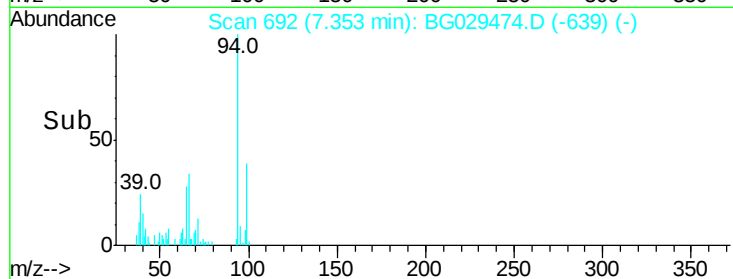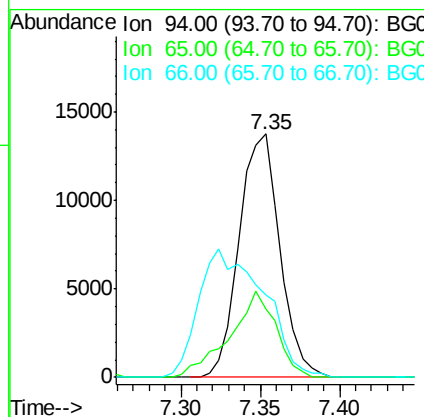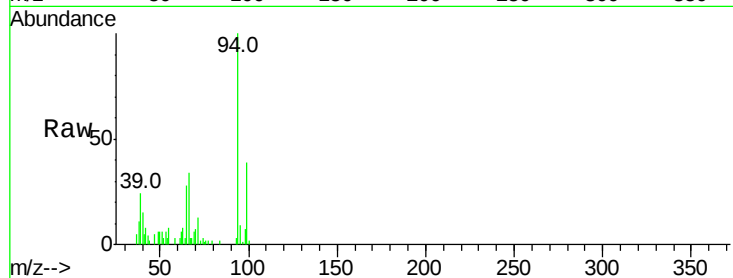

#44

Dimethylphthalate

Concen: 1.999 ng/ul




RT: 14.23 min Scan# 1862


Delta R.T. -0.00 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Tgt Ion:	163	Resp:	44108
Ion Ratio	Lower	Upper	
163	100		
194	3.8	3.5	5.3
164	11.3	7.6	11.4

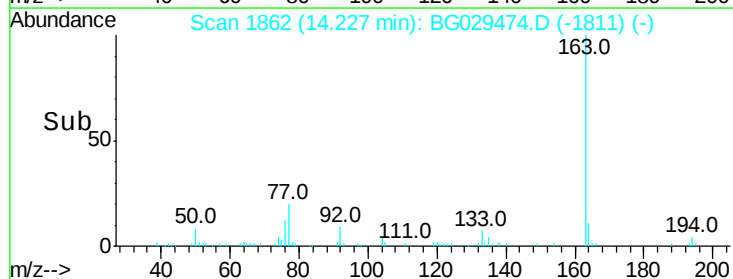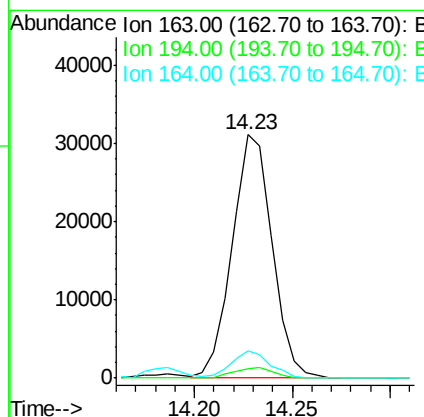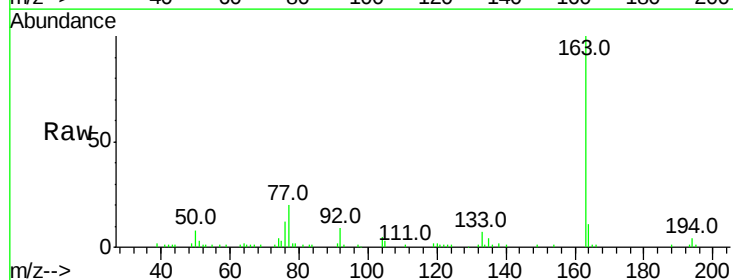

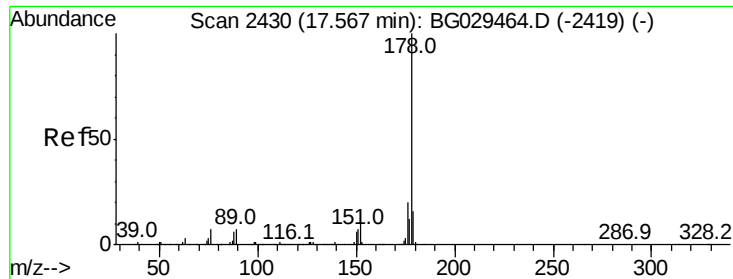





#69
 Phenanthrene
 Concen: 2.775 ng/ul
 RT: 17.57 min Scan# 2431
 Delta R.T. 0.00 min
 Lab File: BG029474.D
 Acq: 26 Oct 2017 12:18

Instrument :
 BNA_G
 ClientSampleId :
 B0D35

Tot Ion	Ratio	Lower	Upper
178	100		
179	16.6	13.0	19.6
176	21.8	15.3	22.9




Manual Integrations
 APPROVED


Sohil
 10/27/2017 5:32:45 PM

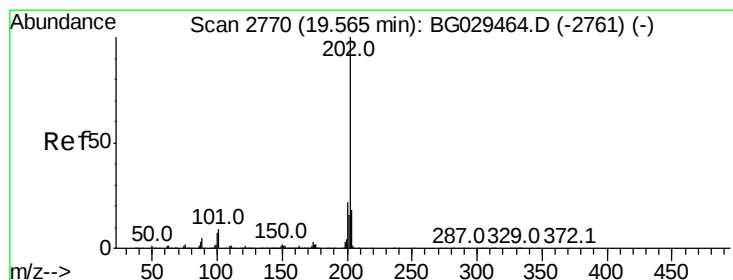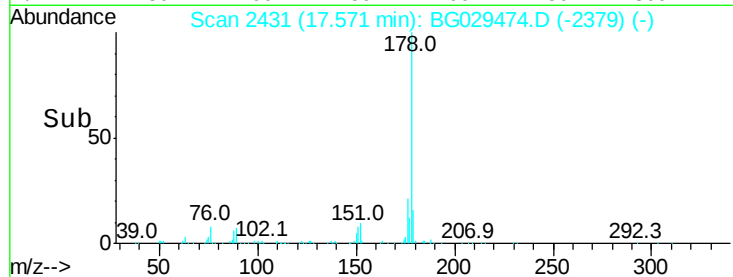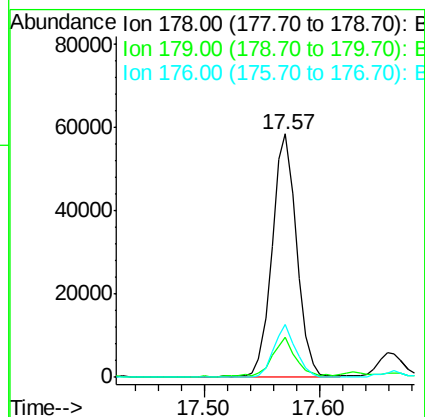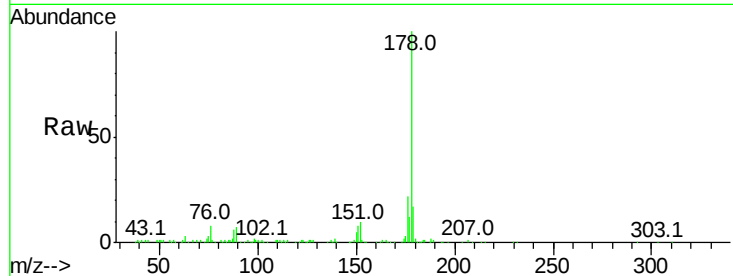

#74
 Fluoranthene
 Concen: 4.192 ng/ul
 RT: 19.57 min Scan# 2771
 Delta R.T. 0.00 min
 Lab File: BG029474.D
 Acq: 26 Oct 2017 12:18

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.2	7.4	11.2
100	6.6	5.6	8.4

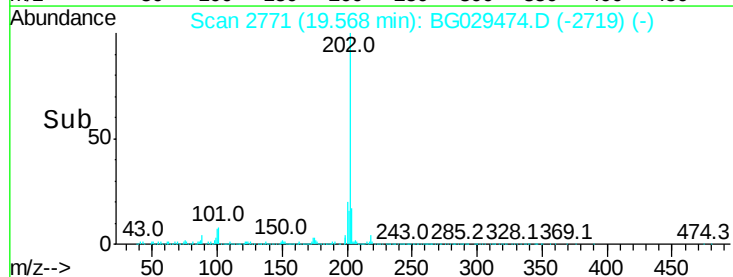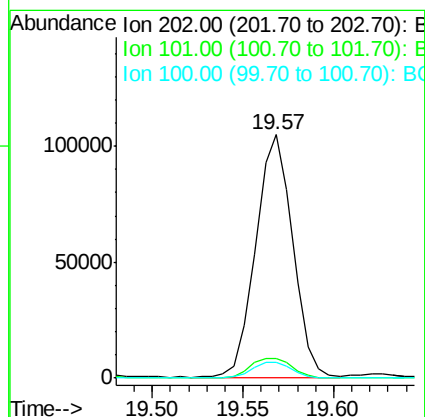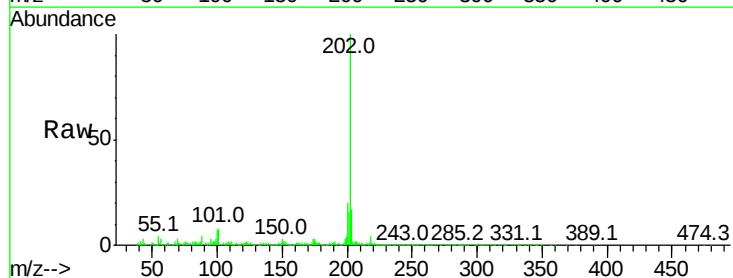

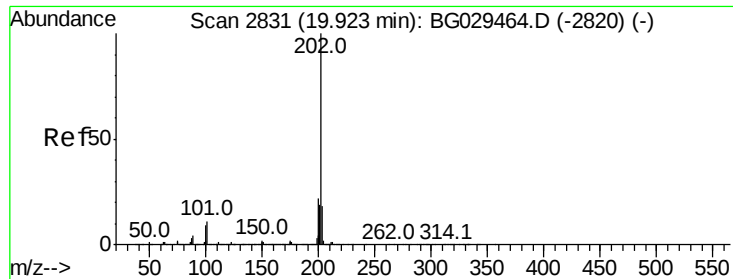

#77

Pvrene

Concen: 4.413 ng/ul

RT: 19.93 min Scan# 2833

Delta R.T. 0.01 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Instrument :

BNA_G





ClientSampleId :

B0D35

Tot Ion:	202	Resp:	176106
Ion Ratio	Lower	Upper	
202	100		
101	9.6	8.4	12.6
100	9.0	7.0	10.6

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:45 PM

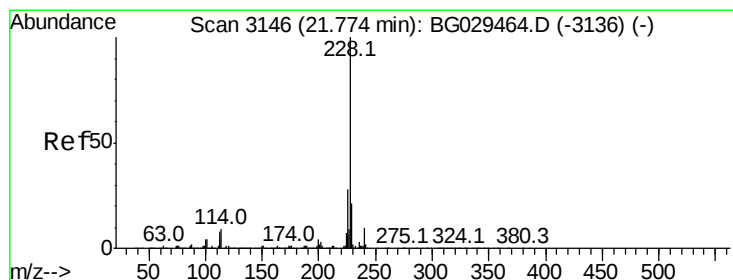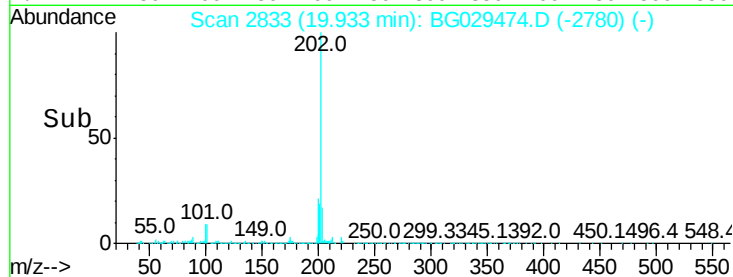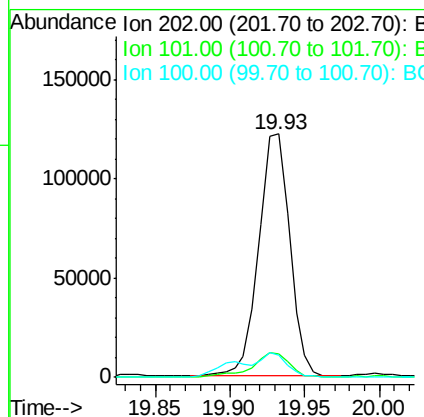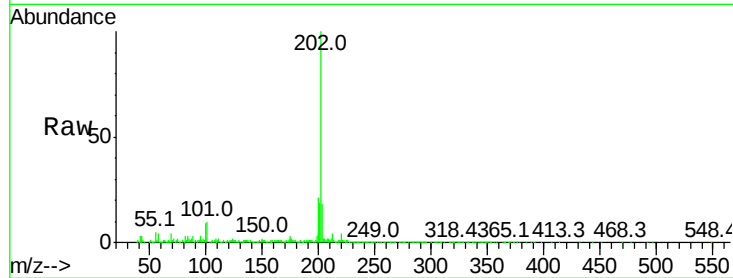

#80

Benzo(a)anthracene

Concen: 2.455 ng/ul




RT: 21.78 min Scan# 3148


Delta R.T. 0.01 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Tgt Ion:	228	Resp:	91613
Ion Ratio	Lower	Upper	
228	100		
229	22.0	16.2	24.4
226	26.8	22.2	33.2

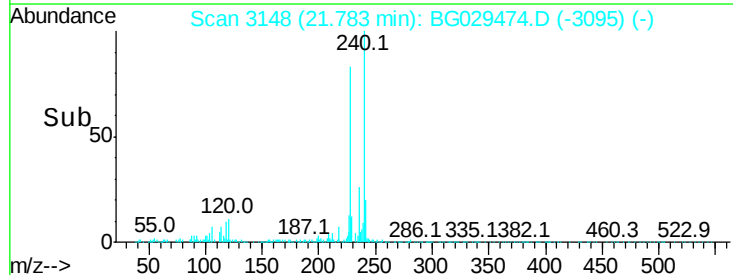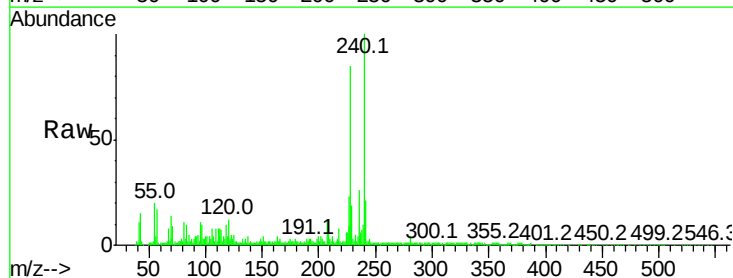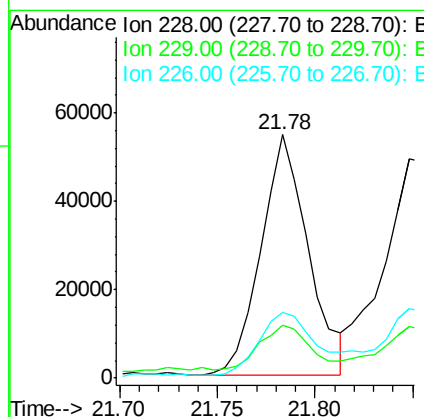

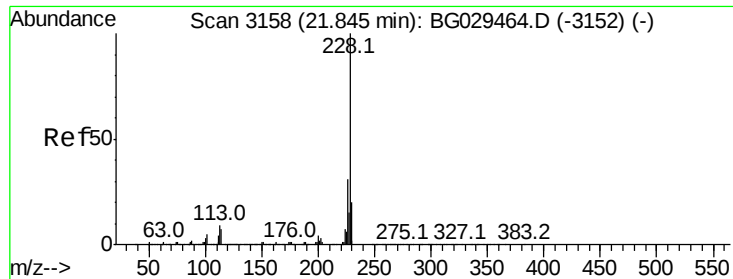

#82

Chrysene

Concen: 2.835 ng/ul m

RT: 21.85 min Scan# 3159

Delta R.T. 0.00 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Instrument :

BNA_G


ClientSampleId :

B0D35

Tot Ion:	228	Resp:	96130
Ion Ratio	Lower	Upper	
228	100		
226	31.7	24.2	36.2
229	23.5	15.2	22.8#

Manual Integrations
APPROVED




Sohil
10/27/2017 5:32:45 PM

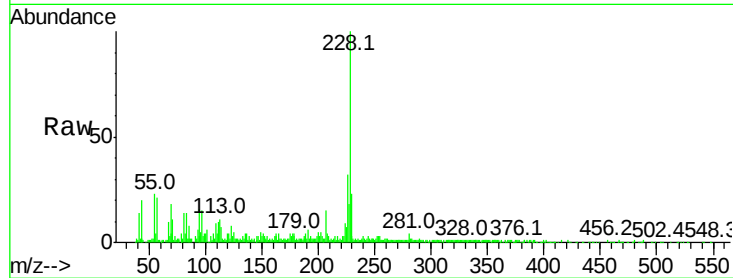

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

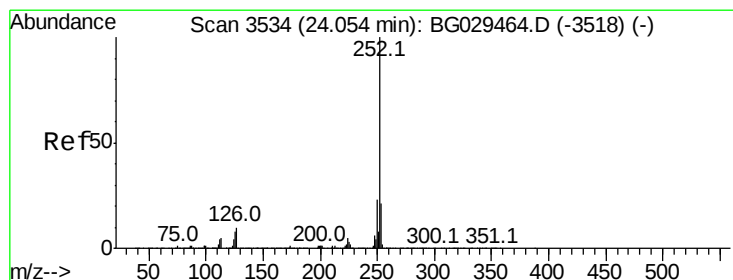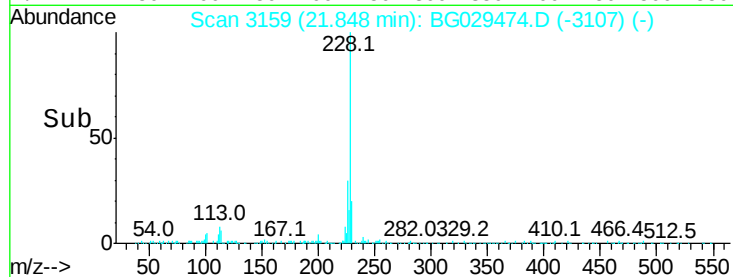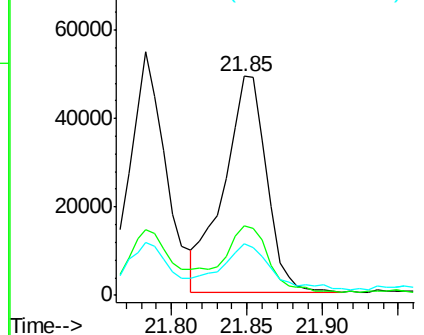

#85

Benzo(b)fluoranthene

Concen: 3.007 ng/ul

RT: 24.07 min Scan# 3537

Delta R.T. 0.02 min

Lab File: BG029474.D




Acq: 26 Oct 2017 12:18


Tgt Ion:	252	Resp:	106480
Ion Ratio	Lower	Upper	
252	100		
253	23.2	17.0	25.4
125	15.5	7.5	11.3#

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

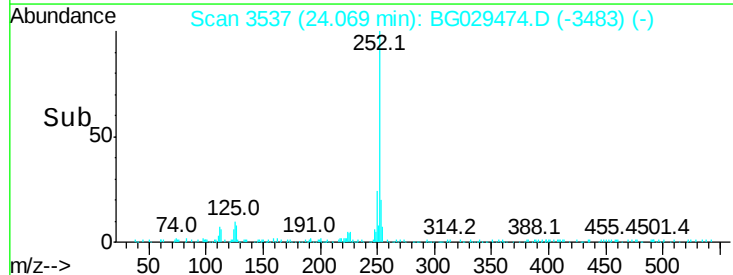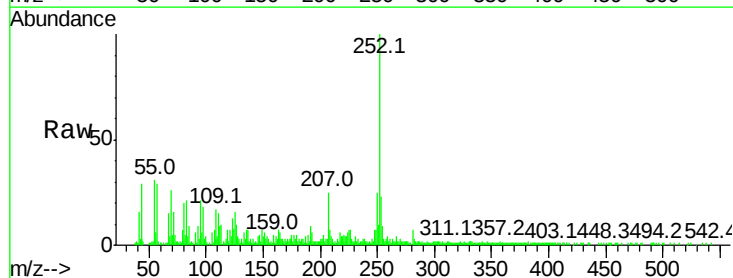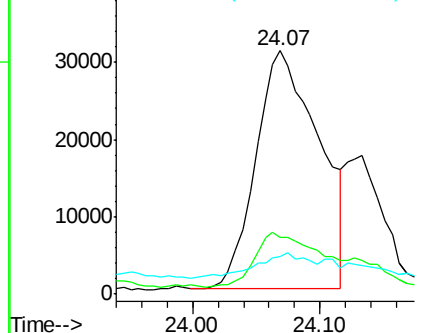

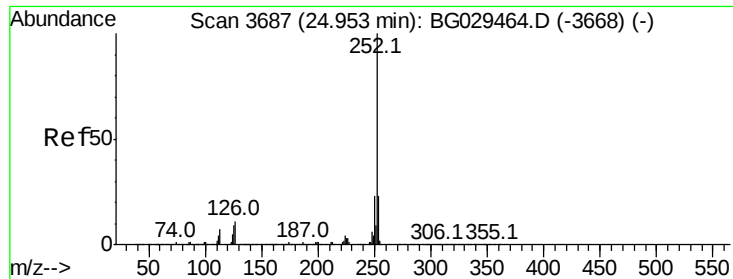





#88
Benzo(a)pyrene
Concen: 2.358 ng/ul
RT: 24.97 min Scan# 3691
Delta R.T. 0.02 min
Lab File: BG029474.D
Acq: 26 Oct 2017 12:18

Instrument :
BNA_G
ClientSampleId :
B0D35

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.8	17.1	25.7
125	13.3	7.8	11.8




Manual Integrations
APPROVED


Sohil
10/27/2017 5:32:45 PM

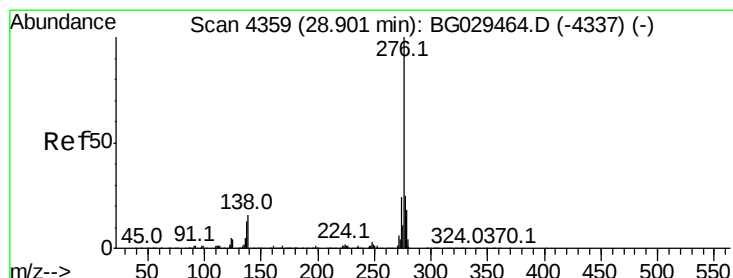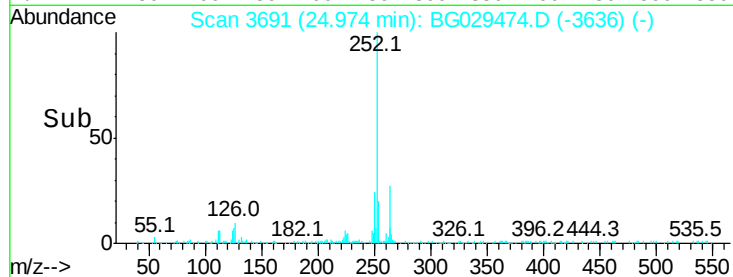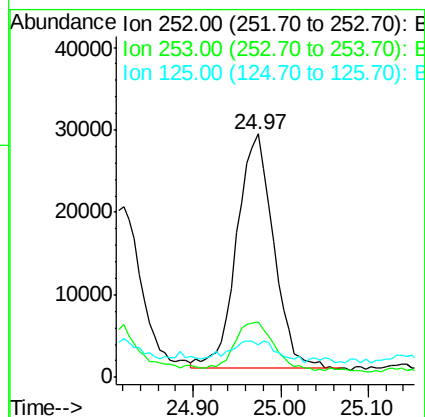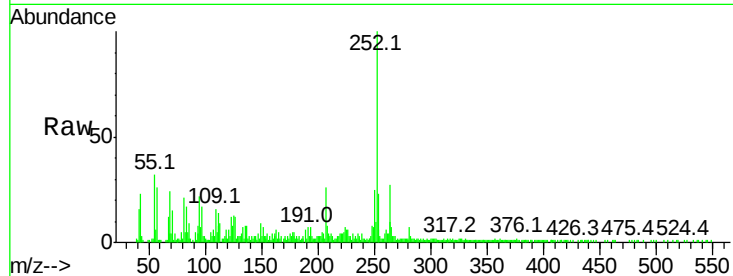

#89
Indeno(1,2,3-cd)pyrene
Concen: 1.125 ng/ul
RT: 28.92 min Scan# 4363
Delta R.T. 0.02 min
Lab File: BG029474.D
Acq: 26 Oct 2017 12:18

Tgt Ion	Ratio	Lower	Upper
276	100		
138	21.9	13.4	20.0
277	21.4	18.6	28.0

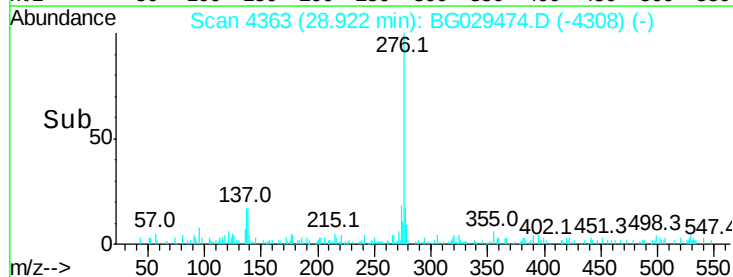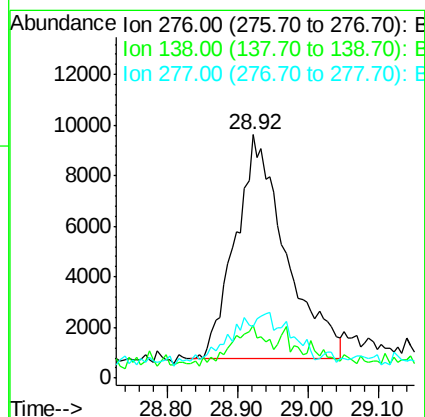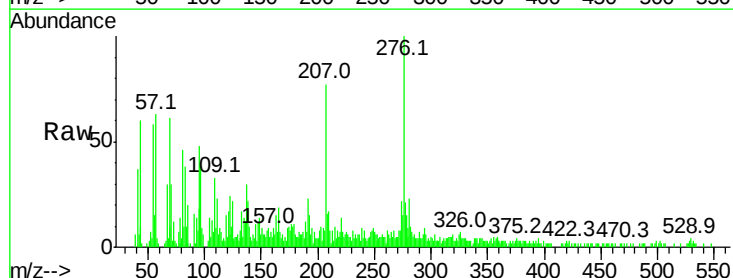

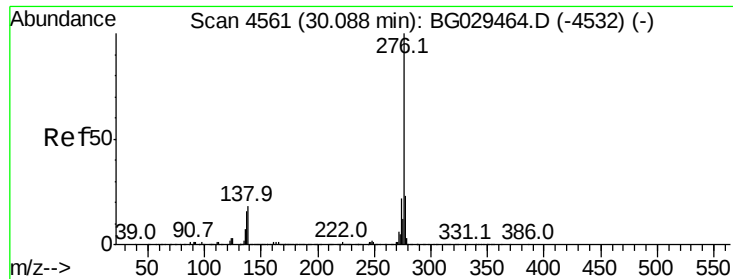

#91

Benzo(a,h,i)perylene

Concen: 1.272 ng/ul

RT: 30.13 min Scan# 4568

Delta R.T. 0.04 min

Lab File: BG029474.D

Acq: 26 Oct 2017 12:18

Instrument :

BNA_G

ClientSampleId :

B0D35

Tot Ion:	276	Resp:	41115
Ion Ratio	Lower	Upper	
276	100		
138	27.9	12.1	18.1#
277	25.3	17.7	26.5

Manual Integrations
APPROVED

Sohil
10/27/2017 5:32:45 PM

