
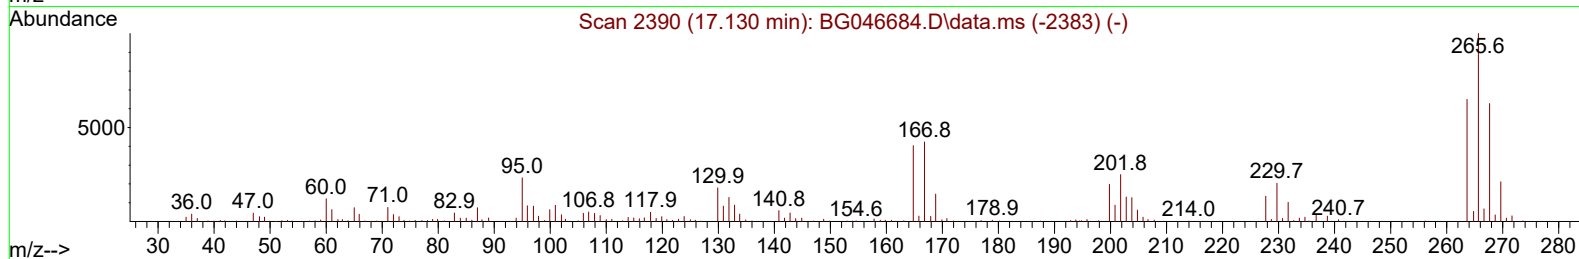
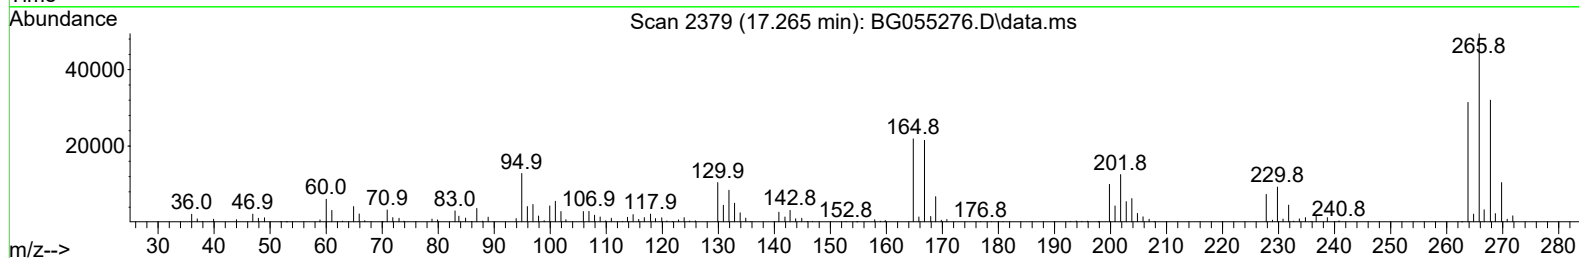


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
Data File : BG055276.D
Acq On : 25 Oct 2022 14:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 17:54:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

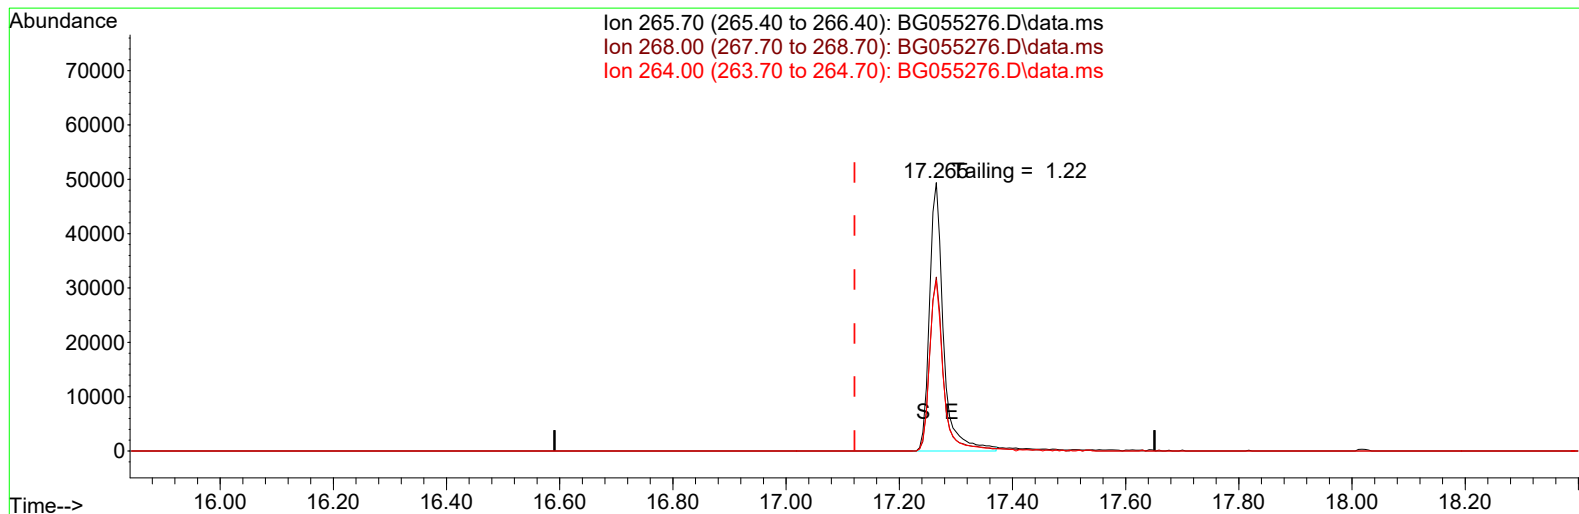

TIC: BG055276.D\data.ms

(70) Pentachlorophenol (C)




17.265min (+ 0.145) 0.00 ng

response 85378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.46
264.00	61.60	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
 Data File : BG055276.D
 Acq On : 25 Oct 2022 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 02 17:54:22 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 20 17:56:56 2021
 Response via : Initial Calibration

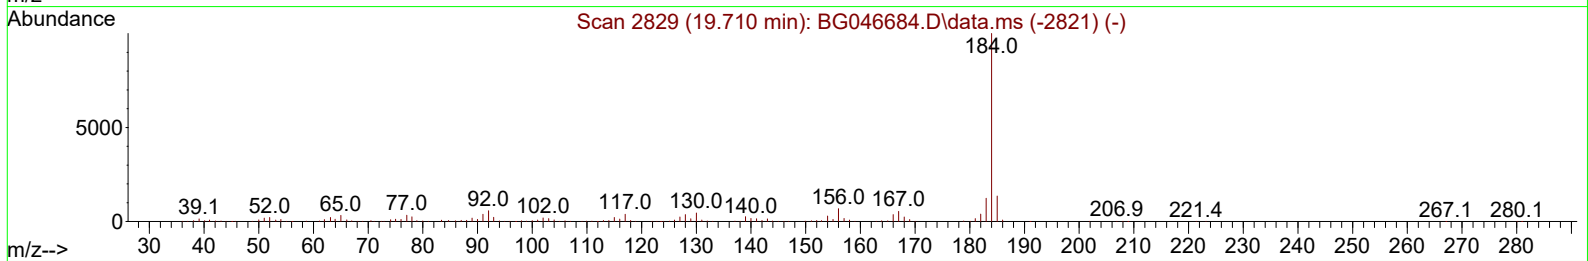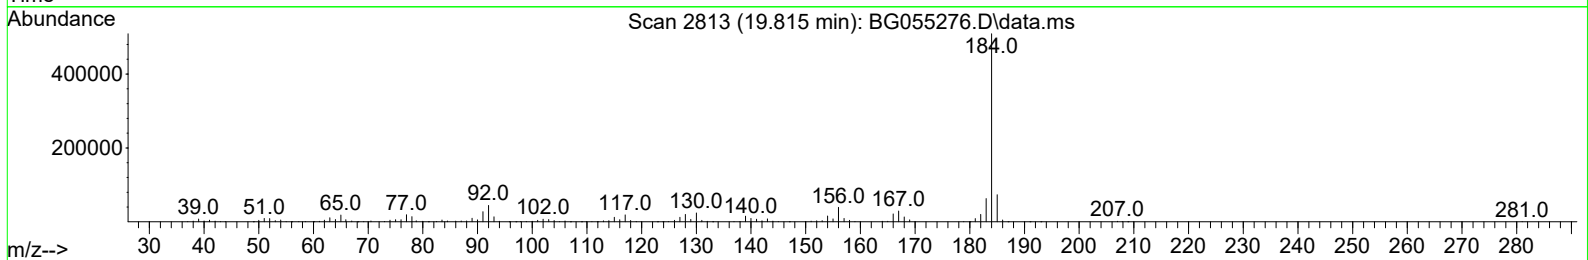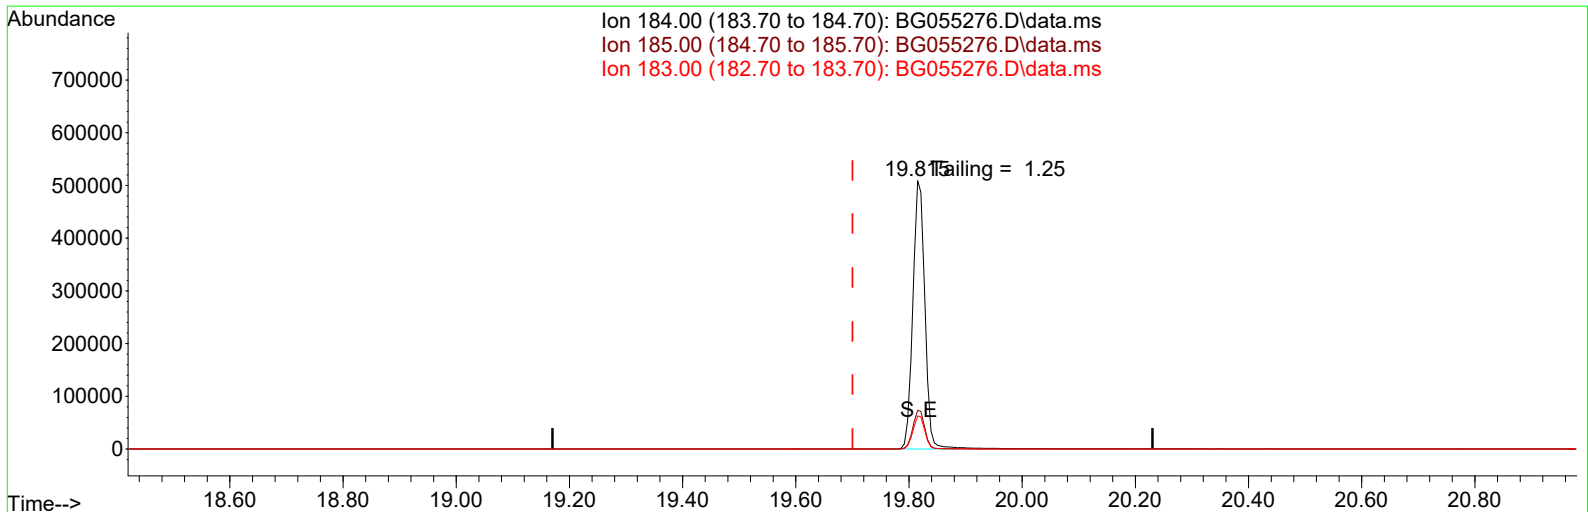

TIC: BG055276.D\data.ms

(77) Benzidine**19.815min (+ 0.115) 0.00 ng****response 754512**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.34
0.00	0.00	0.00