
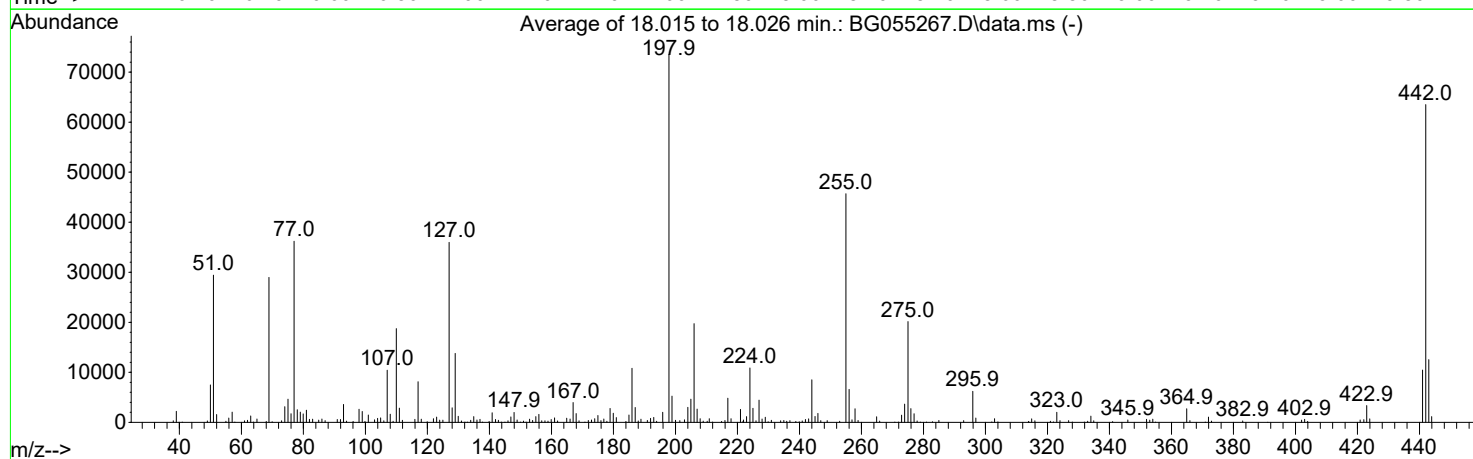


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
 Data File : BG055267.D
 Acq On : 25 Oct 2022 8:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 24 16:54:05 2022

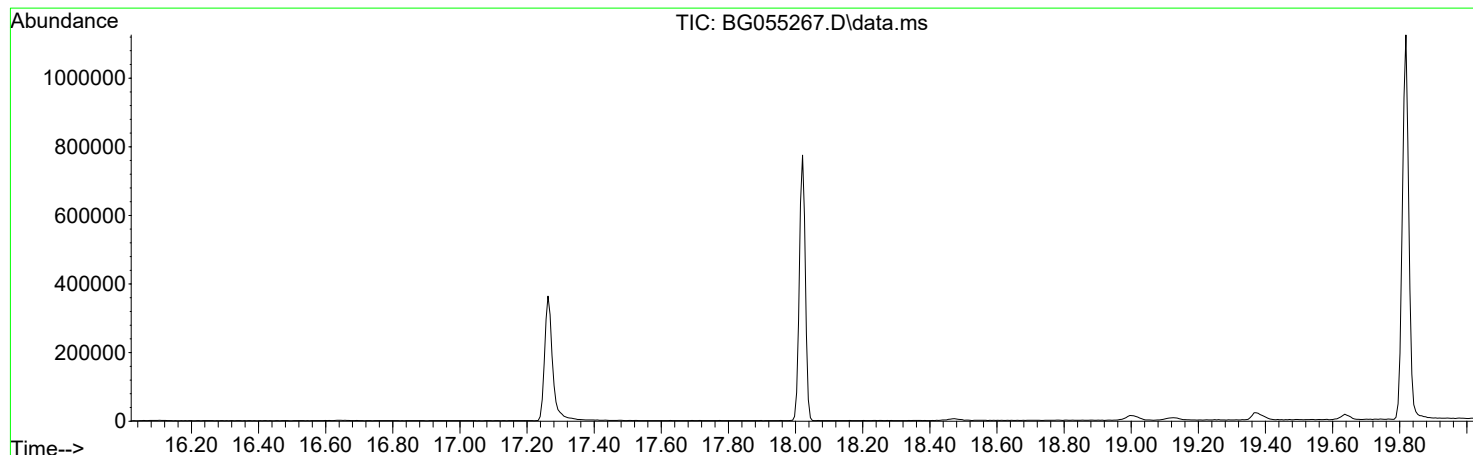




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	29437	PASS
68	69	0.00	2	0.6	186	PASS
69	198	0.00	100	39.4	28968	PASS
70	69	0.00	2	0.4	126	PASS
127	198	10	80	48.9	35976	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73520	PASS
199	198	5	9	7.2	5262	PASS
275	198	10	60	27.4	20160	PASS
365	198	1	100	3.7	2729	PASS
441	198	0.01	100	14.2	10446	PASS
442	442	50	100	100.0	63499	PASS
443	442	15	24	19.8	12547	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
Data File : BG055267.D
Acq On : 25 Oct 2022 8:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:44:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

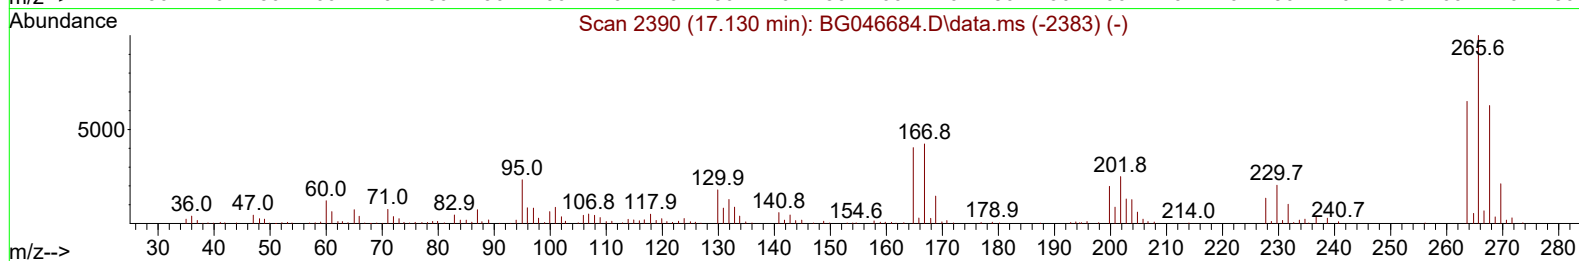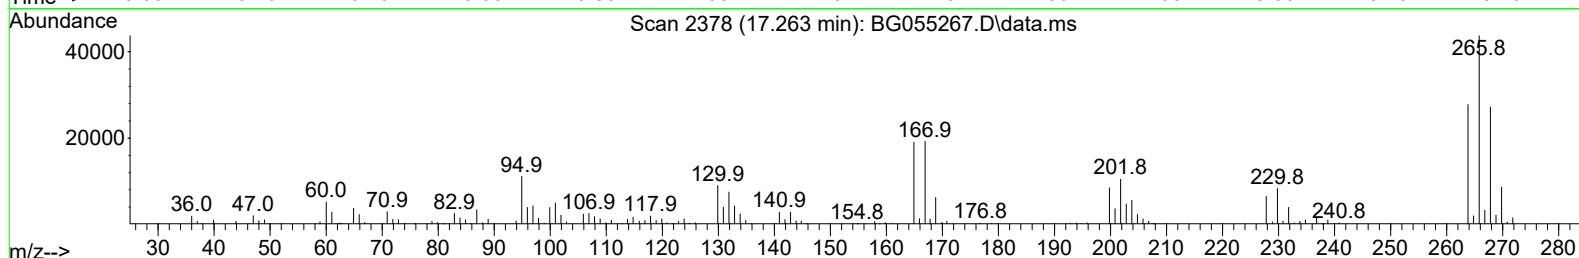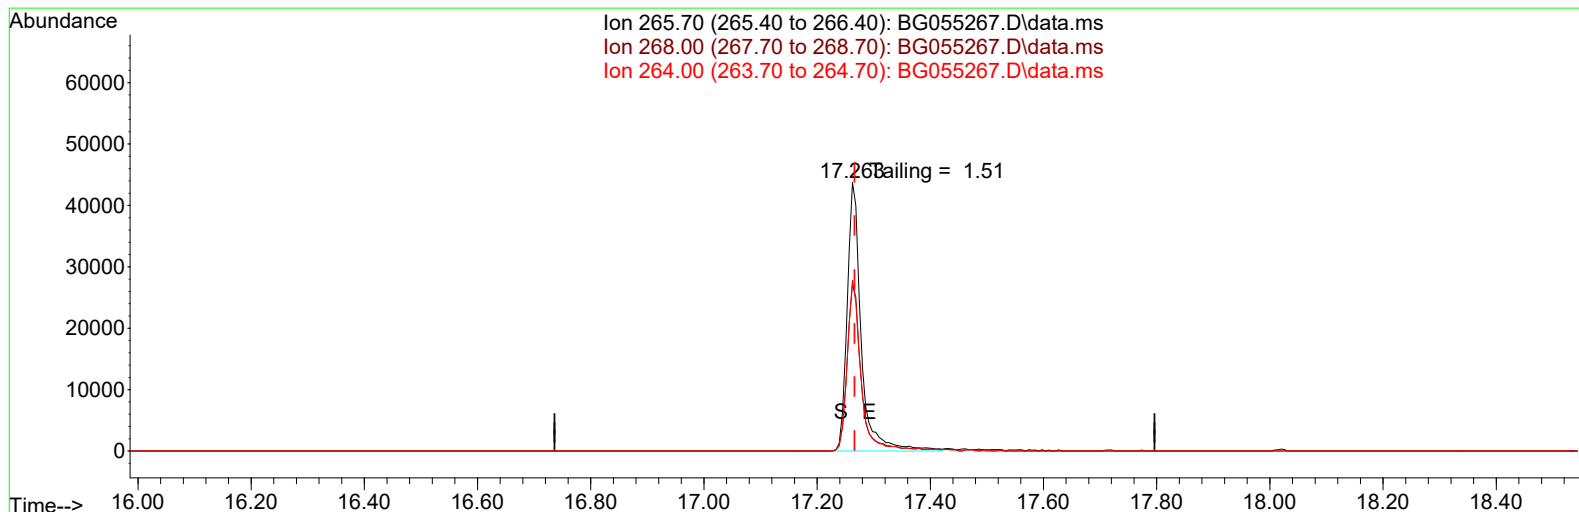

TIC: BG055267.D\data.ms

(70) Pentachlorophenol (C)

17.263min (-0.003) 31364.80 ng




response 75784

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	62.17
264.00	64.40	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
Data File : BG055267.D
Acq On : 25 Oct 2022 8:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 25 12:44:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 24 16:54:05 2022
Response via : Initial Calibration

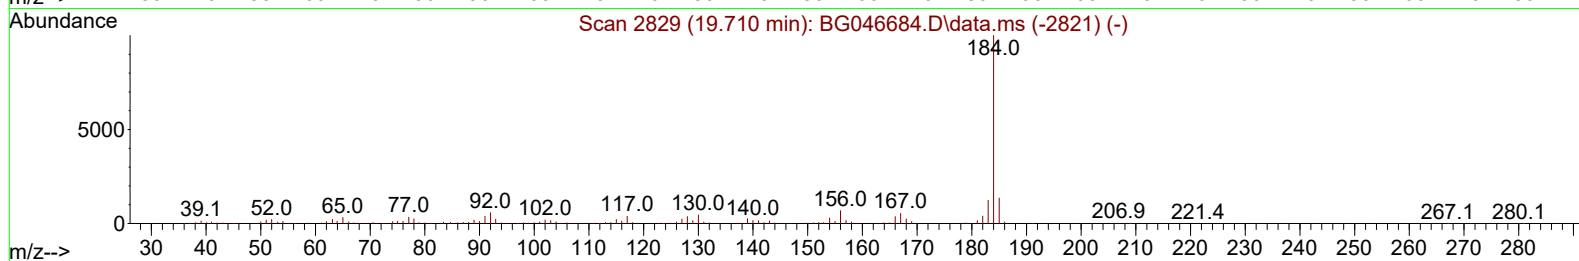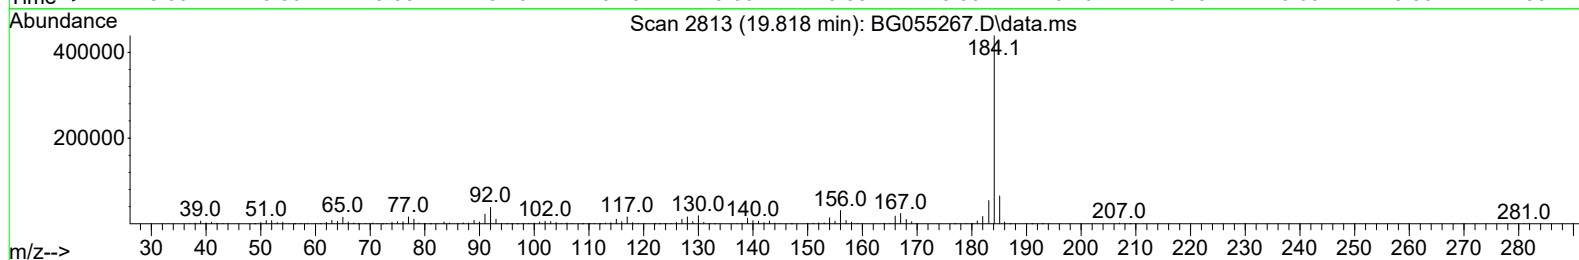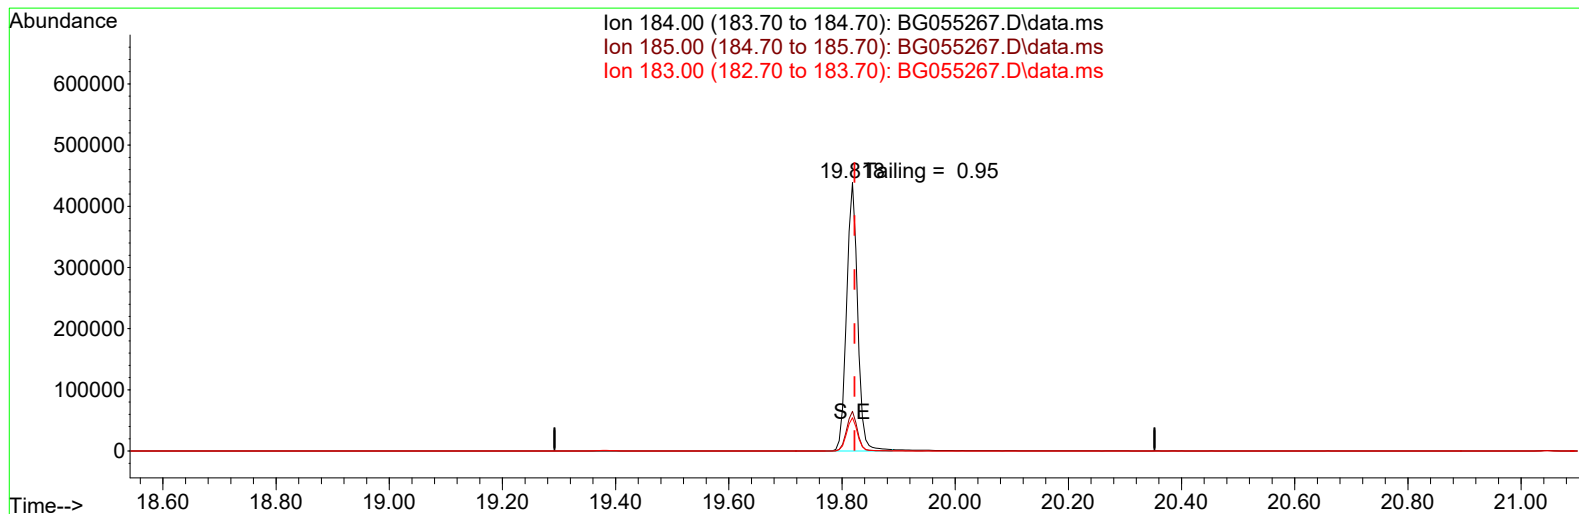

TIC: BG055267.D\data.ms

(77) Benzidine

19.818min (-0.004) 0.00 ng

response 600645

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.81
183.00	12.50	12.39
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_F	<u>BG055267.D</u>
Compound Name	Response	Retention Time
DDT	271272	21.046
DDD	1634	17.263
DDE	2456	18.021
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4090	275362	1.49

Instrument :
BNA_G
ClientSampleId :
DFTPP