
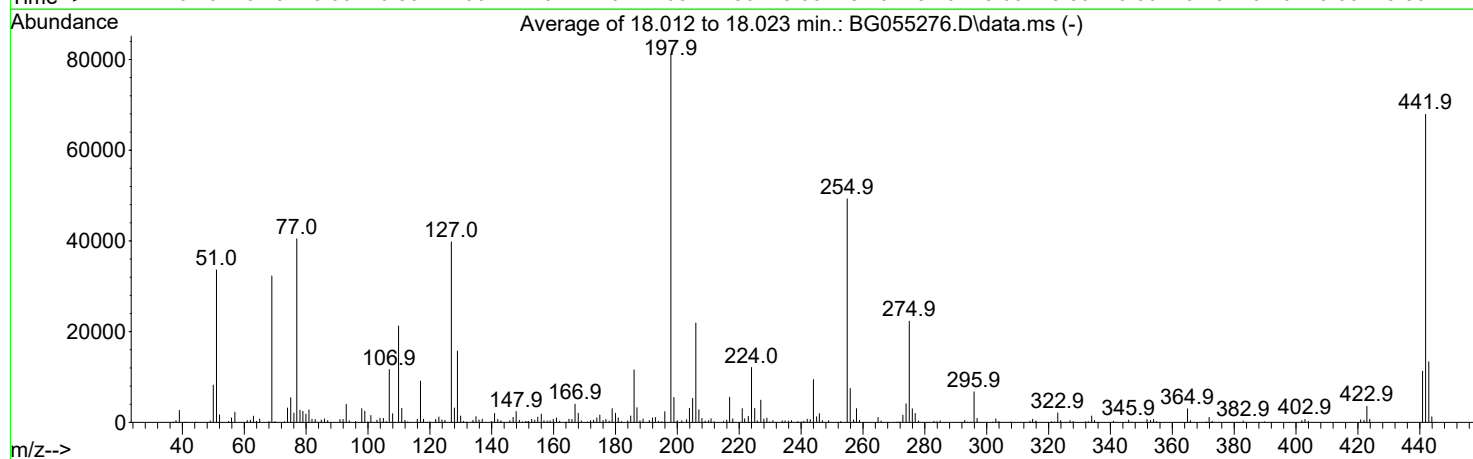


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
 Data File : BG055276.D
 Acq On : 25 Oct 2022 14:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 24 16:54:05 2022

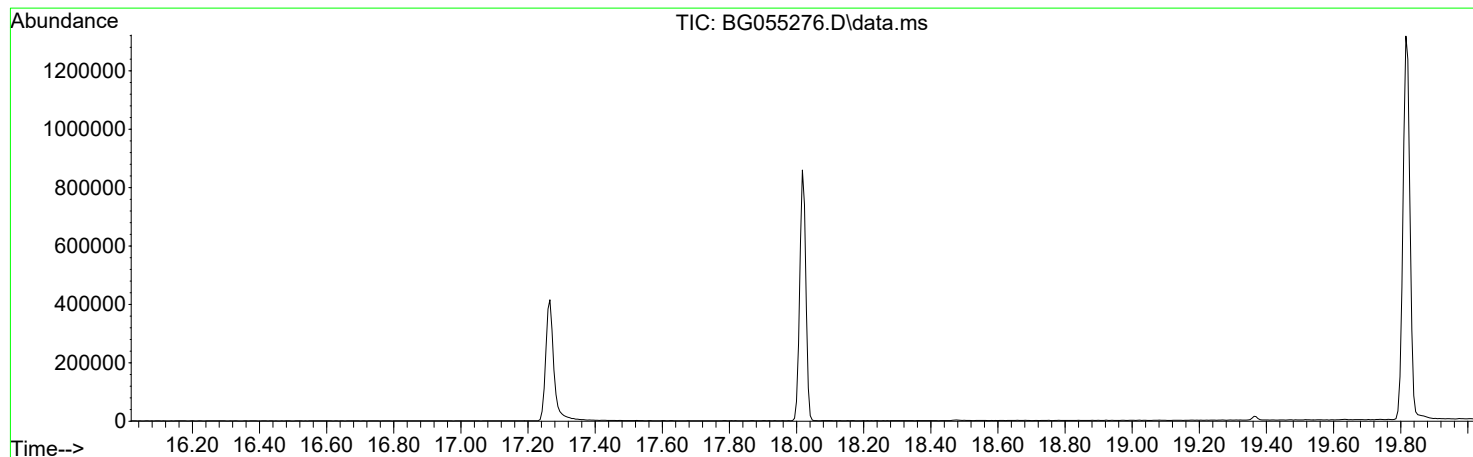




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	33621	PASS
68	69	0.00	2	0.6	204	PASS
69	198	0.00	100	39.8	32267	PASS
70	69	0.00	2	0.4	119	PASS
127	198	10	80	49.1	39797	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	81096	PASS
199	198	5	9	6.8	5515	PASS
275	198	10	60	27.5	22283	PASS
365	198	1	100	3.7	3001	PASS
441	198	0.01	100	13.9	11284	PASS
442	442	50	100	100.0	67901	PASS
443	442	15	24	19.7	13367	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
Data File : BG055276.D
Acq On : 25 Oct 2022 14:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 02 17:54:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

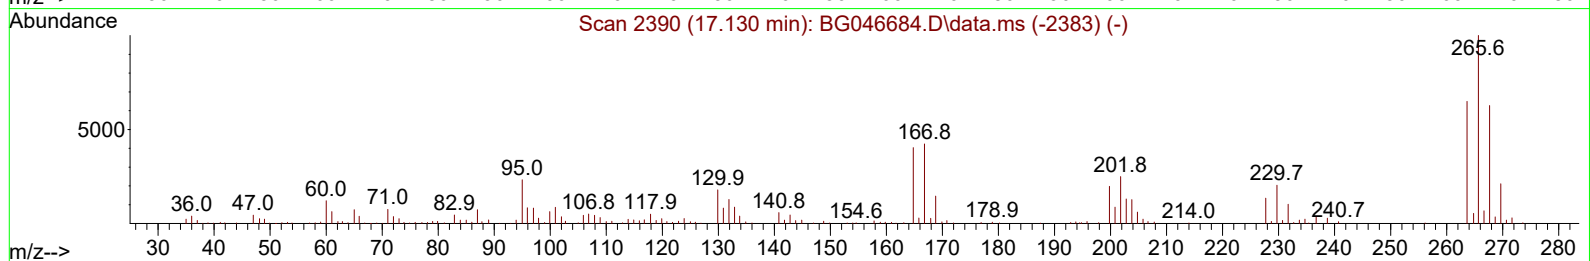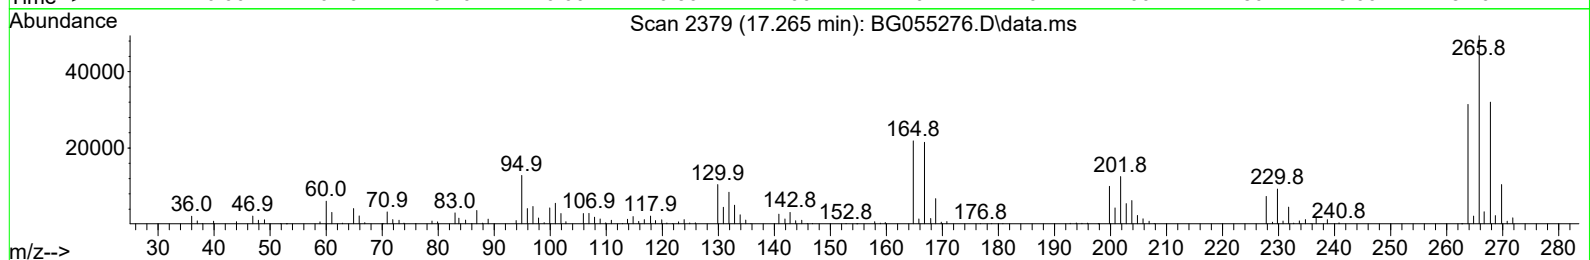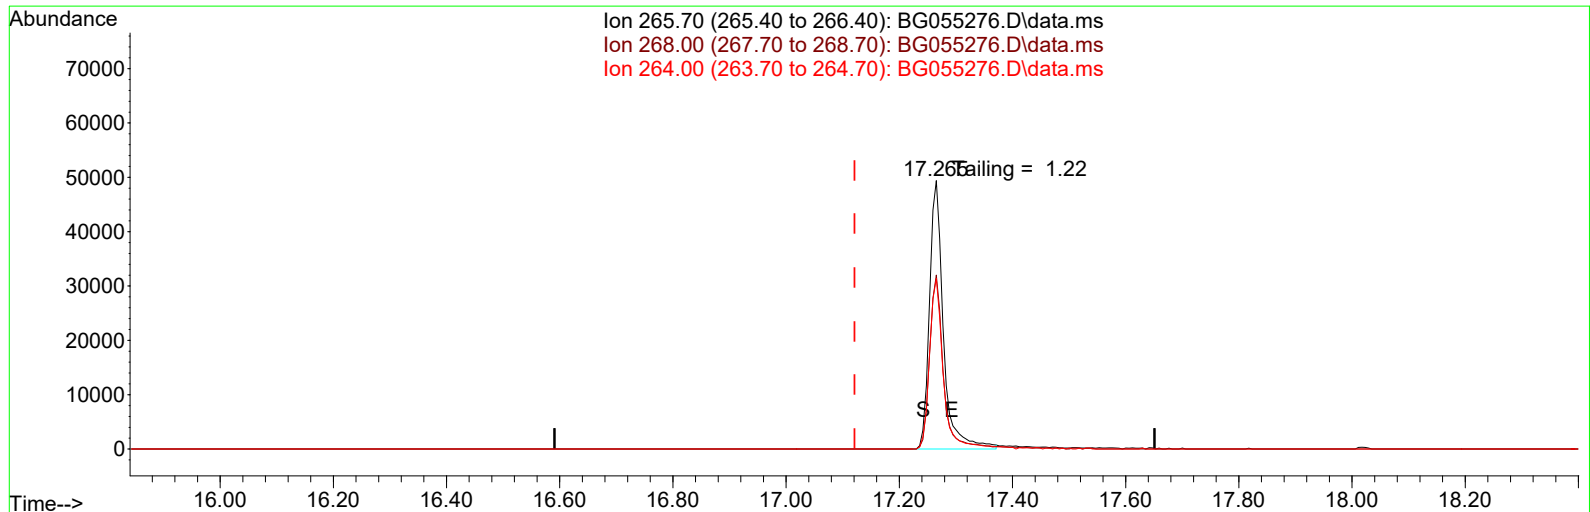

TIC: BG055276.D\data.ms

(70) Pentachlorophenol (C)

17.265min (+ 0.145) 0.00 ng




response 85378

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.46
264.00	61.60	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102522\
Data File : BG055276.D
Acq On : 25 Oct 2022 14:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Nov 02 17:54:22 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 20 17:56:56 2021
Response via : Initial Calibration

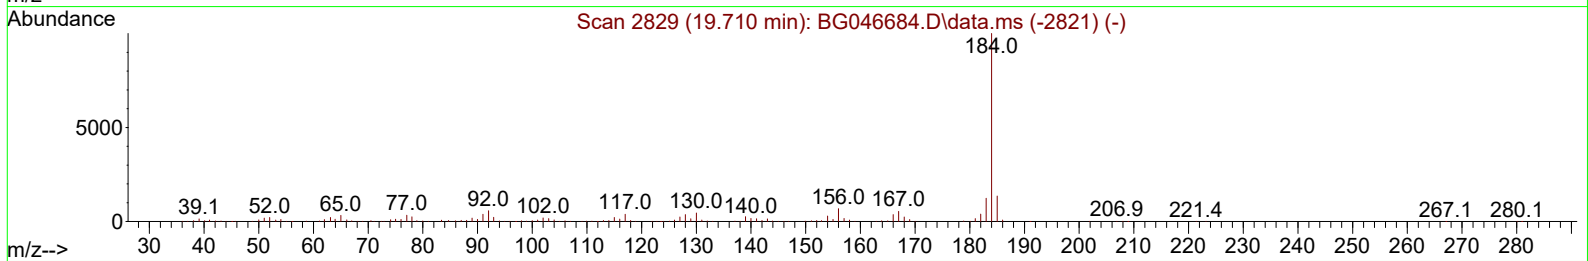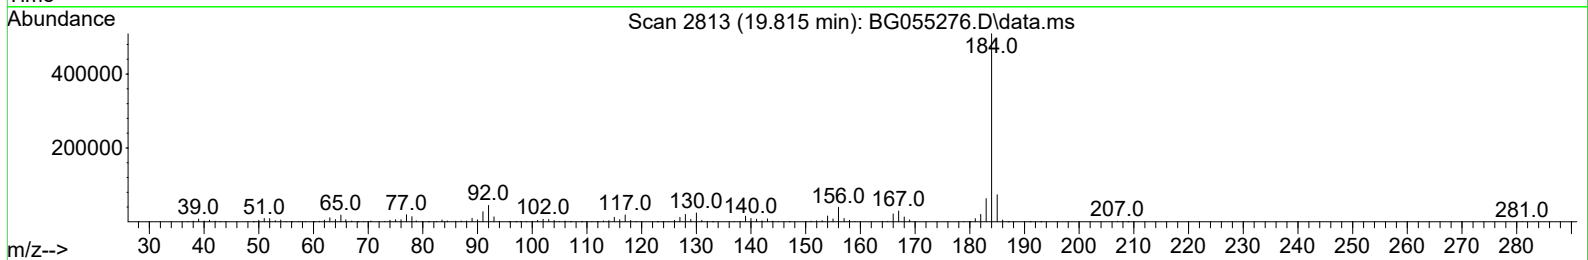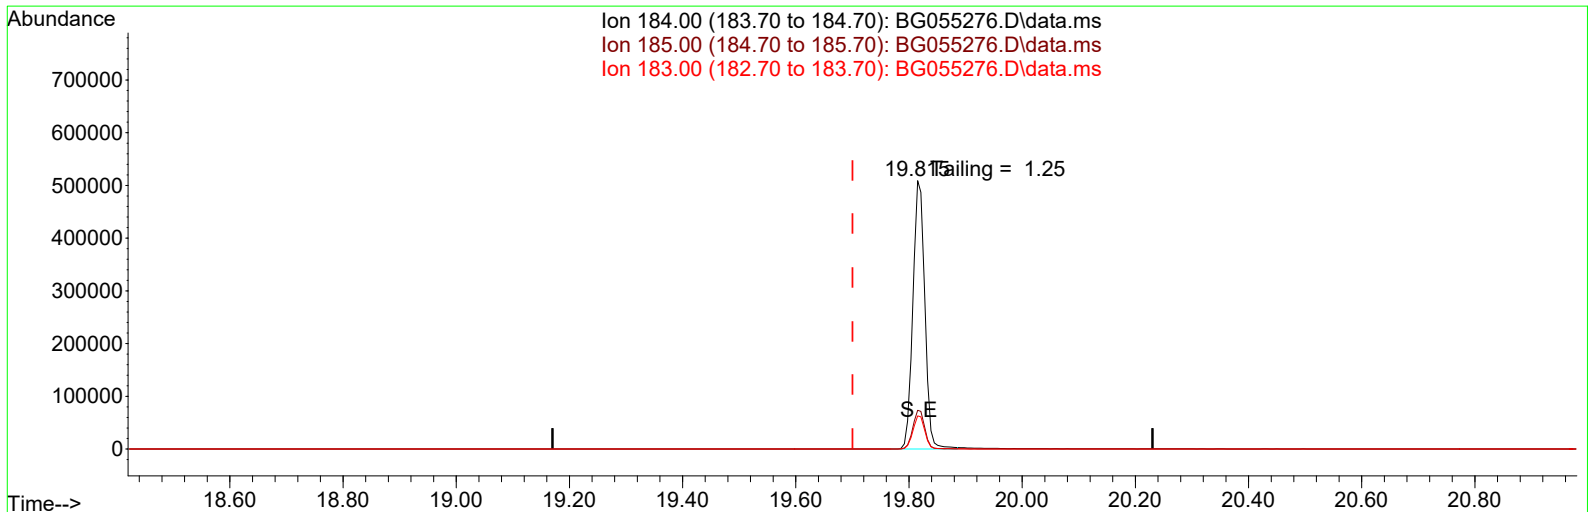

TIC: BG055276.D\data.ms

(77) Benzidine

19.815min (+ 0.115) 0.00 ng

response 754512

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.45
183.00	13.20	12.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_F	<u>BG055276.D</u>
Compound Name	Response	Retention Time
DDT	332975	21.043
DDD	1869	17.265
DDE	2740	18.017
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4609	337584	1.37

Instrument :
BNA_G
ClientSampleId :
DFTPP