

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102615\
 Data File : BG019357.D
 Acq On : 26 Oct 2015 13:25
 Operator : UM/NP
 Sample : G4074-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9H0

Quant Time: Oct 27 03:09:04 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 27 04:07:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	28433	20.00	ng/ul	0.00
18) Naphthalene-d8	11.06	136	118869	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	100589	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	254594	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	305323	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	283141	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.56	96	1673	3.27	ng/uL	0.00
5) Phenol-d5	7.37	99	50124	20.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	30820	20.63	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	33501	20.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	42145	21.61	ng/ul	0.00
19) Nitrobenzene-d5	9.41	128	17119	18.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	21253	20.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.67	165	44708	19.88	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	22719	10.17	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	166203	19.93	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	180392	19.54	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	23328	17.20	ng/ul	0.00
58) Fluorene-d10	15.85	176	151585	19.37	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	32859	19.61	ng/ul	0.00
71) Anthracene-d10	17.70	188	238382	20.45	ng/ul	0.00
79) Pyrene-d10	19.97	212	262534	19.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.04	264	266761	18.47	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.30	163	74293	8.92 ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102615\
Data File : BG019357.D
Acq On : 26 Oct 2015 13:25
Operator : UM/NP
Sample : G4074-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9H0

Quant Time: Oct 27 03:09:04 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 27 04:07:50 2015
Response via : Initial Calibration

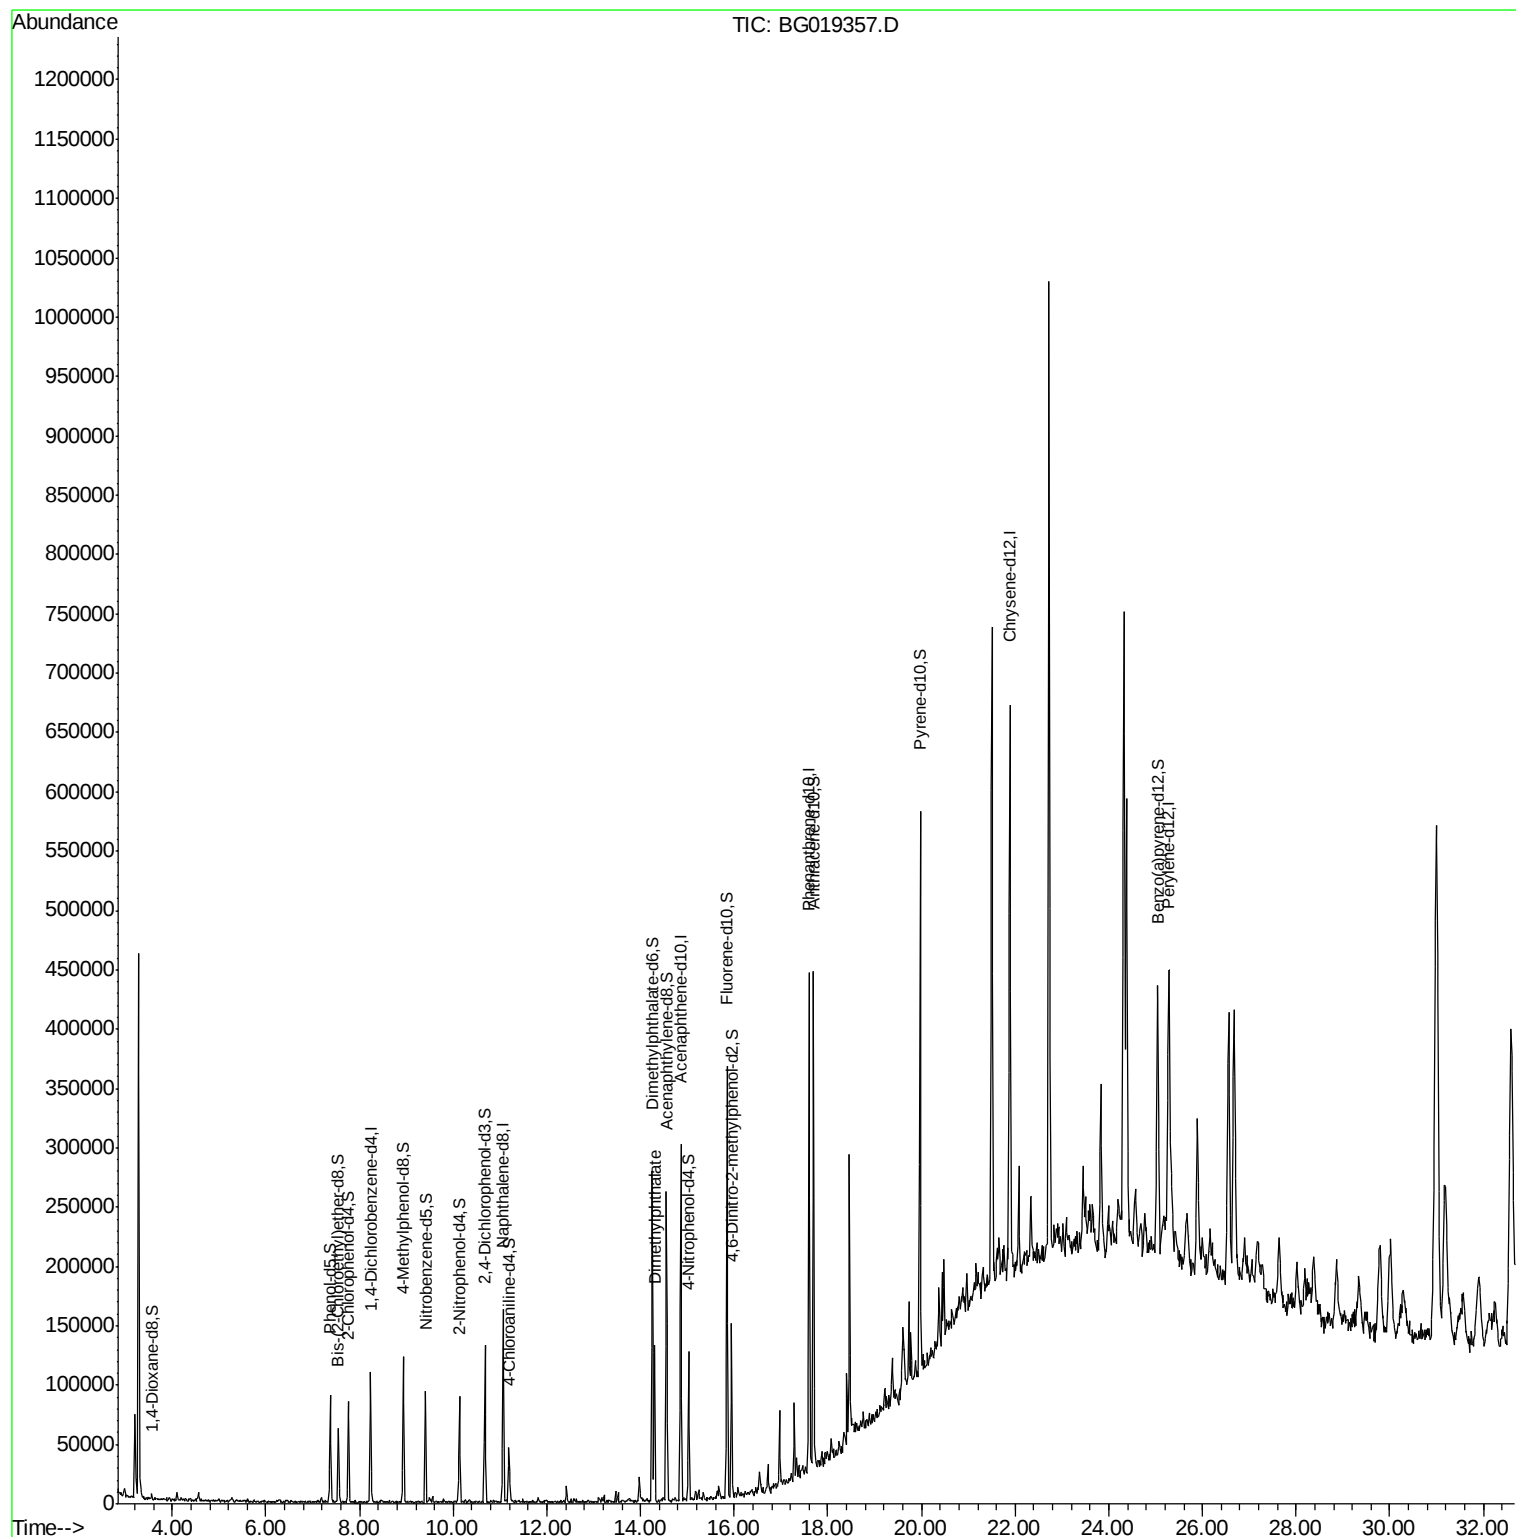

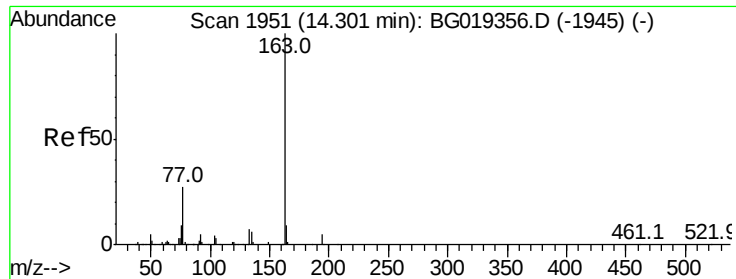

#45

Dimethylphthalate

Concen: 8.92 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. -0.00 min

Lab File: BG019357.D

Acq: 26 Oct 2015 13:25

Instrument :

BNA_G

ClientSampleId :

JG9H0


Tot Ion:163 Resp: 74293

Ion Ratio Lower Upper

163 100

194 4.5 4.3 6.5

164 9.4 7.5 11.3

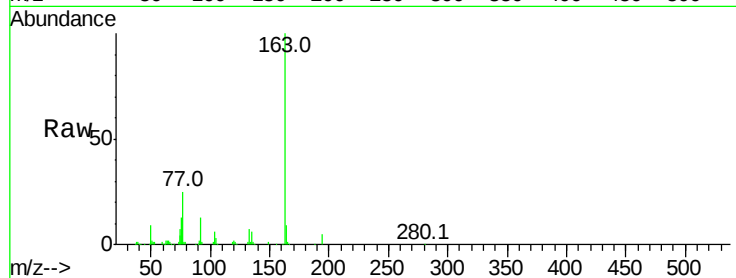

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

