

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102615\
 Data File : BG019358.D
 Acq On : 26 Oct 2015 14:03
 Operator : UM/NP
 Sample : G4074-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JG9L0

Quant Time: Oct 27 03:09:13 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 27 04:07:50 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	42268	20.00	ng/ul	0.00
18) Naphthalene-d8	11.06	136	191383	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.86	164	165469	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.60	188	440630	20.00	ng/ul	0.00
78) Chrysene-d12	21.89	240	534415	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	517179	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.55	96	2299	3.02	ng/uL	0.00
5) Phenol-d5	7.37	99	81013	21.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.55	67	46543	20.96	ng/ul	0.00
9) 2-Chlorophenol-d4	7.76	132	54216	22.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.93	113	63464	21.89	ng/ul	0.00
19) Nitrobenzene-d5	9.40	128	26897	18.51	ng/ul	0.00
22) 2-Nitrophenol-d4	10.13	143	32417	19.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.68	165	73759	20.37	ng/ul	0.00
29) 4-Chloroaniline-d4	11.19	131	63767	17.73	ng/ul	0.00
44) Dimethylphthalate-d6	14.25	166	257531	18.77	ng/ul	0.00
47) Acenaphthylene-d8	14.55	160	300510	19.79	ng/ul	0.00
52) 4-Nitrophenol-d4	15.03	143	43308	19.41	ng/ul	0.00
58) Fluorene-d10	15.85	176	250697	19.48	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.95	200	54568	18.81	ng/ul	0.00
71) Anthracene-d10	17.70	188	416939	20.66	ng/ul	0.00
79) Pyrene-d10	19.96	212	489918	20.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	543434	20.60	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.30	163	45213	3.30 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG102615\
Data File : BG019358.D
Acq On : 26 Oct 2015 14:03
Operator : UM/NP
Sample : G4074-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JG9L0

Quant Time: Oct 27 03:09:13 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG102315.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 27 04:07:50 2015
Response via : Initial Calibration

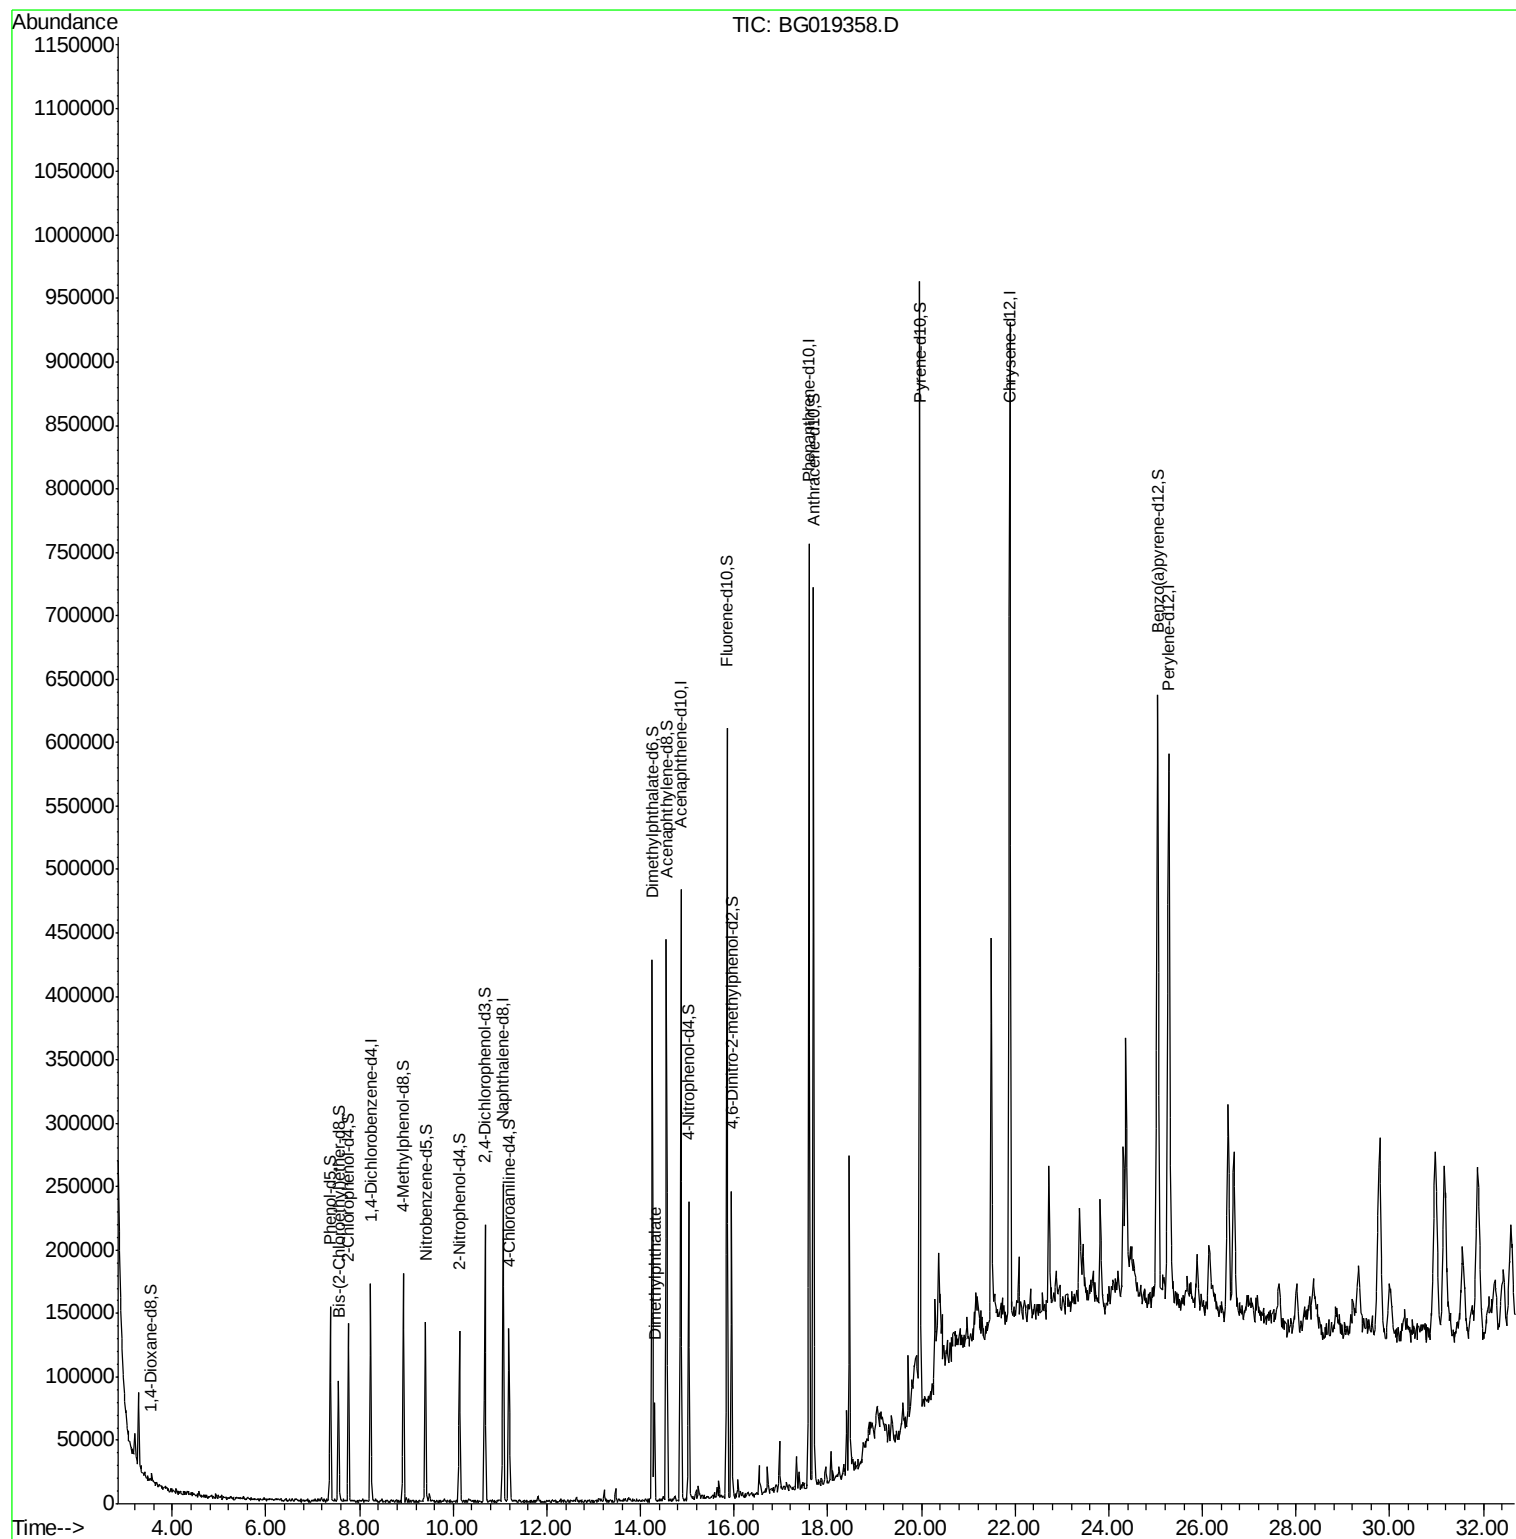

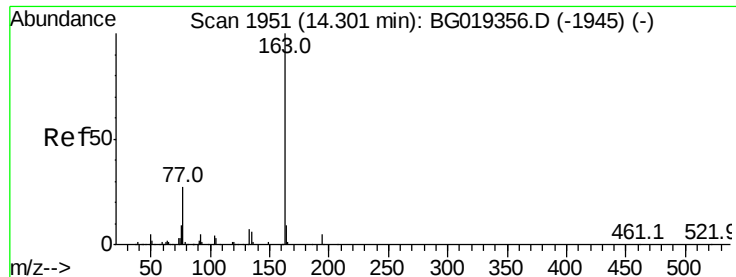

#45

Dimethylphthalate

Concen: 3.30 ng/ul

RT: 14.30 min Scan# 1951

Delta R.T. -0.00 min

Lab File: BG019358.D

Acq: 26 Oct 2015 14:03

Instrument :

BNA_G

ClientSampleId :

JG9L0


Tot Ion:163 Resp: 45213

Ion Ratio Lower Upper

163 100

194 3.9 4.3 6.5#

164 9.1 7.5 11.3

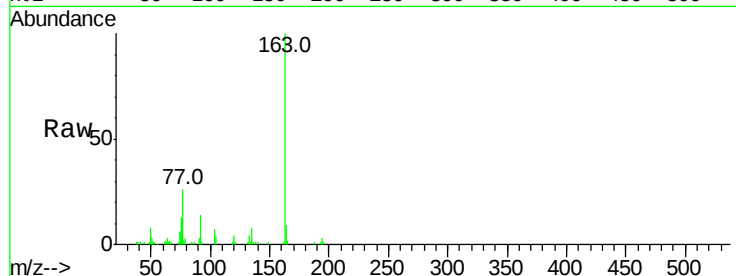

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

