
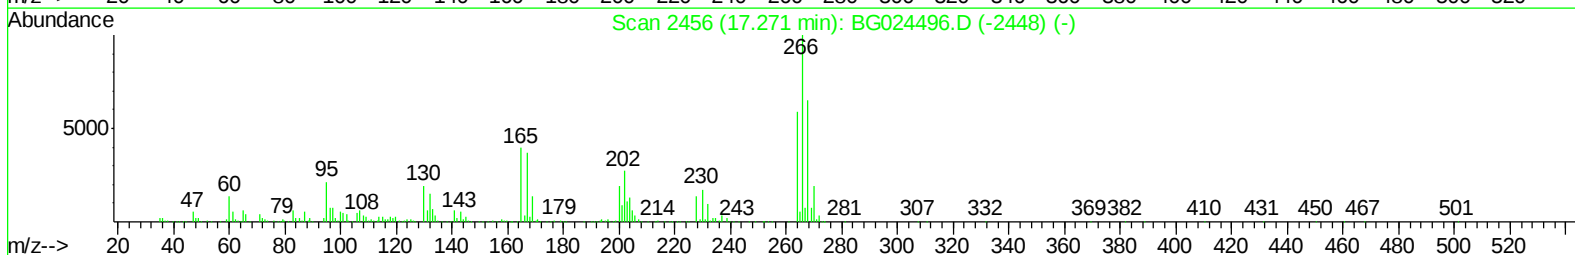
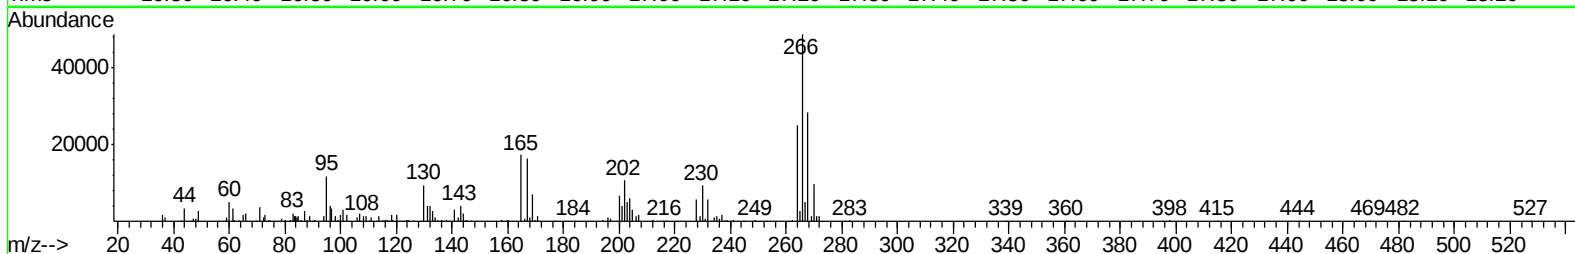


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102616\
Data File : BG024511.D
Acq On : 26 Oct 2016 12:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 18:38:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

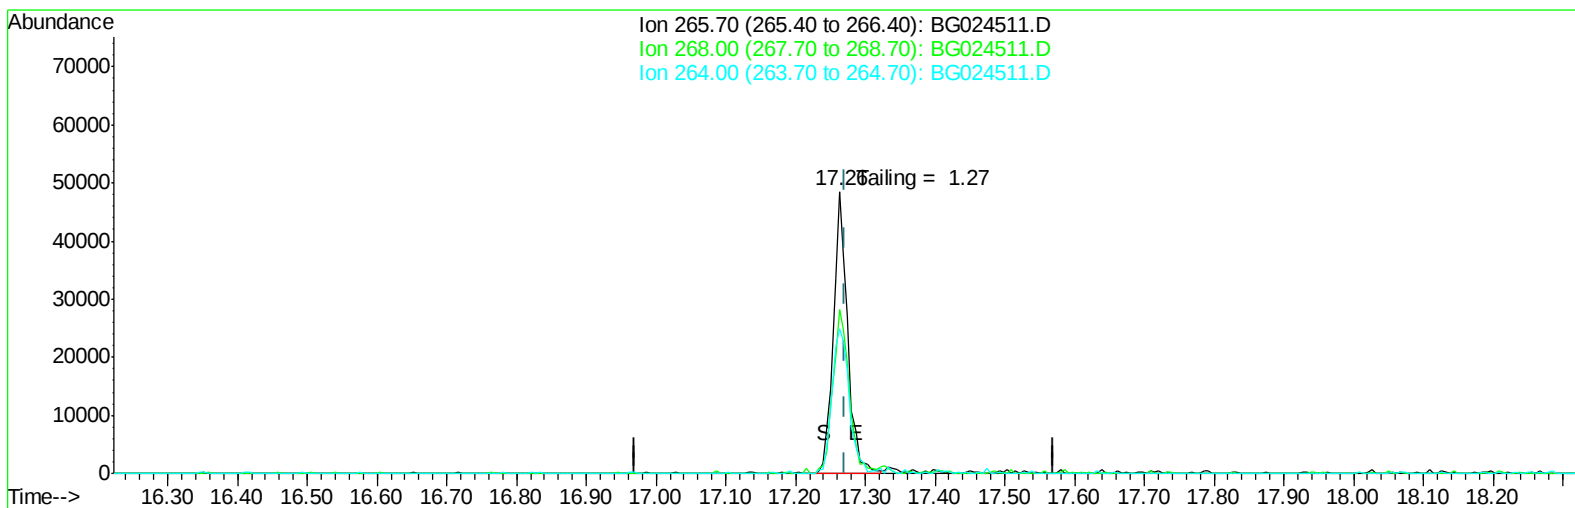

TIC: BG024511.D

(69) Pentachlorophenol (C)




17.263min (-0.008) 144065.00ng

response 68859

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	58.29
264.00	62.60	51.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG102616\
Data File : BG024511.D
Acq On : 26 Oct 2016 12:54
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 18:38:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 26 11:14:13 2016
Response via : Initial Calibration

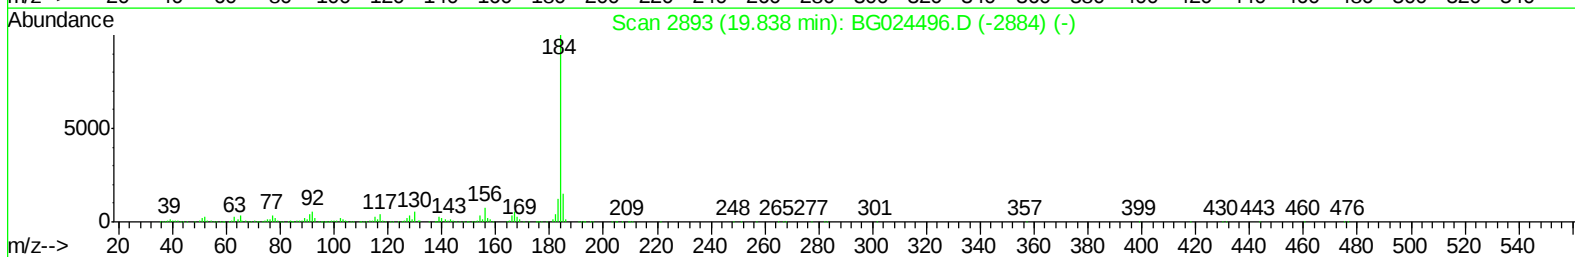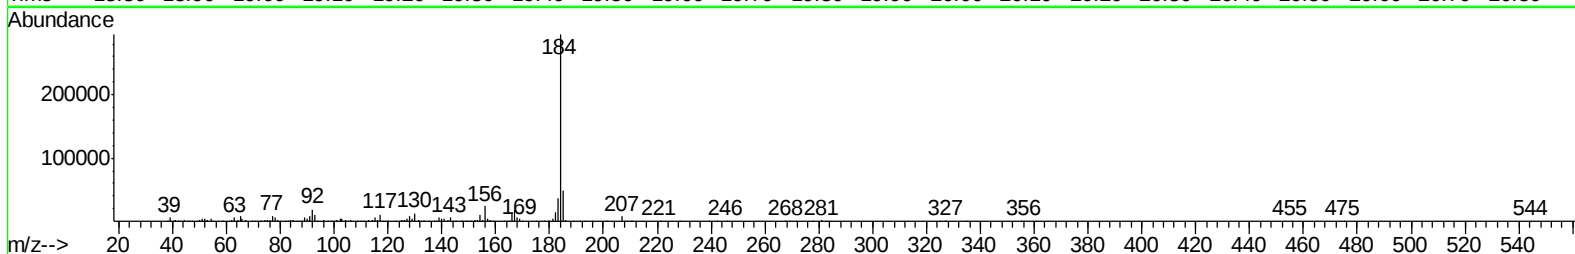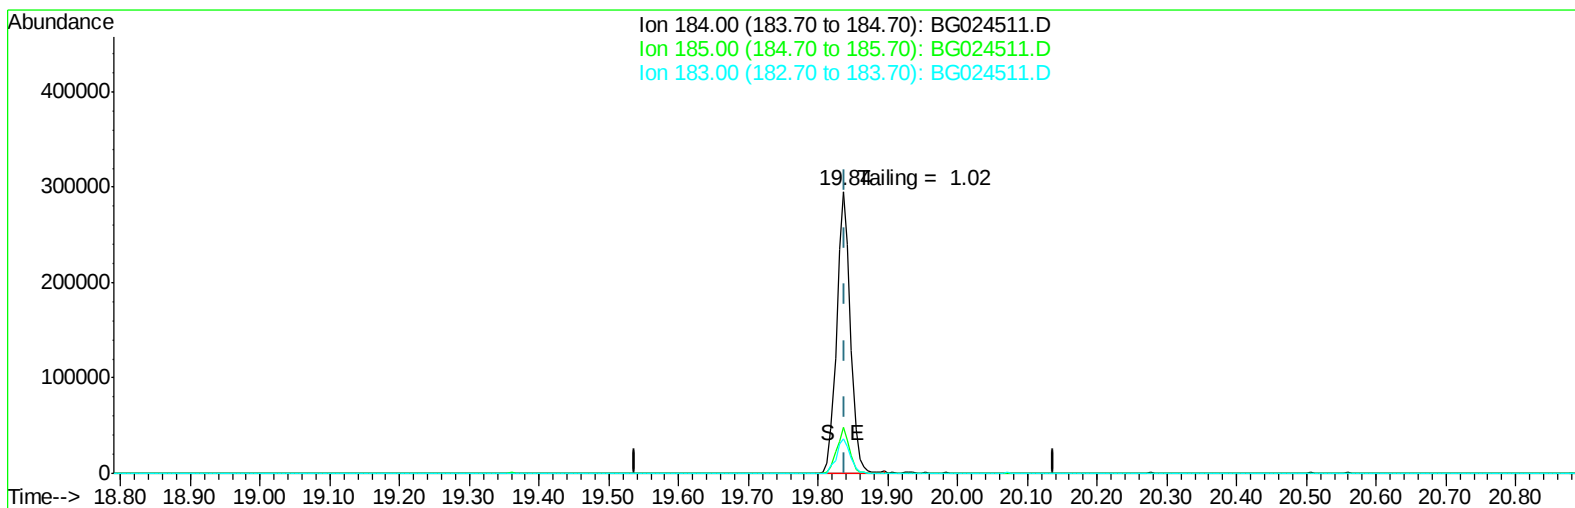

TIC: BG024511.D

(76) Benzidine

19.836min (-0.002) 173899.39ng

response 405630

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	16.18
183.00	13.80	12.40
0.00	0.00	0.00