


Data Path : Z:\HPCHEM1\BNA G\DATA\BG102616\
 Data File : BG024511.D
 Acq On : 26 Oct 2016 12:54
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG102516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 11:14:13 2016

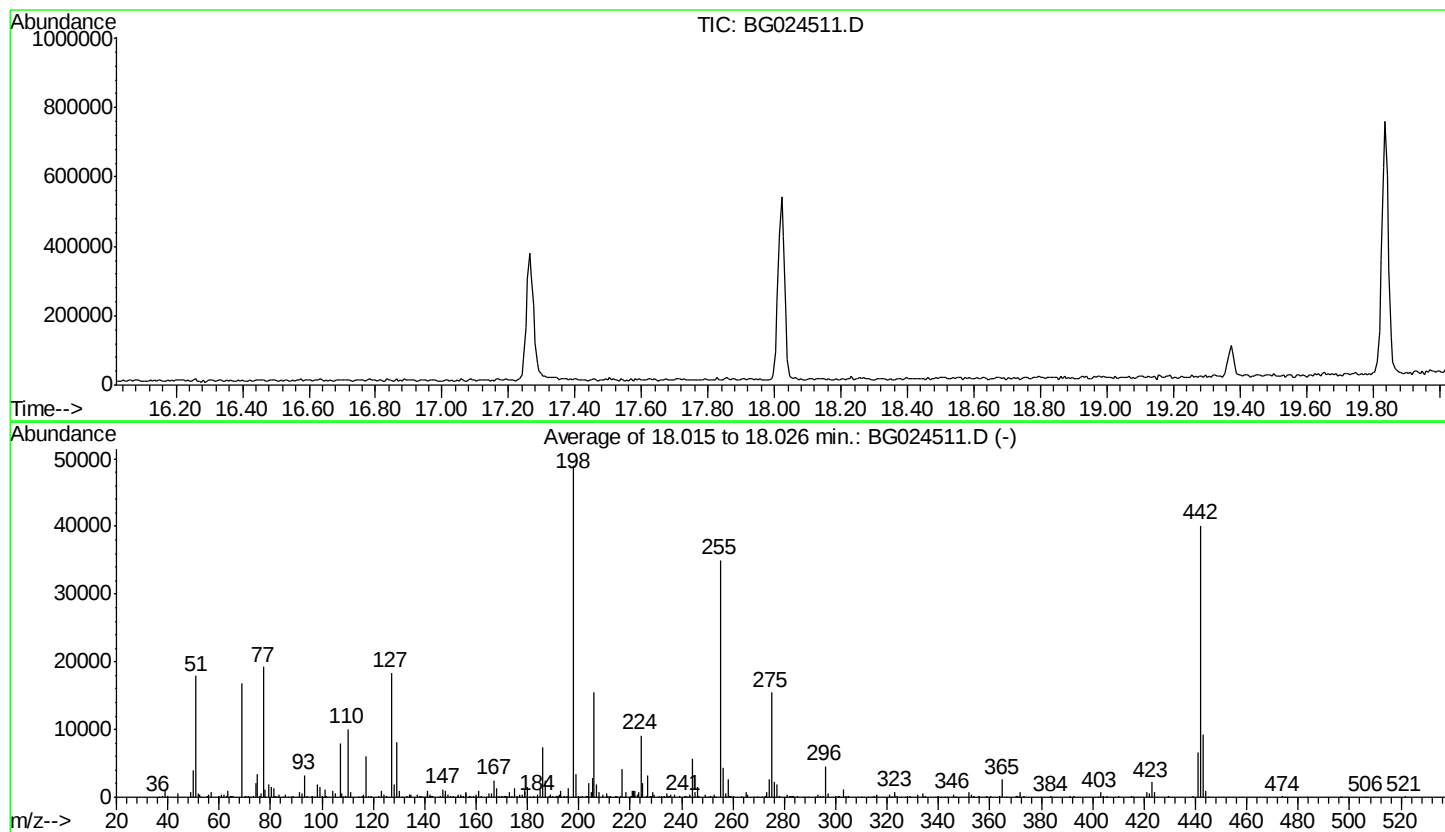

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2575

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	17938	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.5	16896	PASS
70	69	0.00	2	0.7	114	PASS
127	198	10	80	37.6	18426	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48984	PASS
199	198	5	9	7.1	3487	PASS
275	198	10	60	31.6	15501	PASS
365	198	1	100	5.2	2563	PASS
441	442	0.01	24	16.7	6701	PASS
442	198	50	100	82.0	40154	PASS
443	442	15	24	23.3	9361	PASS