
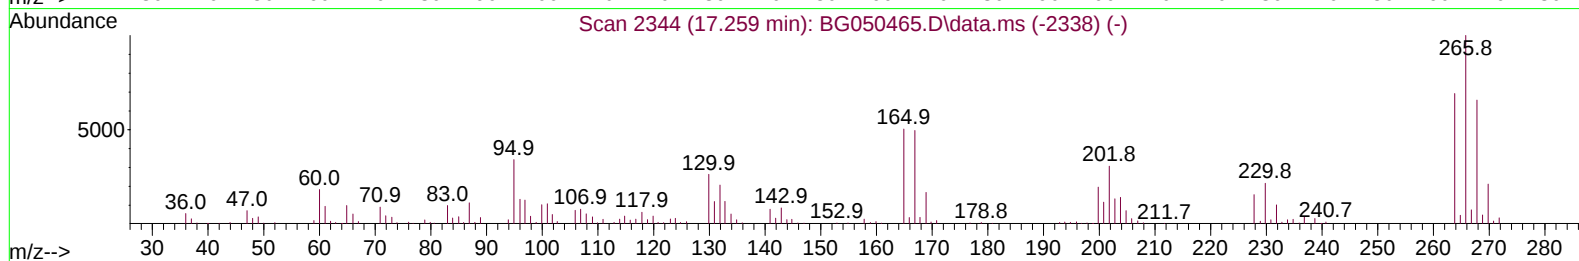
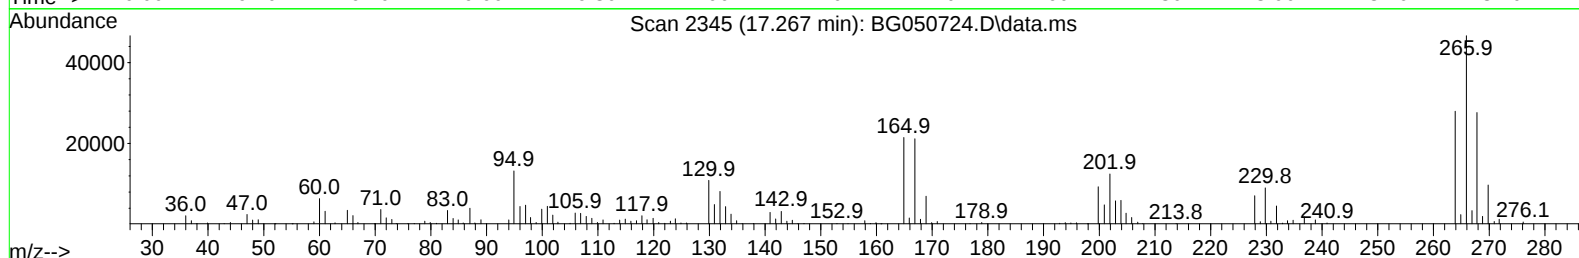


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102621\
Data File : BG050724.D
Acq On : 26 Oct 2021 8:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 09:30:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

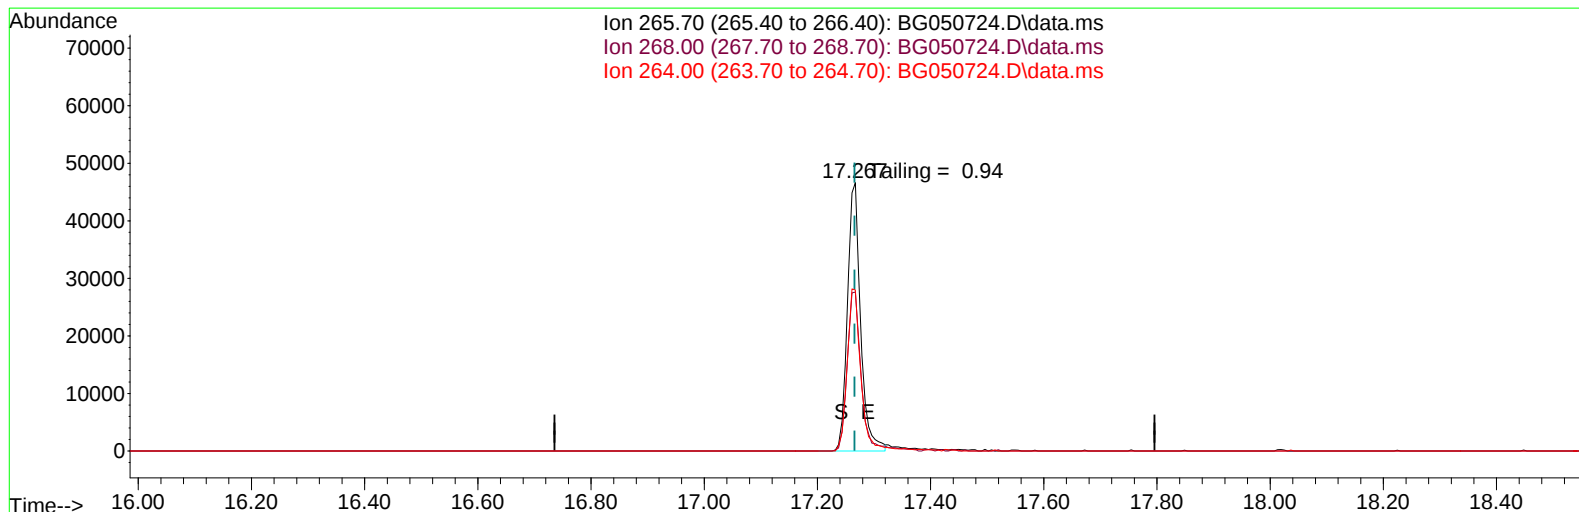

TIC: BG050724.D\data.ms

(70) Pentachlorophenol (C)


17.267min (+ 0.002) 18614.40 ng

response 77415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.25
264.00	61.30	60.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102621\
Data File : BG050724.D
Acq On : 26 Oct 2021 8:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 26 09:30:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

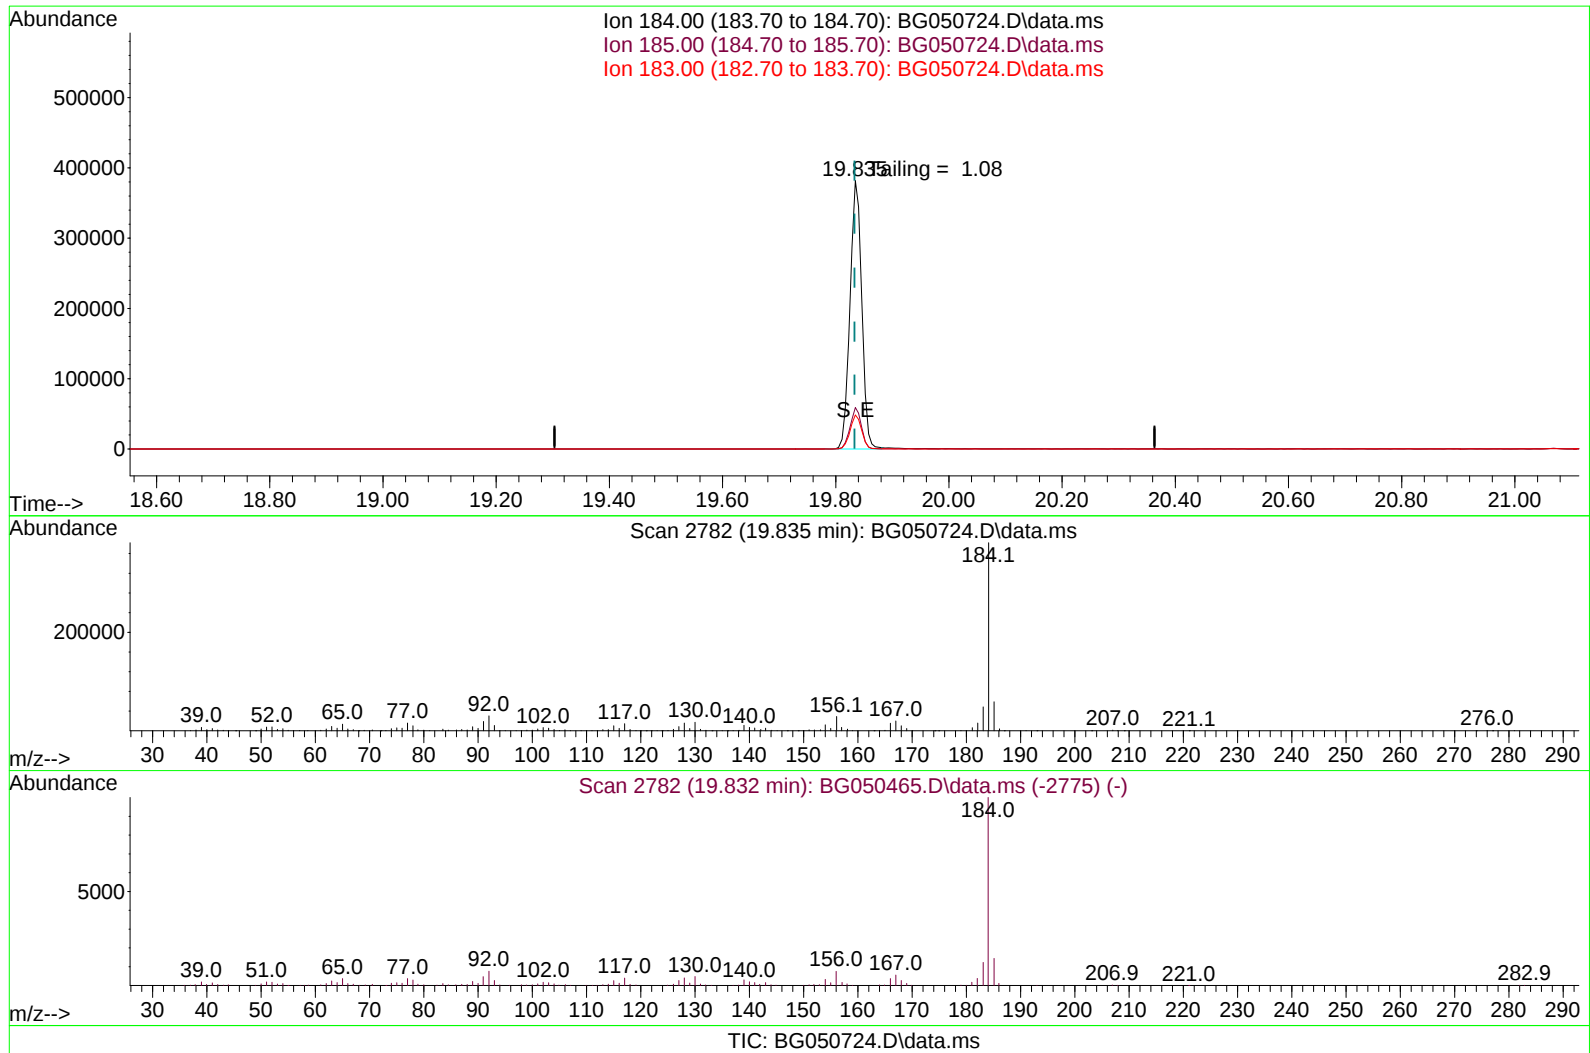**(77) Benzidine****19.835min (+ 0.002) 317348.22 ng****response 555424**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.47
183.00	11.70	12.69
0.00	0.00	0.00