
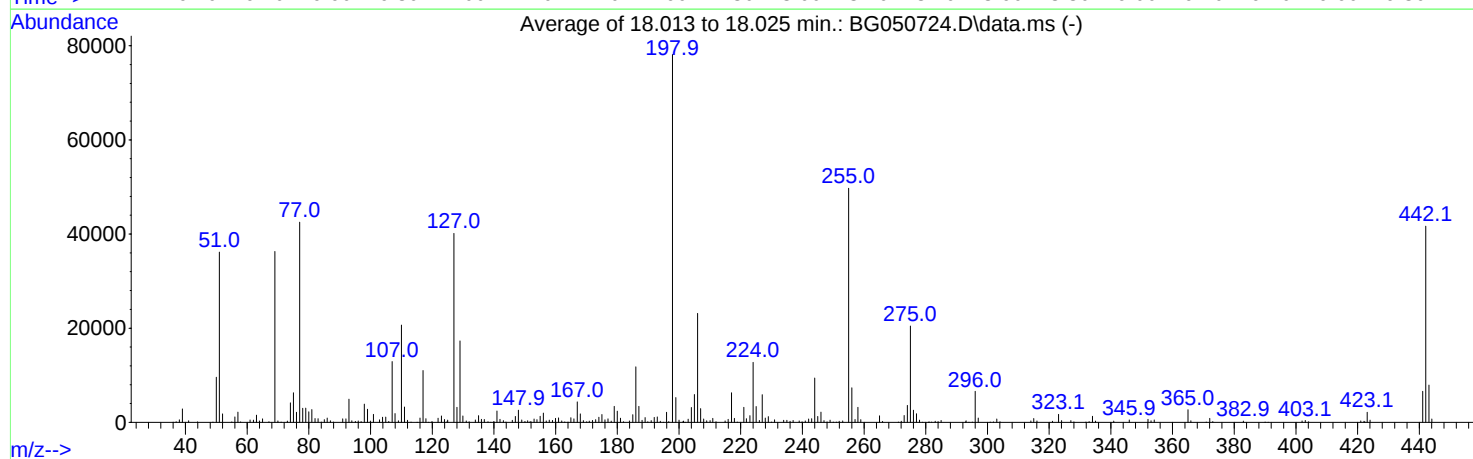


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102621\
 Data File : BG050724.D
 Acq On : 26 Oct 2021 8:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 14 10:56:22 2021

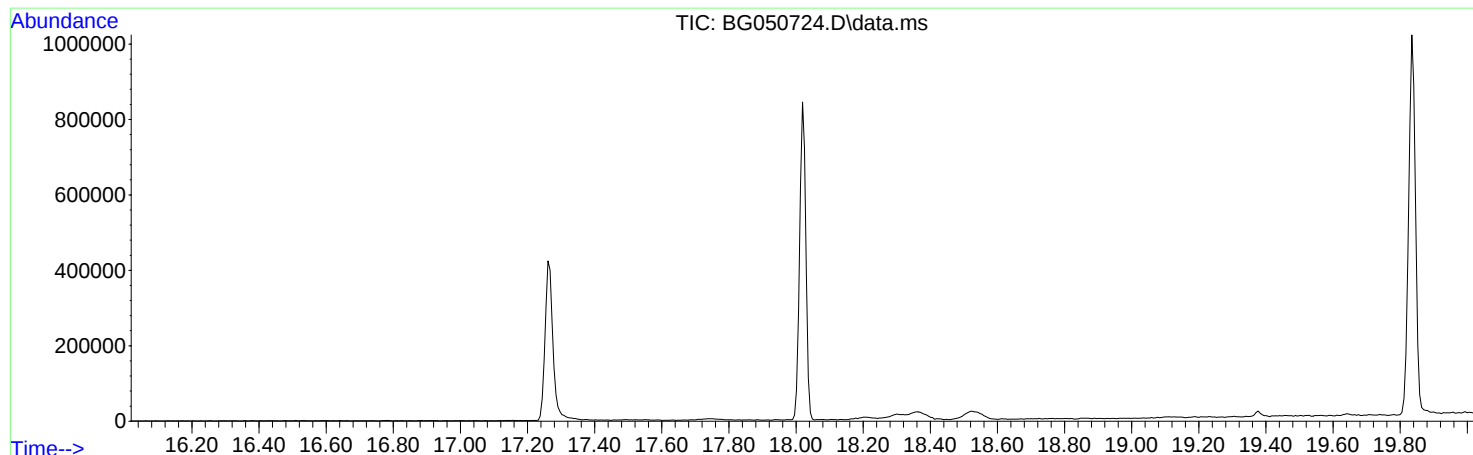




AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	36179	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.5	36304	PASS
70	69	0.00	2	0.8	298	PASS
127	198	10	80	51.4	40155	PASS
197	198	0.00	2	0.2	173	PASS
198	198	100	100	100.0	78139	PASS
199	198	5	9	6.8	5282	PASS
275	198	10	60	26.2	20454	PASS
365	198	1	100	3.5	2698	PASS
441	198	0.01	100	8.4	6596	PASS
442	442	50	100	100.0	41659	PASS
443	442	15	24	19.0	7930	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102621\
Data File : BG050724.D
Acq On : 26 Oct 2021 8:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 26 09:30:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

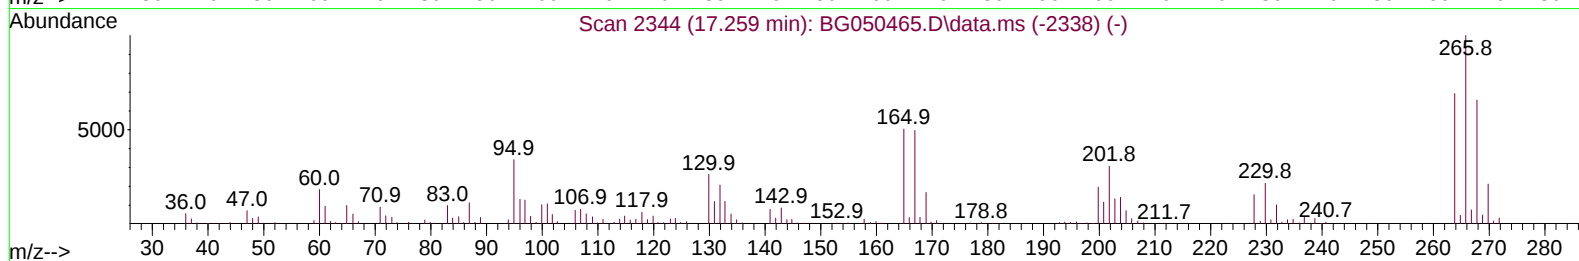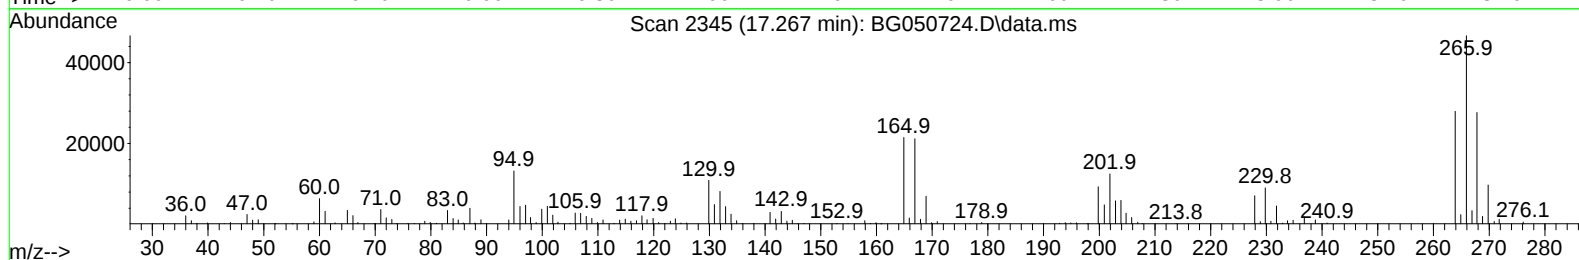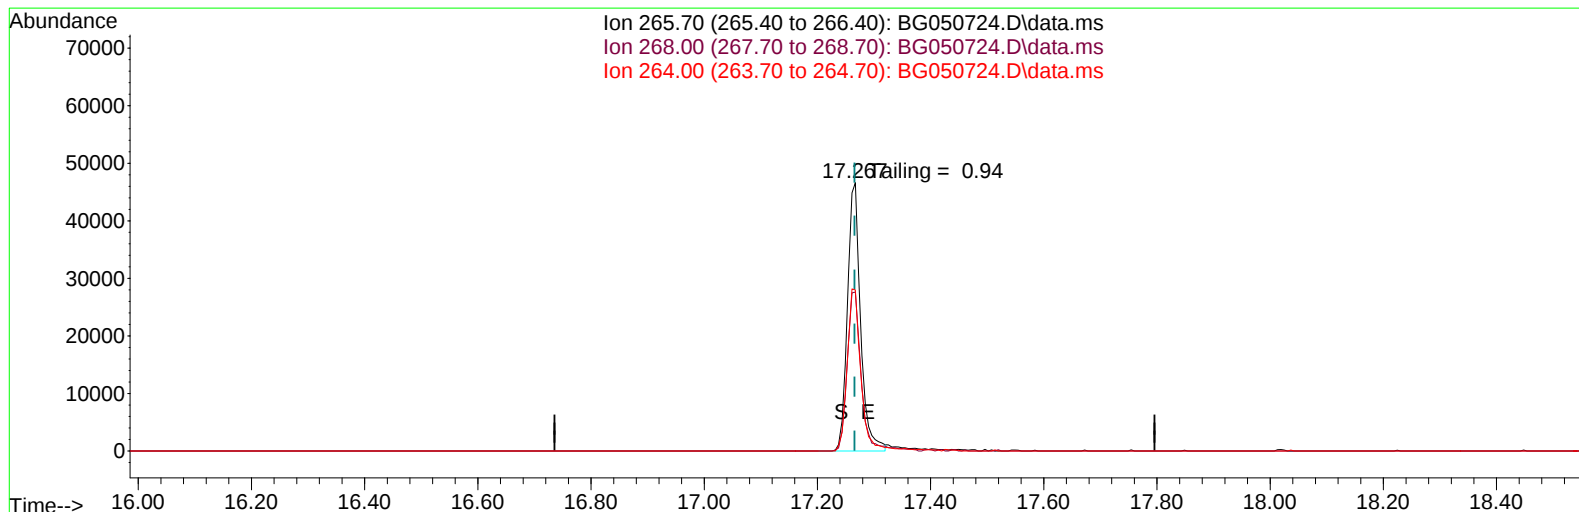

TIC: BG050724.D\data.ms

(70) Pentachlorophenol (C)

17.267min (+ 0.002) 18614.40 ng




response 77415

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	59.25
264.00	61.30	60.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102621\
Data File : BG050724.D
Acq On : 26 Oct 2021 8:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 26 09:30:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 14 10:56:22 2021
Response via : Initial Calibration

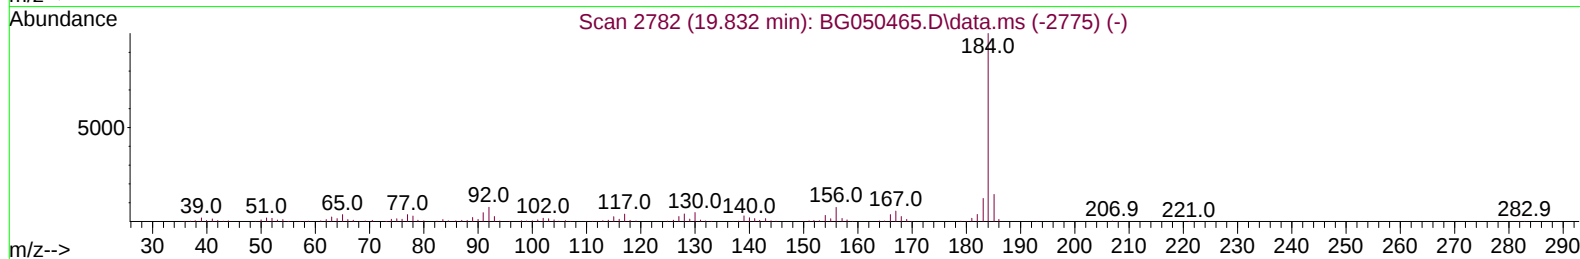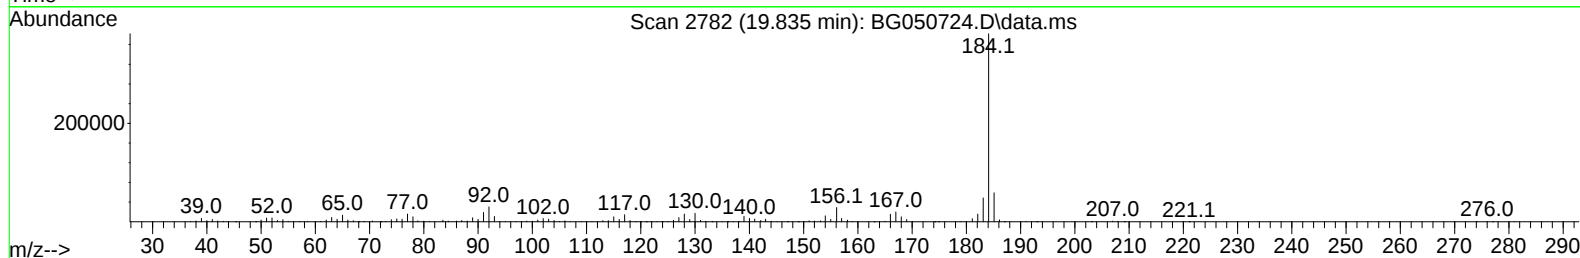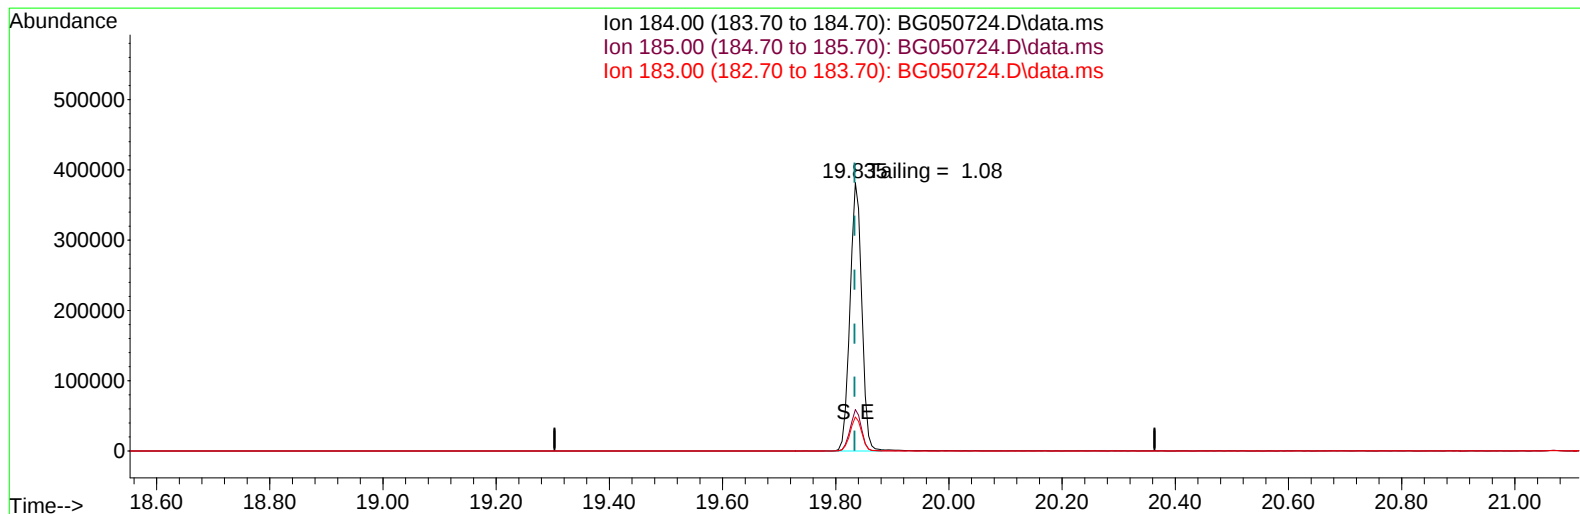

TIC: BG050724.D\data.ms

(77) Benzidine

19.835min (+ 0.002) 317348.22 ng

response 555424

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.47
183.00	11.70	12.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/26/2021	BNA_G	BG050724.D
Compound Name	Response	Retention Time
DDT	243423	21.06
DDD	2220	20.61
DDE	197	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2417	245840	0.98

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP