
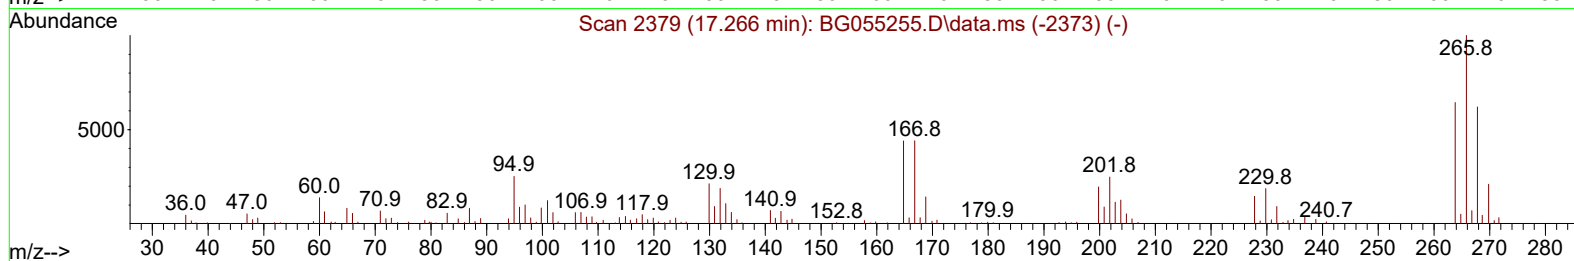
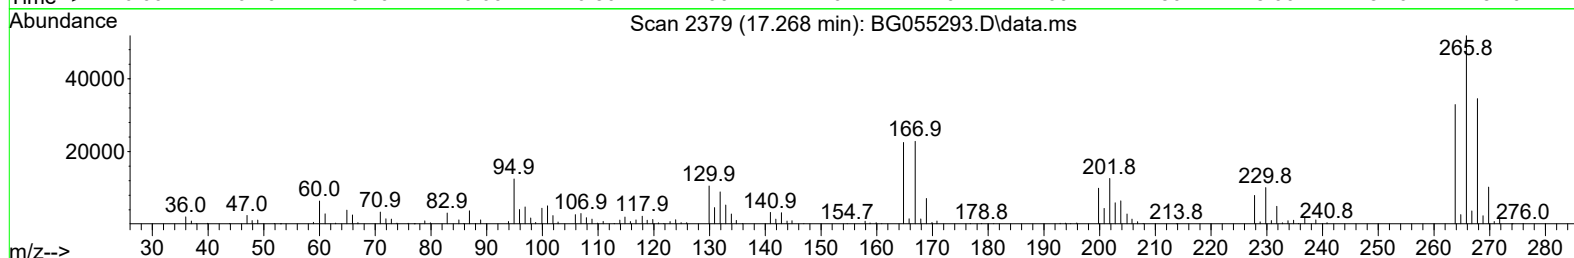


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
 Data File : BG055293.D
 Acq On : 26 Oct 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 09:30:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 24 16:54:05 2022
 Response via : Initial Calibration

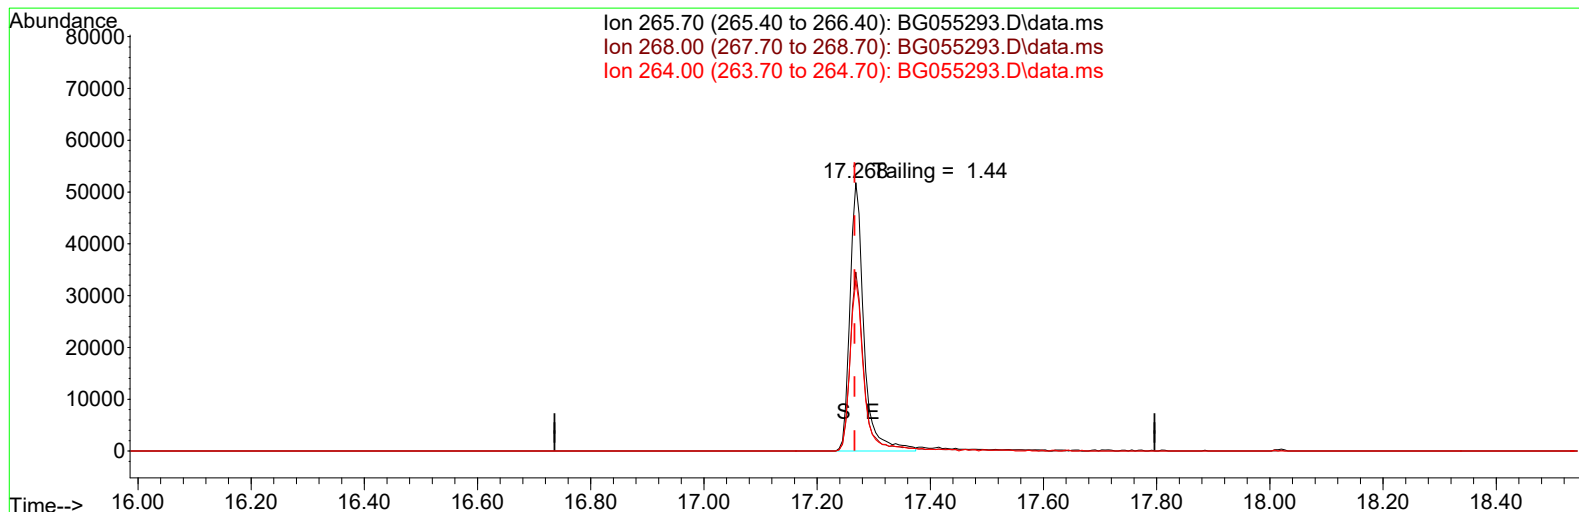

TIC: BG055293.D\data.ms

(70) Pentachlorophenol (C)




17.268min (+ 0.002) 33652.41 ng

response 89292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.50	66.67
264.00	64.40	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG102622\
 Data File : BG055293.D
 Acq On : 26 Oct 2022 10:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 28 09:30:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG102422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 24 16:54:05 2022
 Response via : Initial Calibration

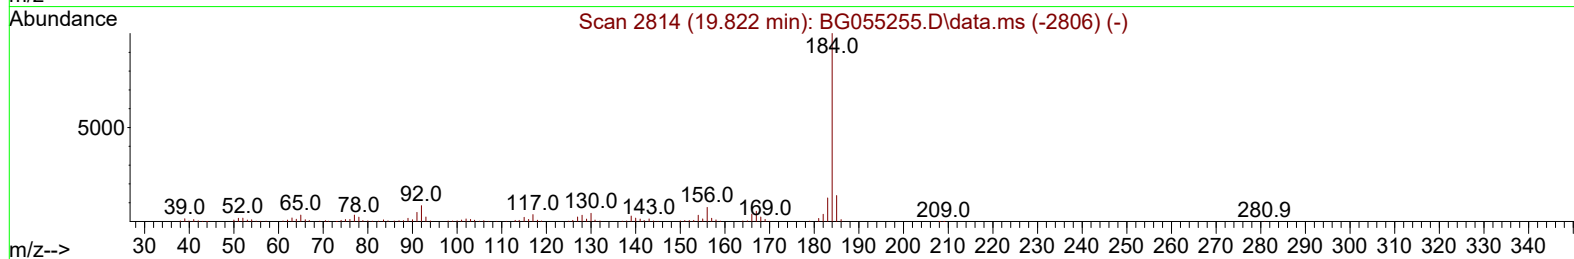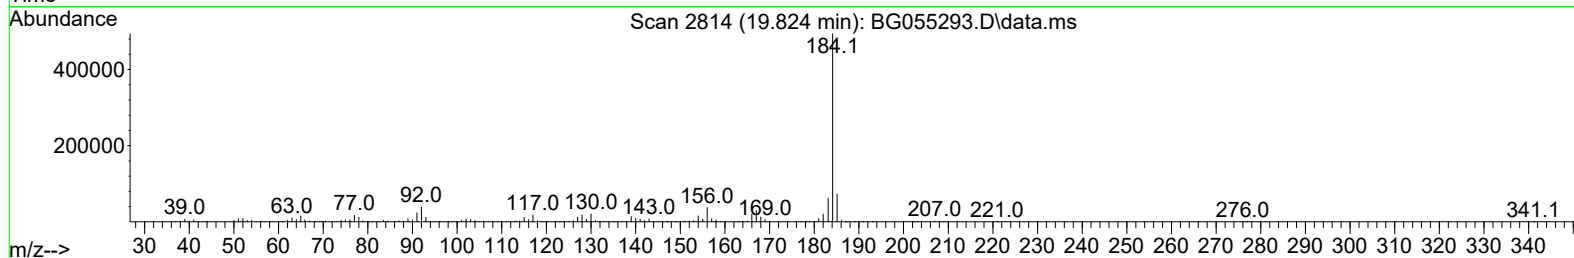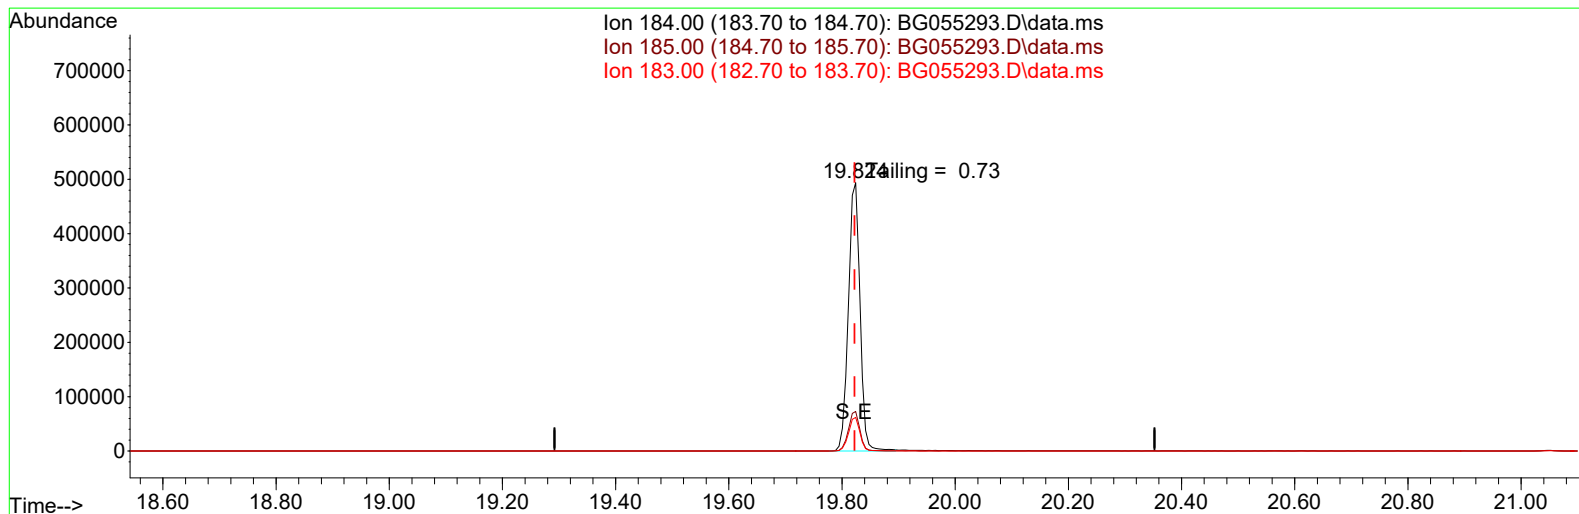

TIC: BG055293.D\data.ms

(77) Benzidine**19.824min (+ 0.002) 34136.01 ng****response 708336**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.71
183.00	12.50	12.55
0.00	0.00	0.00